
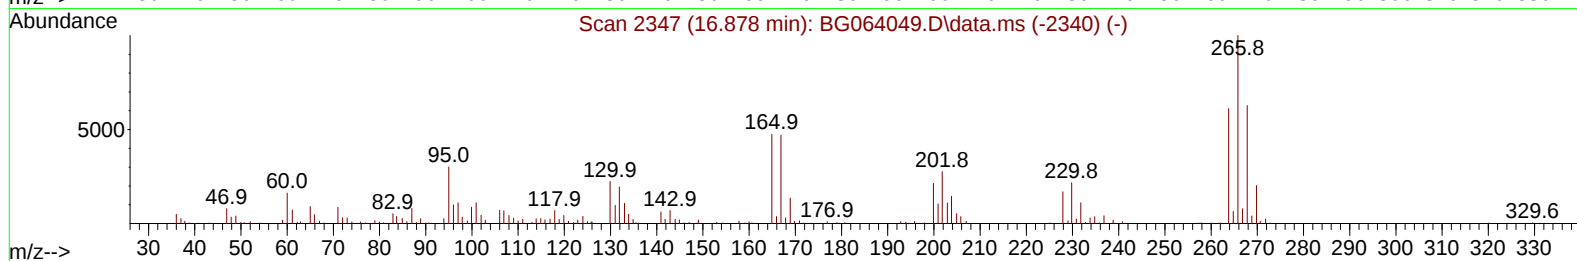
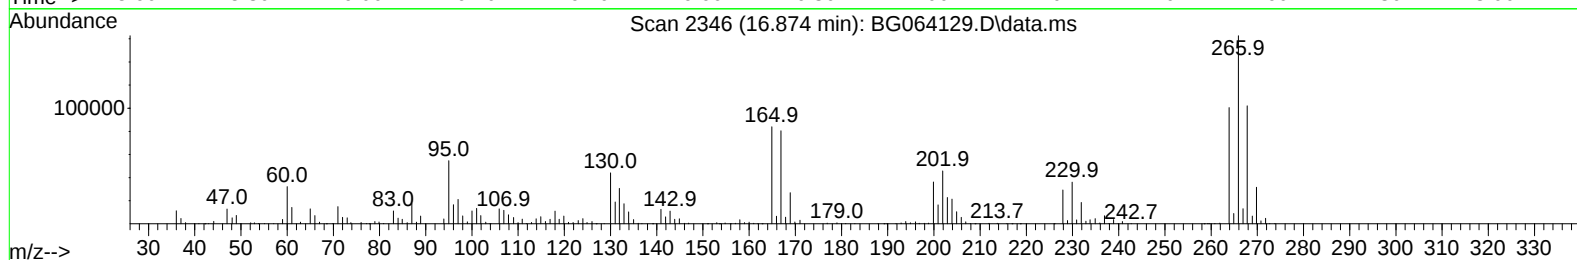


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040125\
Data File : BG064129.D
Acq On : 1 Apr 2025 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 12:38:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

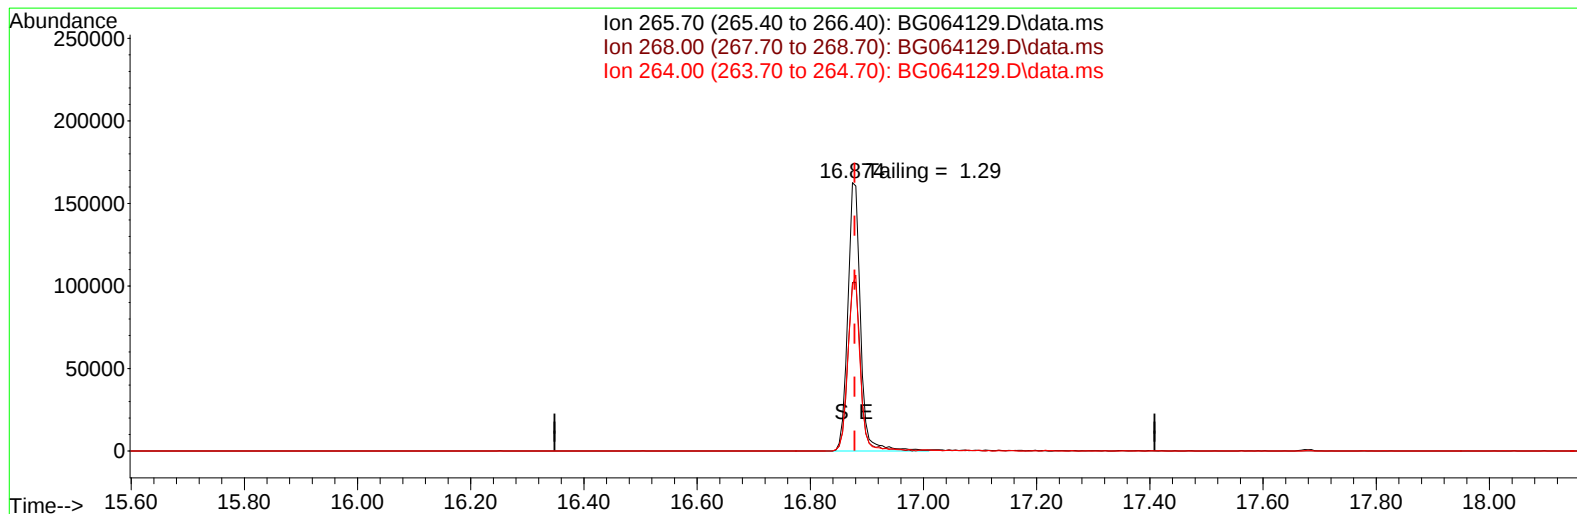

TIC: BG064129.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.004) 18192.74 ng

response 250619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.76
264.00	61.10	61.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040125\
Data File : BG064129.D
Acq On : 1 Apr 2025 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 12:38:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

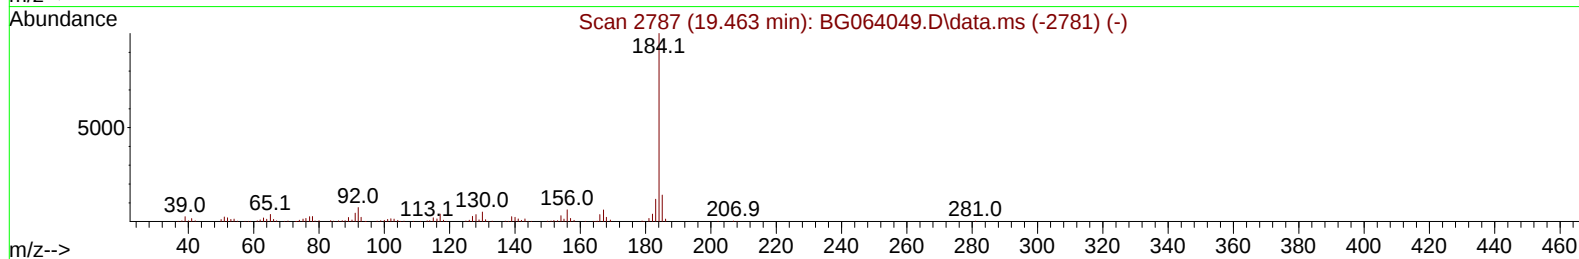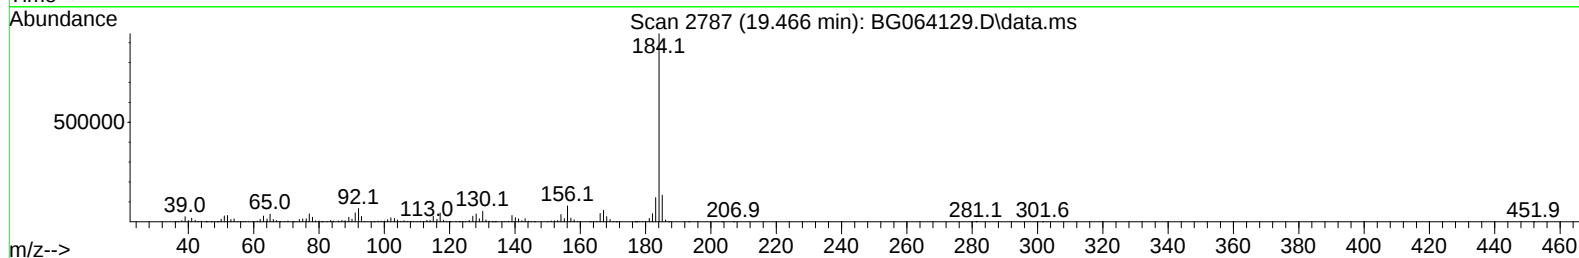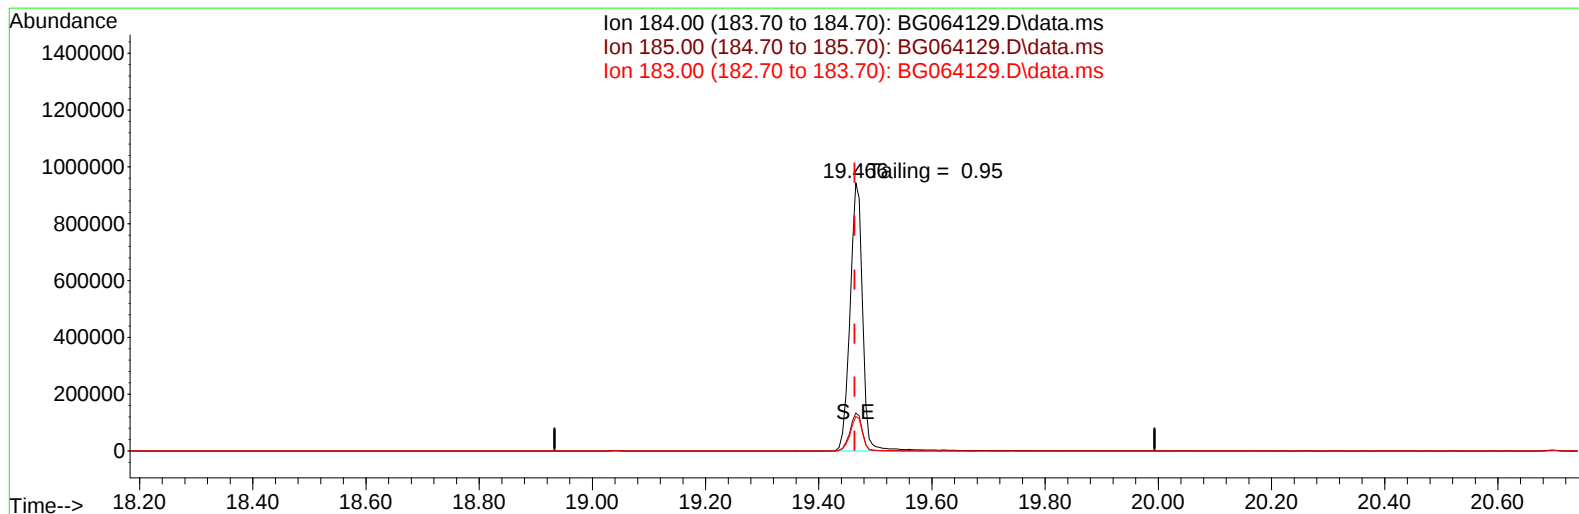

TIC: BG064129.D\data.ms

(77) Benzidine**19.466min (+ 0.003) 44246.31 ng****response 1453902**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.18
183.00	11.90	12.89
0.00	0.00	0.00