


Data Path : Z:\HPCHEM1\BNA_G\Data\BG040215\
Data File : BG016216.D
Acq On : 2 Apr 2015 8:52
Operator : TP/IZ
Sample : DFTPP17
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP17

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG033115.M
Title : SVOA CALIBRATION
Last Update : Wed Apr 01 04:39:57 2015

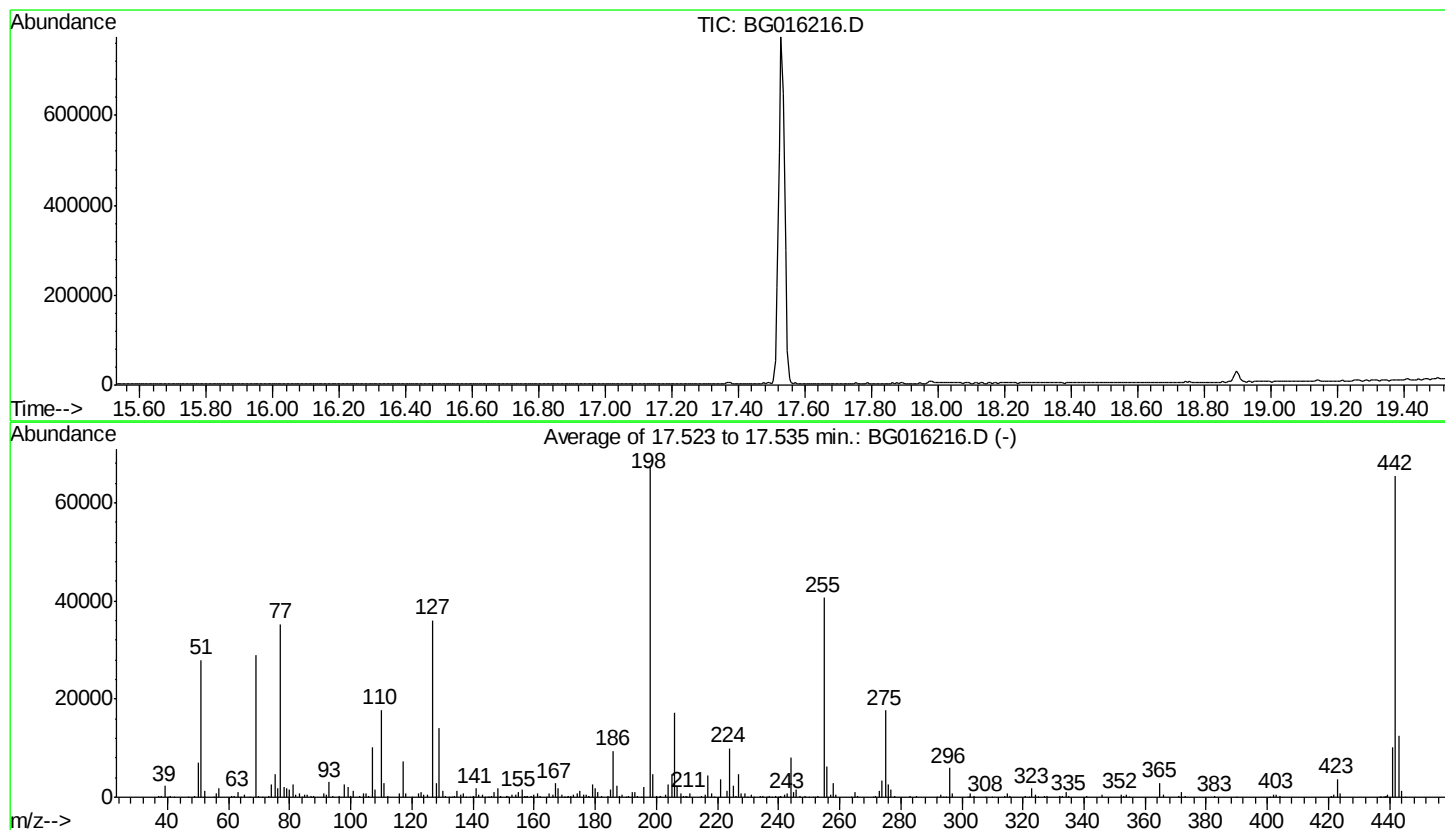

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	27950	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.7	28880	PASS
70	69	0.00	2	0.8	224	PASS
127	198	10	80	53.3	36010	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67568	PASS
199	198	5	9	6.8	4612	PASS
275	198	10	60	26.2	17713	PASS
365	198	1	100	4.4	2985	PASS
441	443	0.01	100	82.2	10239	PASS
442	198	50	100	97.0	65538	PASS
443	442	15	24	19.0	12450	PASS