
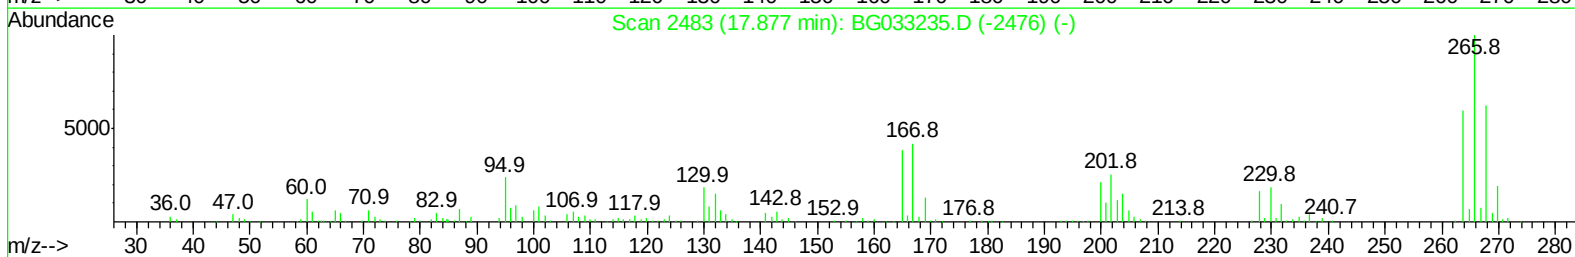
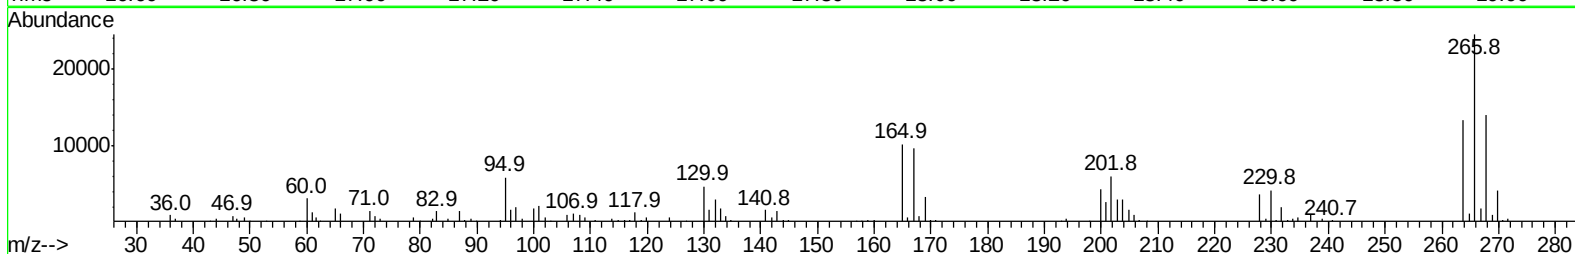


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG040218\
Data File : BG033478.D
Acq On : 2 Apr 2018 9:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 05:49:02 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

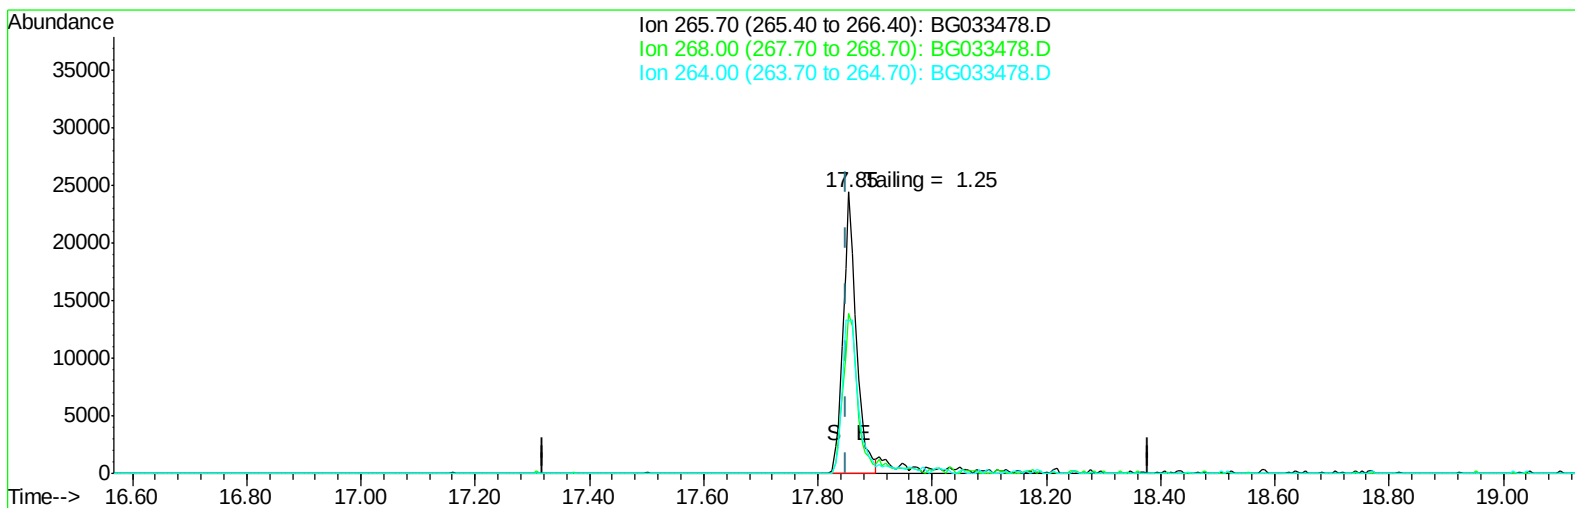

TIC: BG033478.D

(69) Pentachlorophenol (C)




17.854min (+0.004) 19202.29ng

response 39531

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.03
264.00	62.00	54.15
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG040218\
Data File : BG033478.D
Acq On : 2 Apr 2018 9:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 05:49:02 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

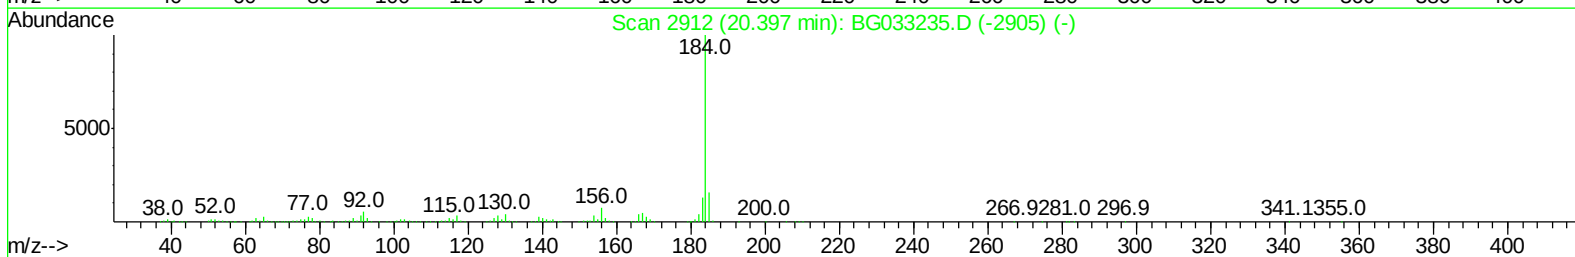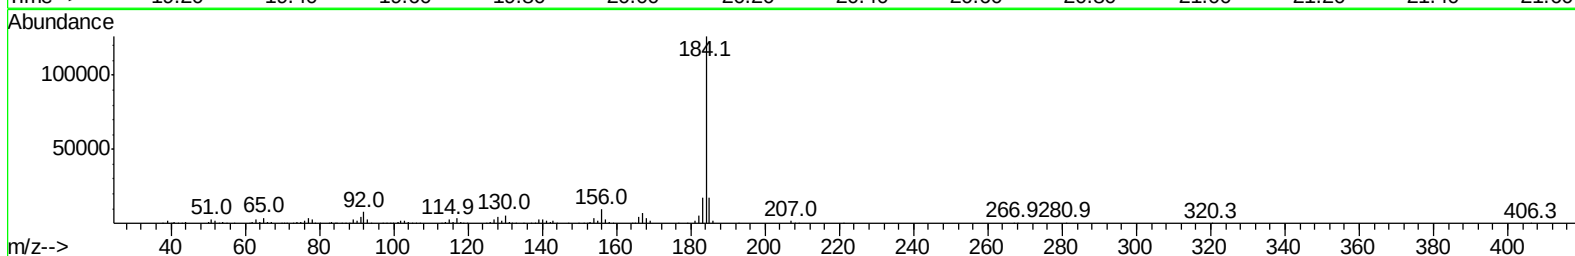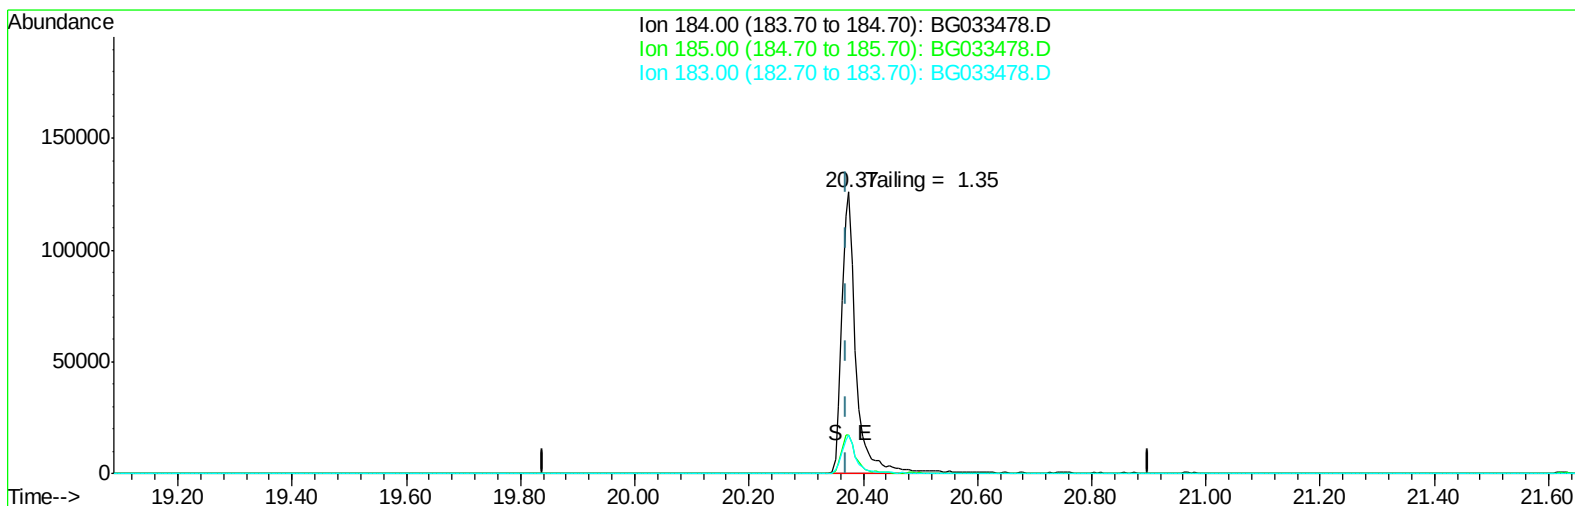

TIC: BG033478.D

(76) Benzidine

20.375min (+0.004) 125319.67ng

response 217503

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.68
183.00	13.30	13.55
0.00	0.00	0.00