

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG040218\
 Data File : BG033504.D
 Acq On : 3 Apr 2018 1:39
 Operator : SJ/JU
 Sample : J2114-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 032718-SIDI-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.481	27	33	43	rBV	140585	274067	6.69%	1.819%
2	3.569	43	48	56	rVB	84736	131112	3.20%	0.870%
3	6.295	506	512	526	rBV2	138660	316522	7.73%	2.100%
4	7.982	793	799	821	rBV2	87406	267698	6.54%	1.776%
5	8.375	860	866	887	rBV	303253	683689	16.69%	4.537%
6	8.863	942	949	960	rBV	80901	196378	4.79%	1.303%
7	9.198	997	1006	1022	rBV	478119	994448	24.28%	6.599%
8	10.062	1146	1153	1175	rBV	392237	901710	22.01%	5.984%
9	11.748	1432	1440	1449	rBV2	137452	300969	7.35%	1.997%
10	14.104	1834	1841	1858	rBV	1341144	2341403	57.16%	15.537%
11	15.479	2068	2075	2089	rBV2	316335	558559	13.64%	3.707%
12	16.954	2319	2326	2340	rBV	796997	1420242	34.67%	9.424%
13	17.095	2346	2350	2359	rVB3	22708	41092	1.00%	0.273%
14	18.211	2534	2540	2552	rBV	439771	787038	19.21%	5.223%
15	20.732	2962	2969	2984	rBV	2859421	4096191	100.00%	27.182%
16	22.553	3271	3279	3294	rBV	453715	922513	22.52%	6.122%
17	26.319	3908	3920	3937	rBV	250256	836056	20.41%	5.548%


Sum of corrected areas: 15069687

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG040218\
Data File : BG033504.D
Acq On : 3 Apr 2018 1:39
Operator : SJ/JU
Sample : J2114-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032718-SIDI-E-U-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

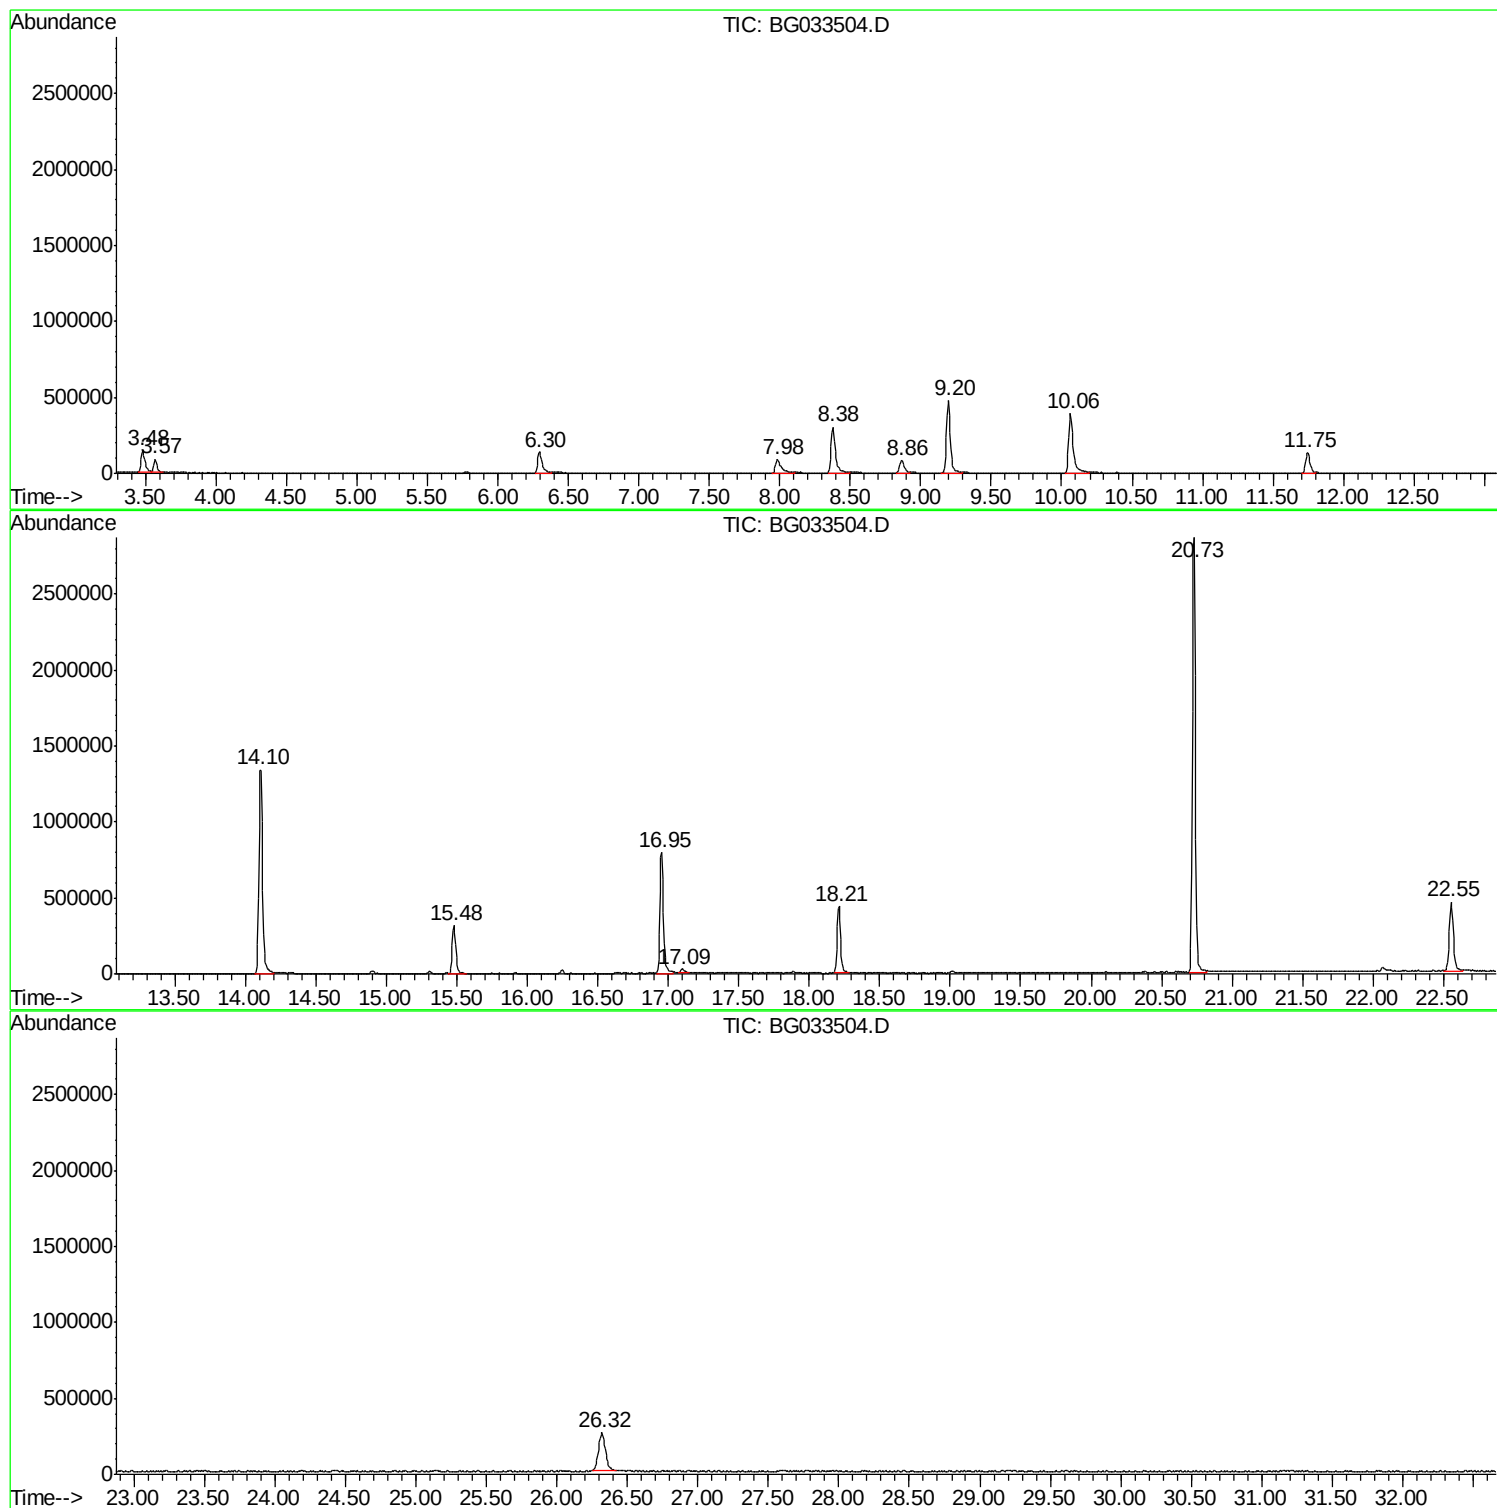

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG040218\
Data File : BG033504.D
Acq On : 3 Apr 2018 1:39
Operator : SJ/JU
Sample : J2114-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032718-SIDI-E-U-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.57	13.35 ng	131112	1,4-Dichlorobenzene-d4	8.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	47
3		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4		1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	38
5		Butanoic acid, 2-hydroxy-2-methyl-	132	C6H12O3	032793-34-3	37

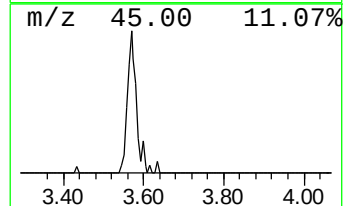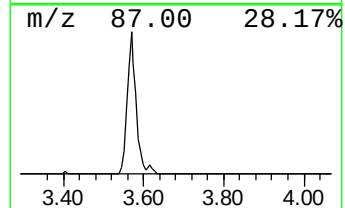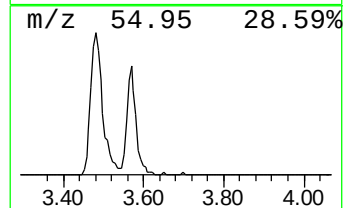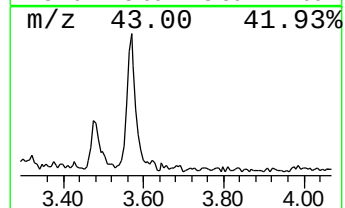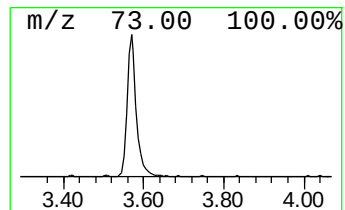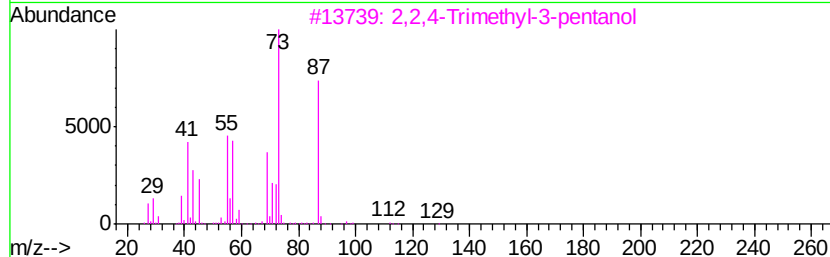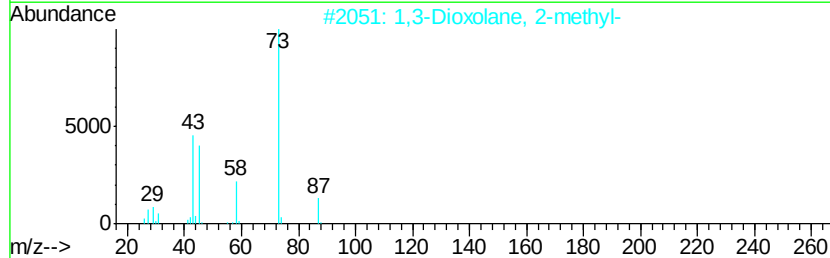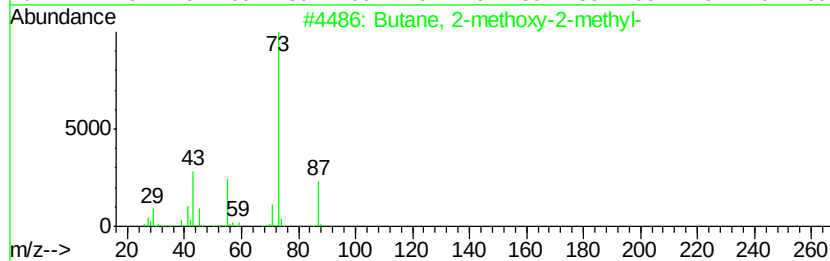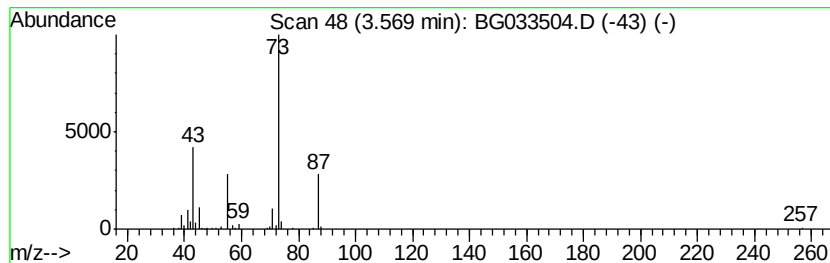

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG040218\
Data File : BG033504.D
Acq On : 3 Apr 2018 1:39
Operator : SJ/JU
Sample : J2114-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032718-SIDI-E-U-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown8.38 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.38	69.63 ng	683689	1,4-Dichlorobenzene-d4	8.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		Tranlylcypromine-propionyl	189	C12H15NO	1000123-86-3	10

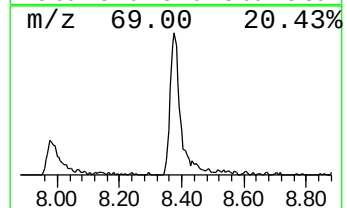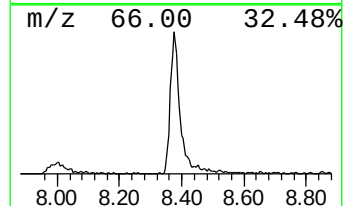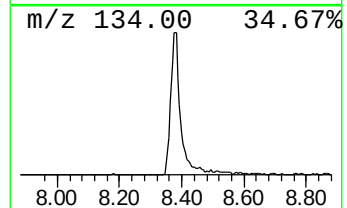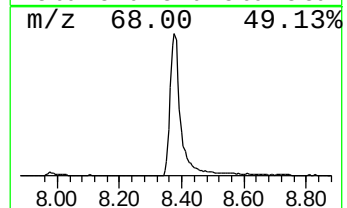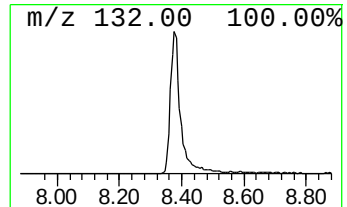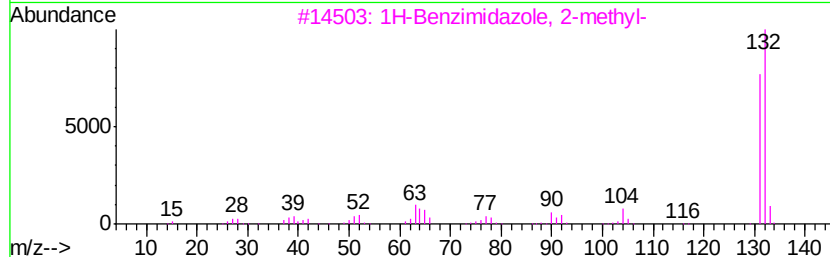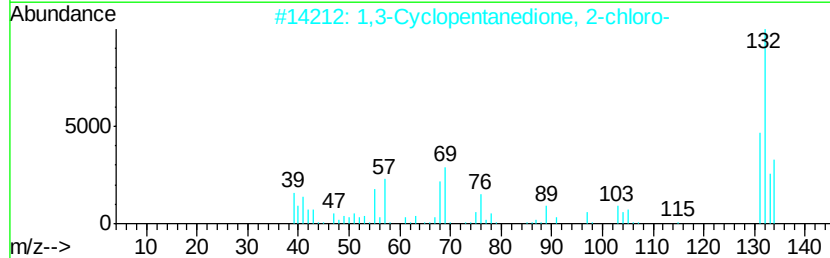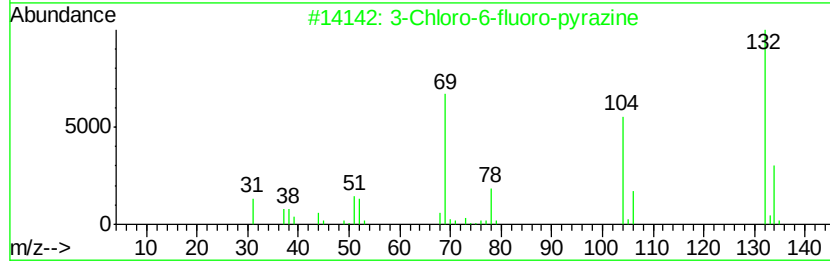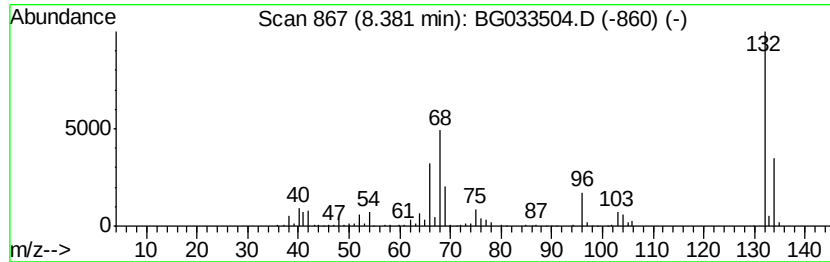

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG040218\
Data File : BG033504.D
Acq On : 3 Apr 2018 1:39
Operator : SJ/JU
Sample : J2114-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032718-SIDI-E-U-M

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.57	13.4	ng	131112	1	8.86	196378	20.0
unknown8.38	8.38	69.6	ng	683689	1	8.86	196378	20.0