


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG040218\
 Data File : BG033478.D
 Acq On : 2 Apr 2018 9:23
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 28 18:34:58 2018

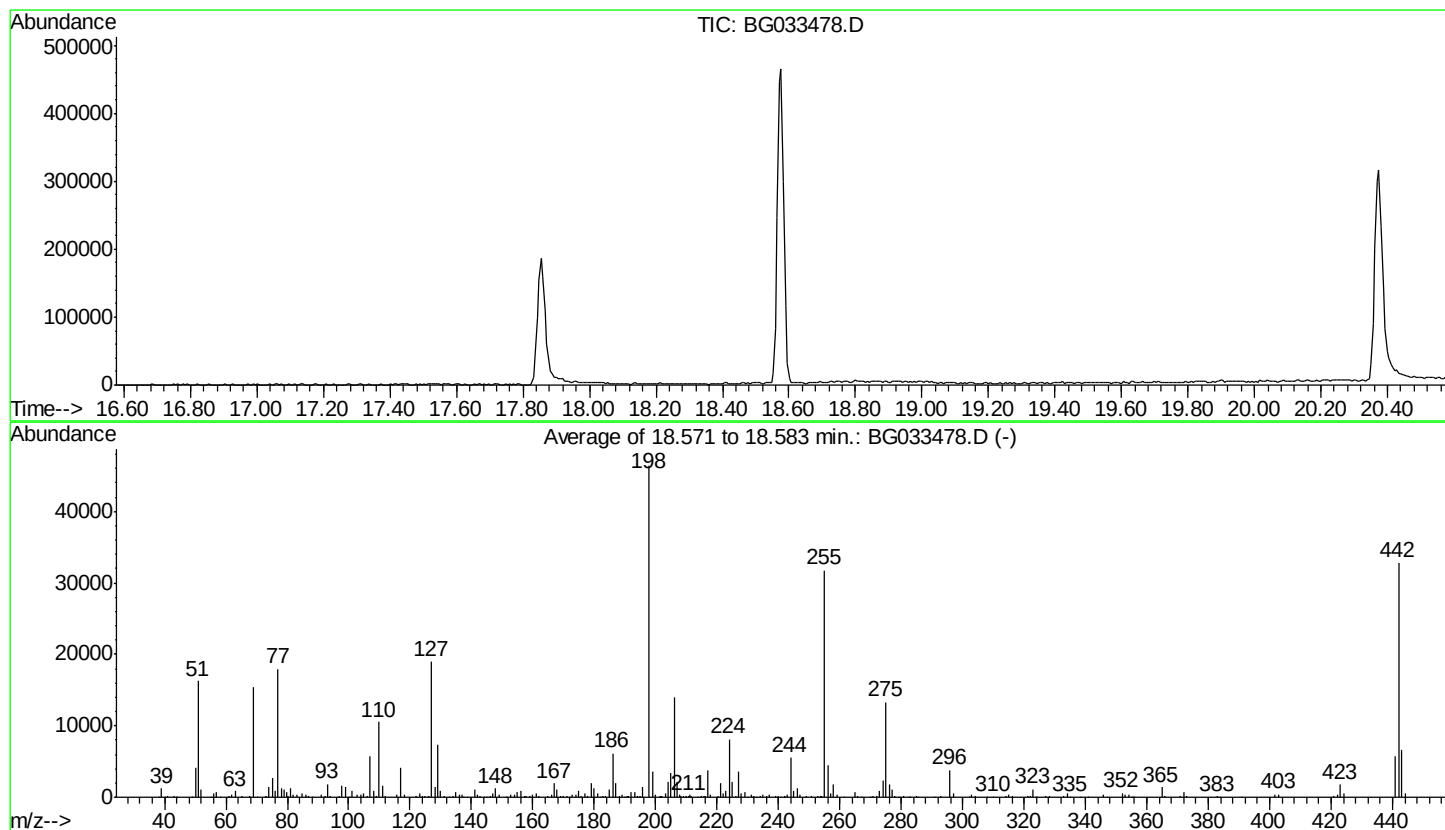

AutoFind: Scans 2601, 2602, 2603; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	16270	PASS
68	69	0.00	2	1.0	157	PASS
69	198	0.00	100	33.4	15490	PASS
70	69	0.00	2	0.4	60	PASS
127	198	10	80	40.8	18927	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46410	PASS
199	198	5	9	7.9	3670	PASS
275	198	10	60	28.7	13310	PASS
365	198	1	100	3.0	1389	PASS
441	443	0.01	100	86.1	5717	PASS
442	198	50	100	70.7	32800	PASS
443	442	15	24	20.2	6641	PASS