
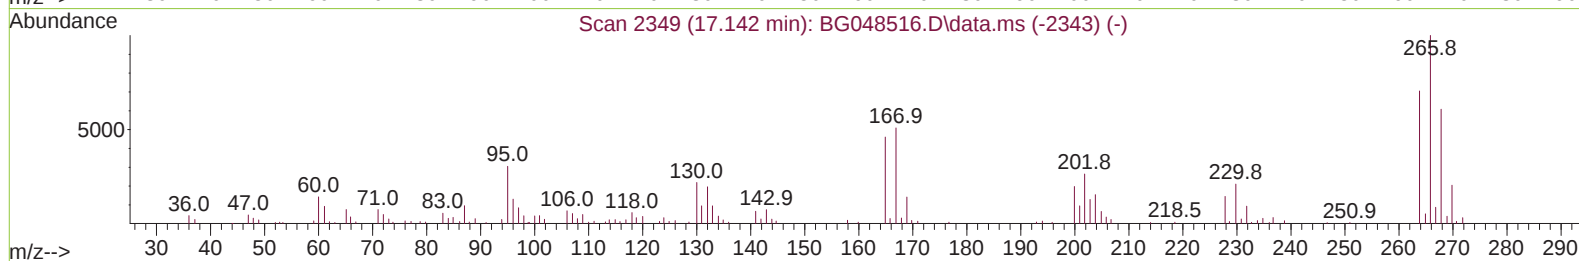
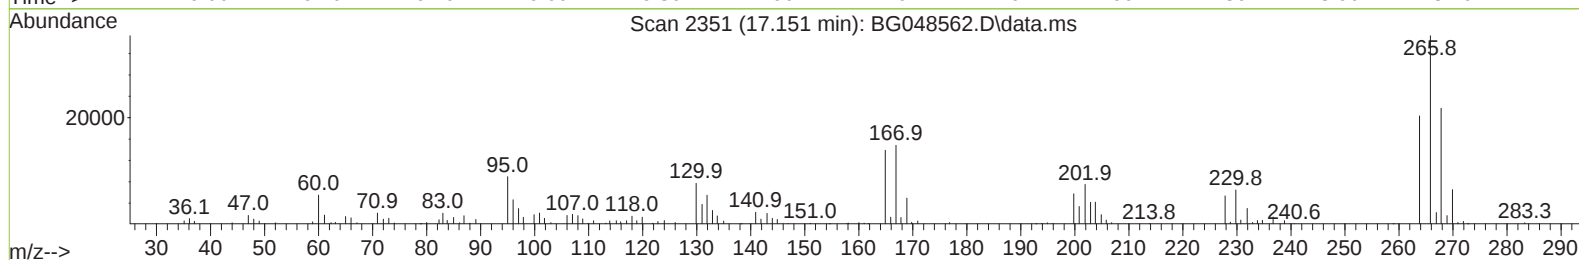


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040221\
Data File : BG048562.D
Acq On : 2 Apr 2021 8:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 09:32:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 11:19:59 2021
Response via : Initial Calibration

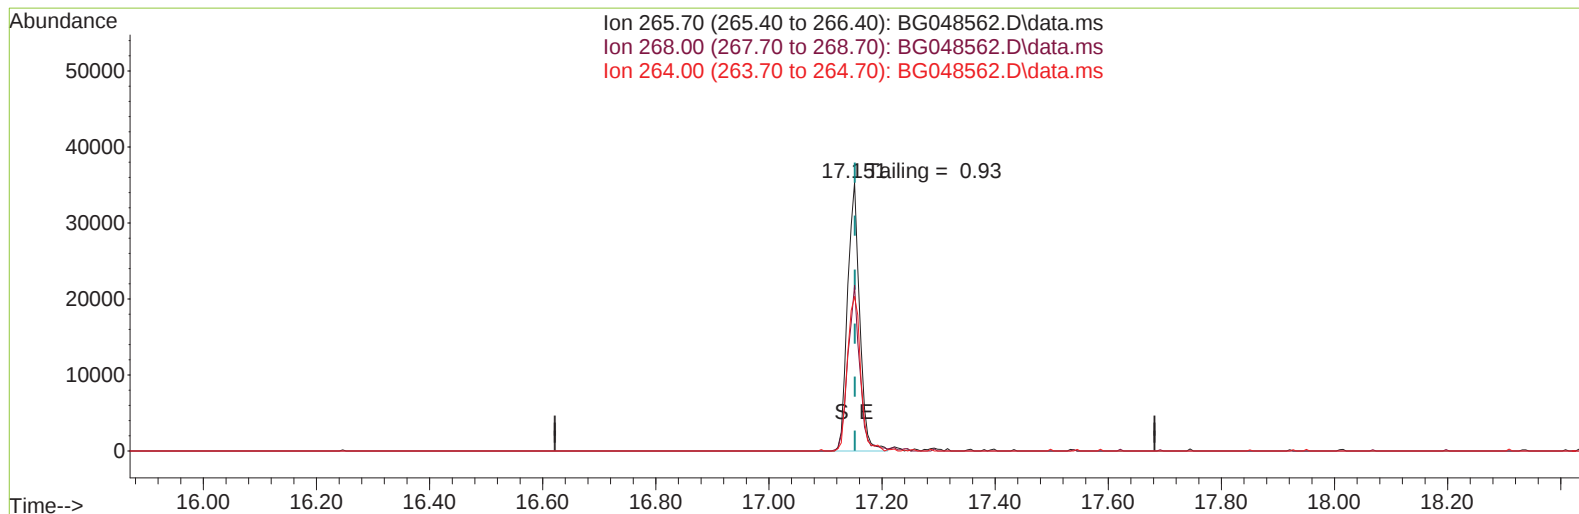

TIC: BG048562.D\data.ms

(70) Pentachlorophenol (C)




17.151min (-0.001) 137971.51 ng

response 52608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	61.65
264.00	70.50	57.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040221\
Data File : BG048562.D
Acq On : 2 Apr 2021 8:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 09:32:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 11:19:59 2021
Response via : Initial Calibration

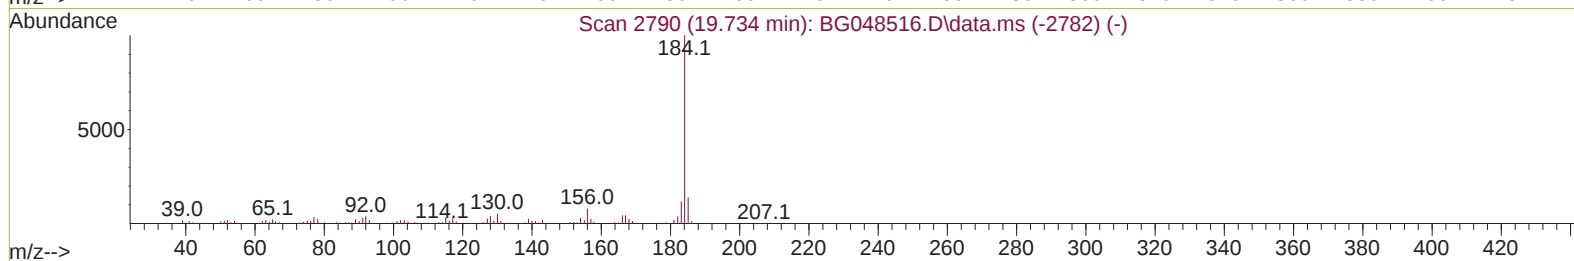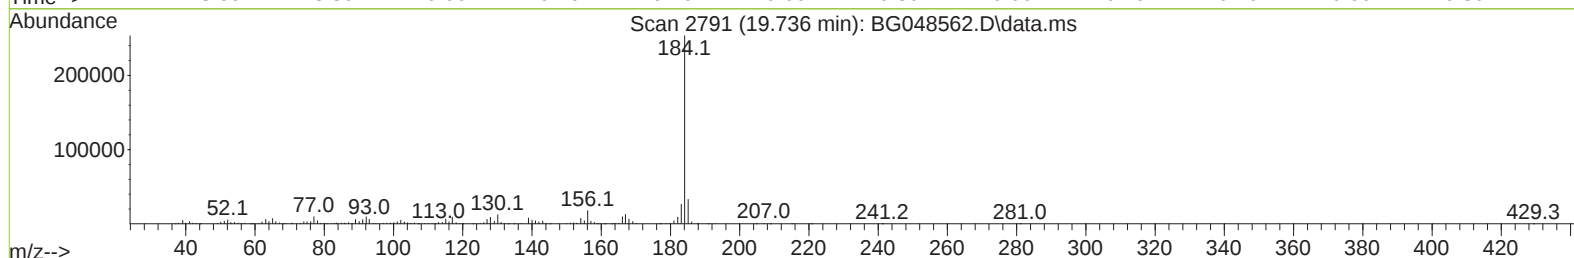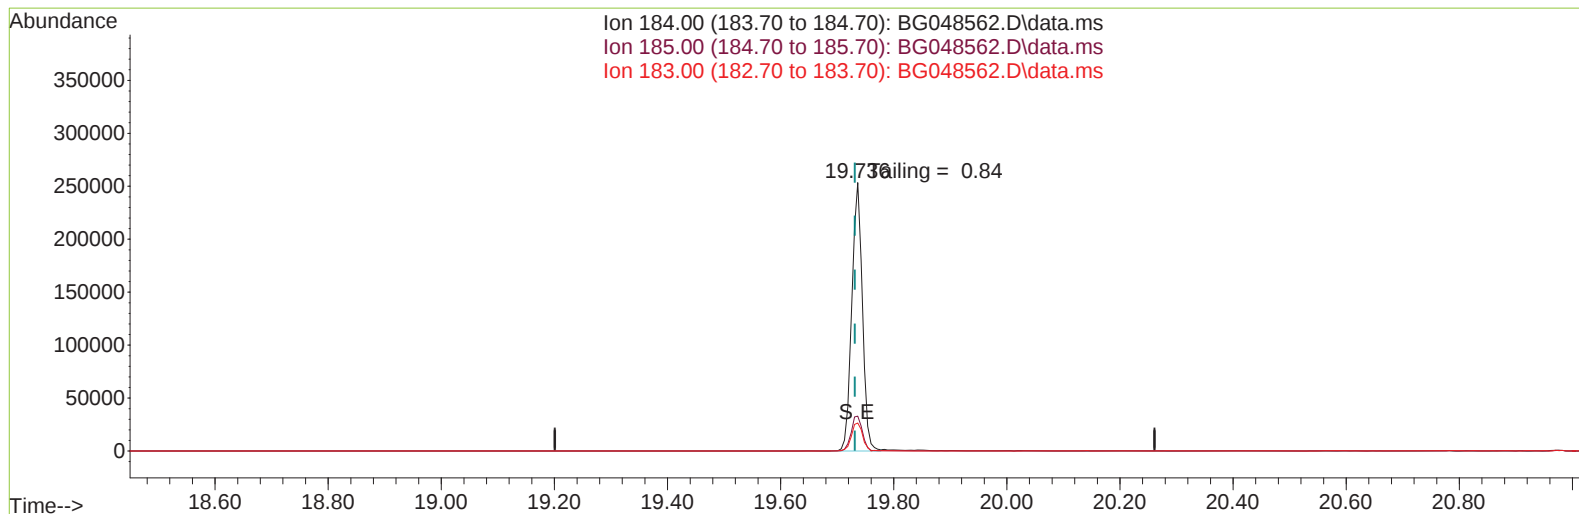

TIC: BG048562.D\data.ms

(77) Benzidine**19.736min (+ 0.005) 89987.22 ng****response 332149**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.00
183.00	11.50	10.43
0.00	0.00	0.00