

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040221\
 Data File : BG048564.D
 Acq On : 2 Apr 2021 11:10
 Operator : CG/JU
 Sample : PB135464BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB135464BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.641	386	392	398	rBV	226278	364539	16.76%	4.780%
2	7.245	658	665	674	rBV	246931	429521	19.75%	5.632%
3	8.103	805	811	819	rVB	85944	135613	6.24%	1.778%
4	8.426	857	866	875	rVB	305200	536317	24.66%	7.033%
5	9.272	1002	1010	1017	rBV	264583	476078	21.89%	6.243%
6	10.929	1285	1292	1302	rVB	104409	187701	8.63%	2.461%
7	13.373	1700	1708	1714	rBV	780958	1199088	55.14%	15.723%
8	14.754	1937	1943	1950	rBV	171192	271692	12.49%	3.563%
9	16.240	2188	2196	2204	rBV	459949	680932	31.31%	8.929%
10	17.504	2405	2411	2419	rBV	237370	362262	16.66%	4.750%
11	20.112	2849	2855	2861	rBV	1671962	2174492	100.00%	28.514%
12	21.799	3136	3142	3150	rBV	223633	387149	17.80%	5.077%
13	25.148	3703	3712	3729	rVB3	132758	420800	19.35%	5.518%




Sum of corrected areas: 7626184

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040221\
Data File : BG048564.D
Acq On : 2 Apr 2021 11:10
Operator : CG/JU
Sample : PB135464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135464BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

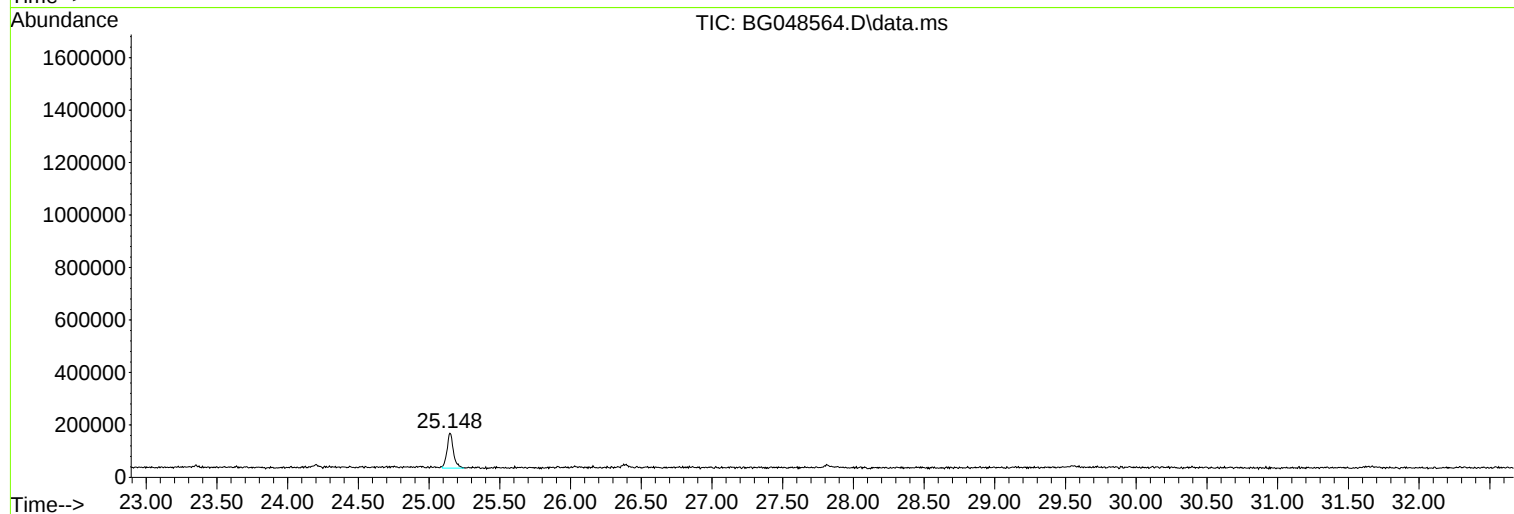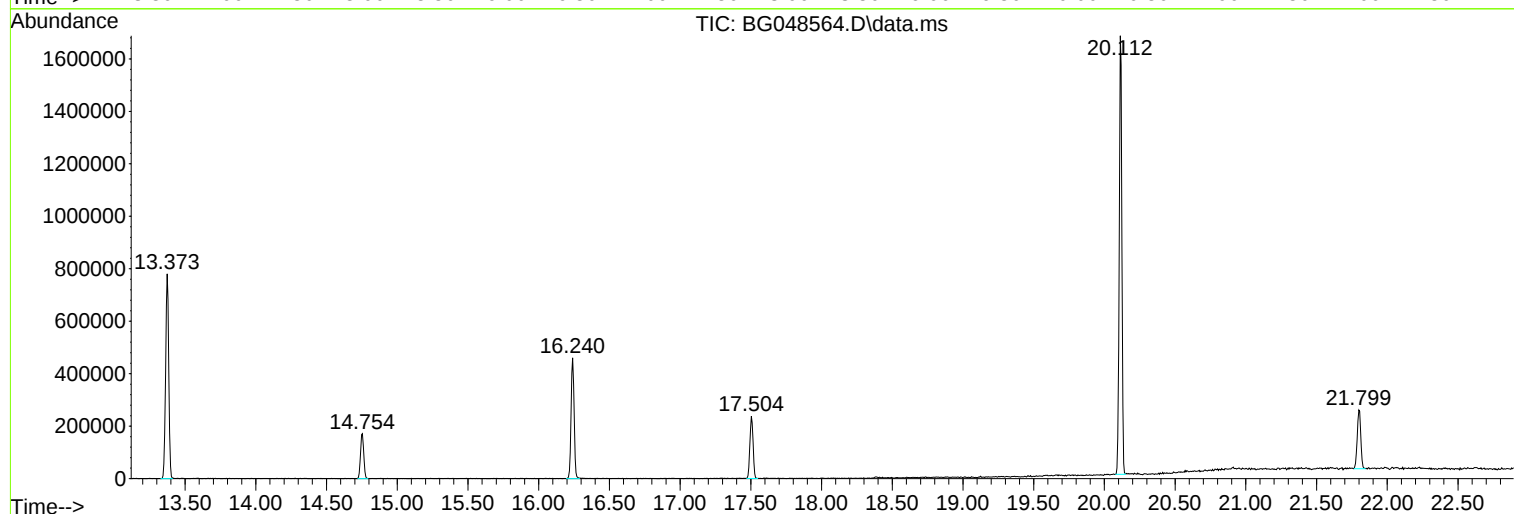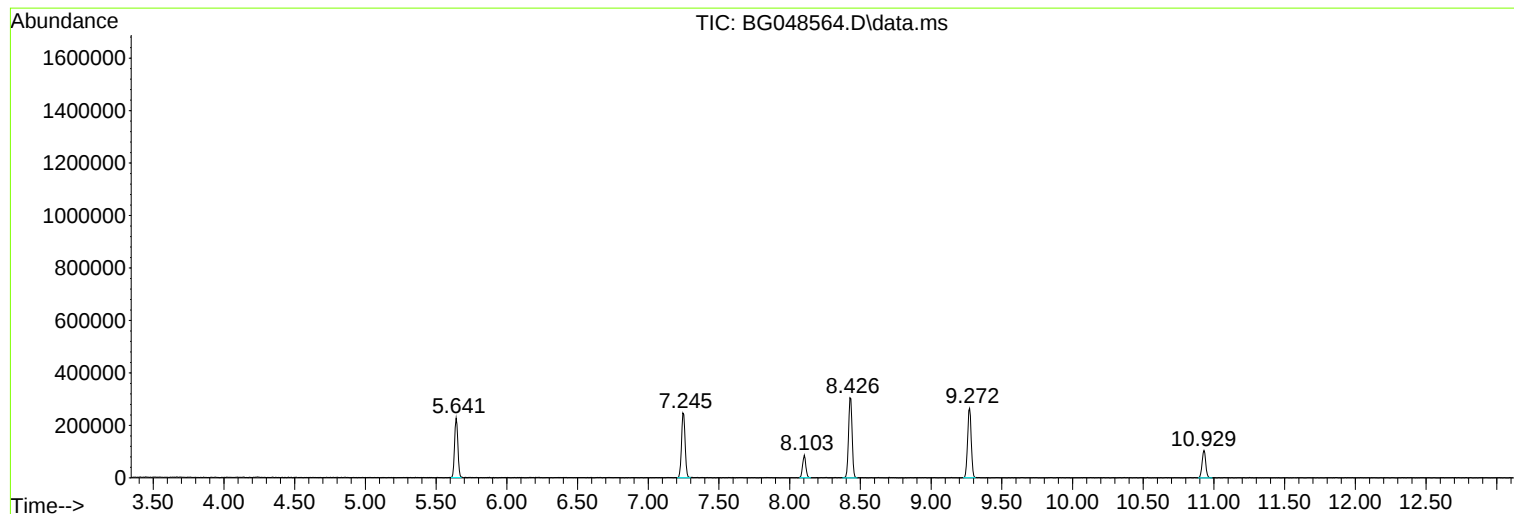

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040221\
Data File : BG048564.D
Acq On : 2 Apr 2021 11:10
Operator : CG/JU
Sample : PB135464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135464BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040221\
Data File : BG048564.D
Acq On : 2 Apr 2021 11:10
Operator : CG/JU
Sample : PB135464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135464BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------