
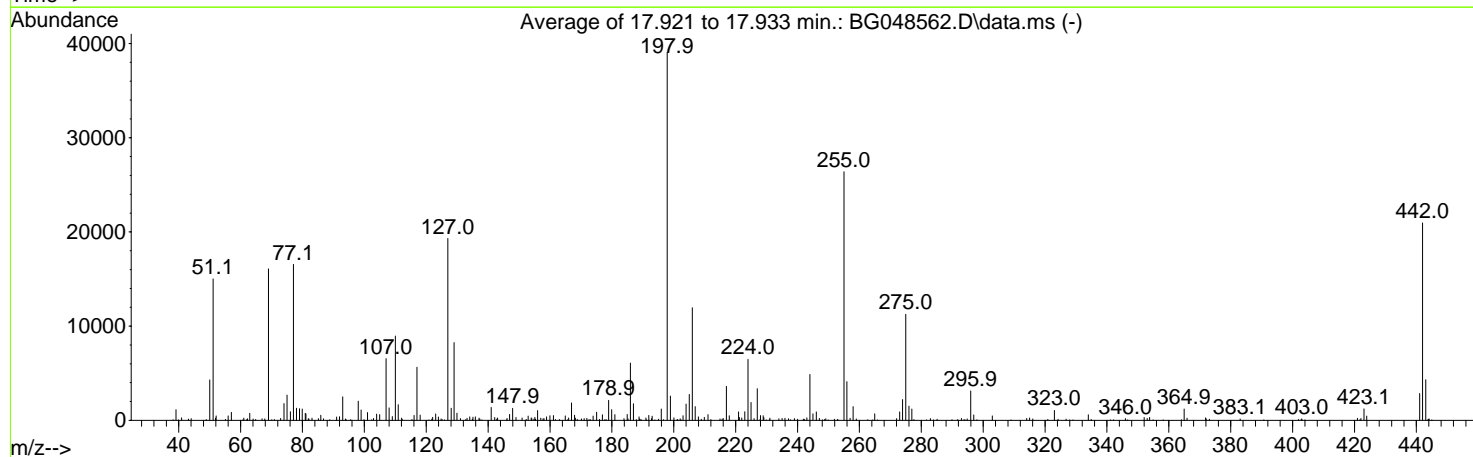


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040221\  
 Data File : BG048562.D  
 Acq On : 2 Apr 2021 8:48  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Apr 02 10:20:56 2021

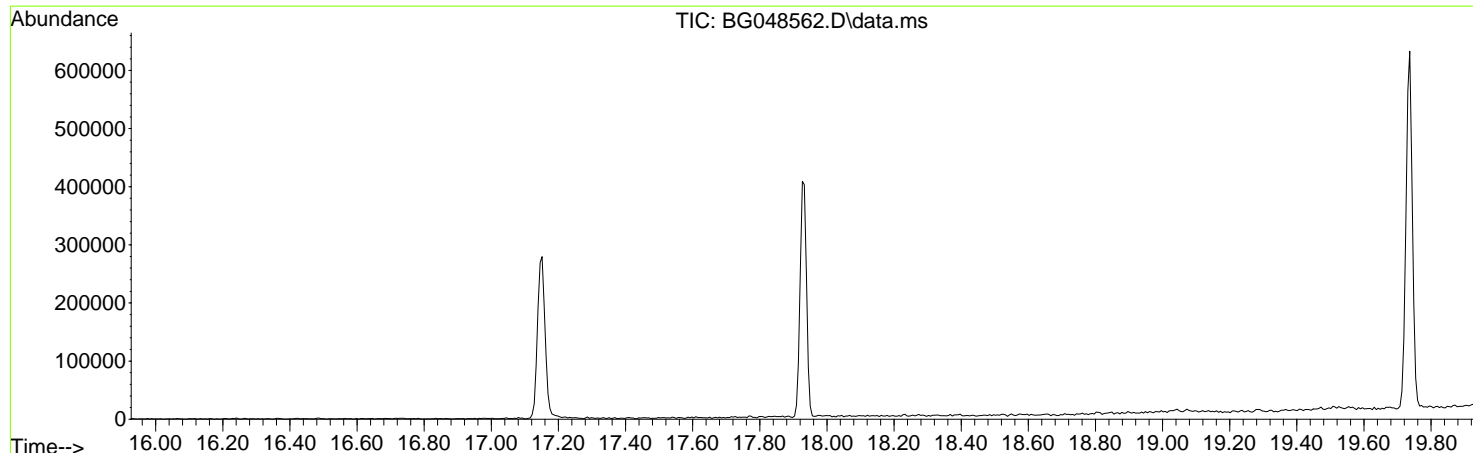

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	15020	PASS
68	69	0.00	2	0.9	146	PASS
69	198	0.00	100	41.2	16077	PASS
70	69	0.00	2	0.5	76	PASS
127	198	10	80	49.4	19302	PASS
197	198	0.00	2	0.2	63	PASS
198	198	100	100	100.0	39045	PASS
199	198	5	9	6.6	2591	PASS
275	198	10	60	28.8	11254	PASS
365	198	1	100	3.1	1209	PASS
441	198	0.01	100	7.3	2860	PASS
442	198	50	100	53.7	20960	PASS
443	442	15	24	20.6	4319	PASS

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/2/2021	BNA_G	<u>BG048562.D</u>
Compound Name	Response	Retention Time
DDT	150634	20.976
DDD	2554	20.518
DDE	250	20.024
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2804	153438	1.83

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040221\  
 Data File : BG048562.D  
 Acq On : 2 Apr 2021 8:48  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampled :**  
 DFTPP

Quant Time: Apr 02 09:32:05 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Apr 01 11:19:59 2021  
 Response via : Initial Calibration

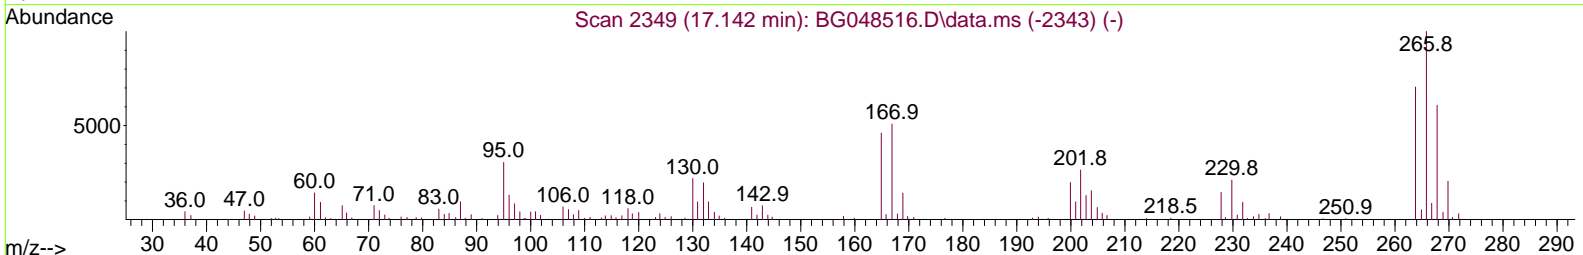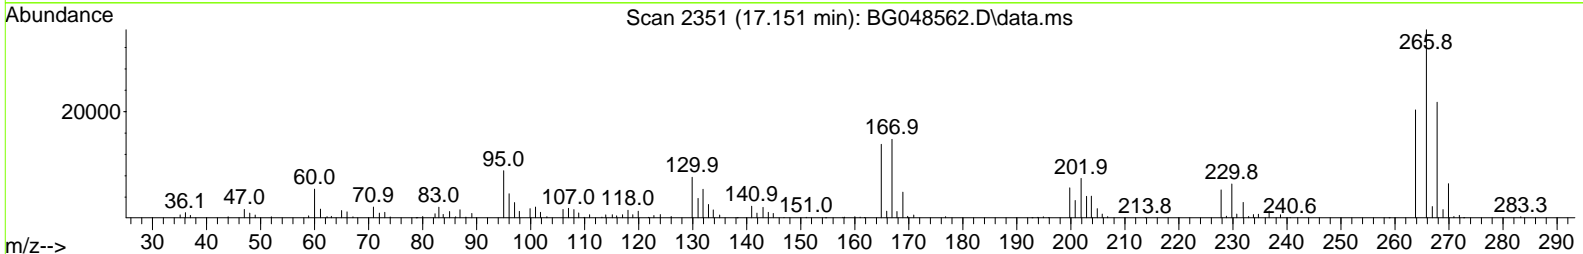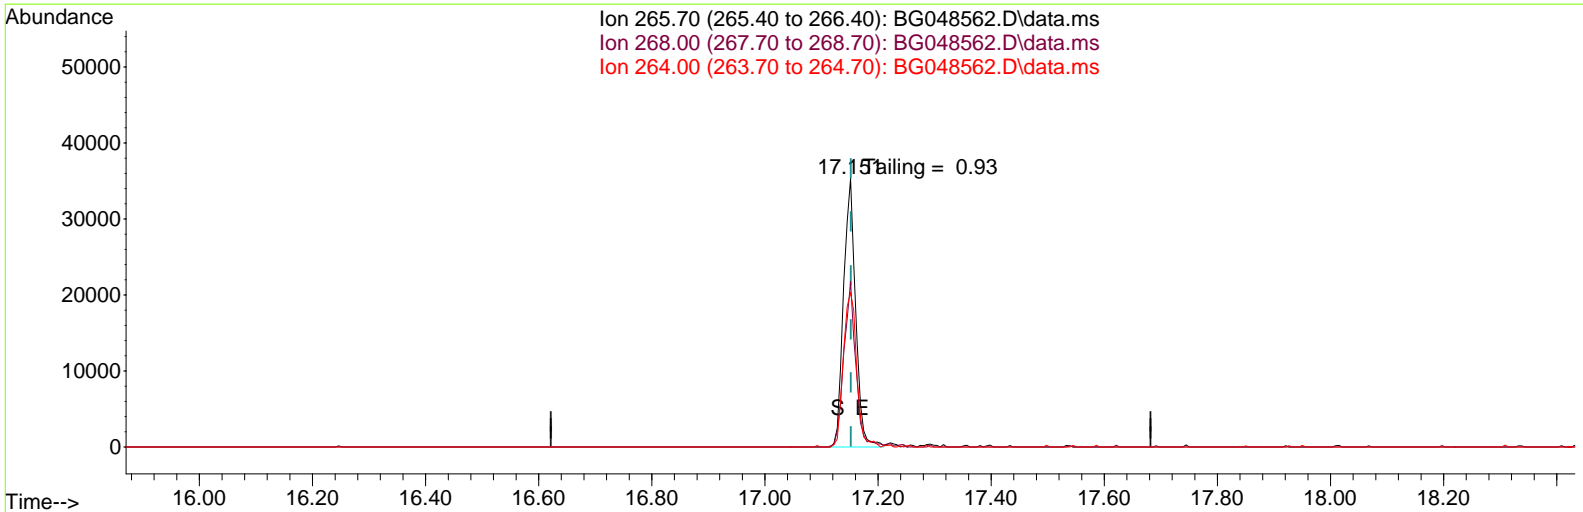

TIC: BG048562.D\data.ms

(70) Pentachlorophenol (C)

17.151min (-0.001) 137971.51 ng




response 52608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	61.65
264.00	70.50	57.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG040221\  
 Data File : BG048562.D  
 Acq On : 2 Apr 2021 8:48  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 02 09:32:05 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Apr 01 11:19:59 2021  
 Response via : Initial Calibration

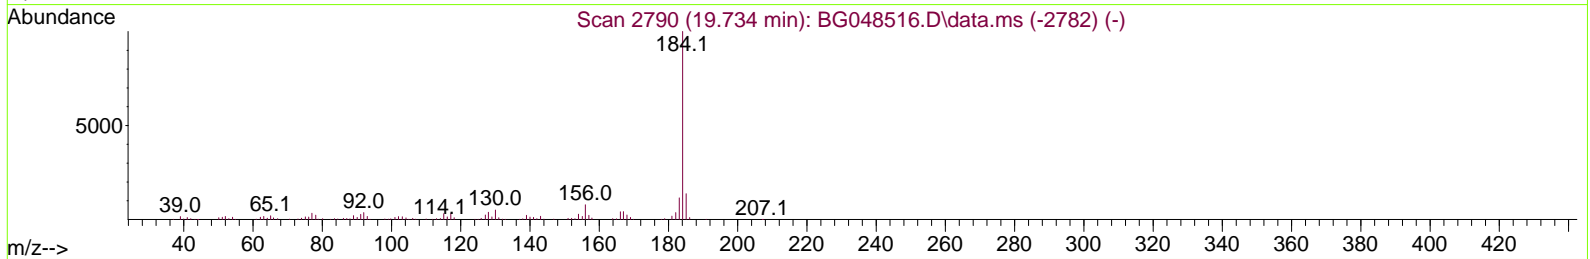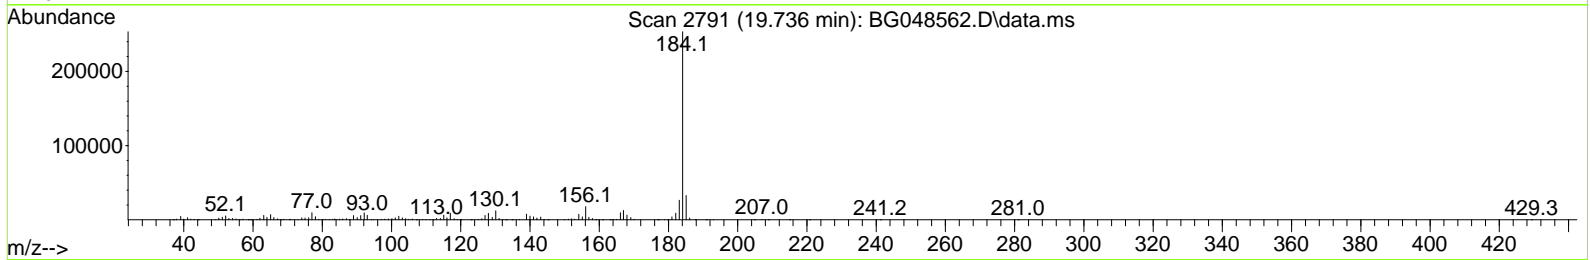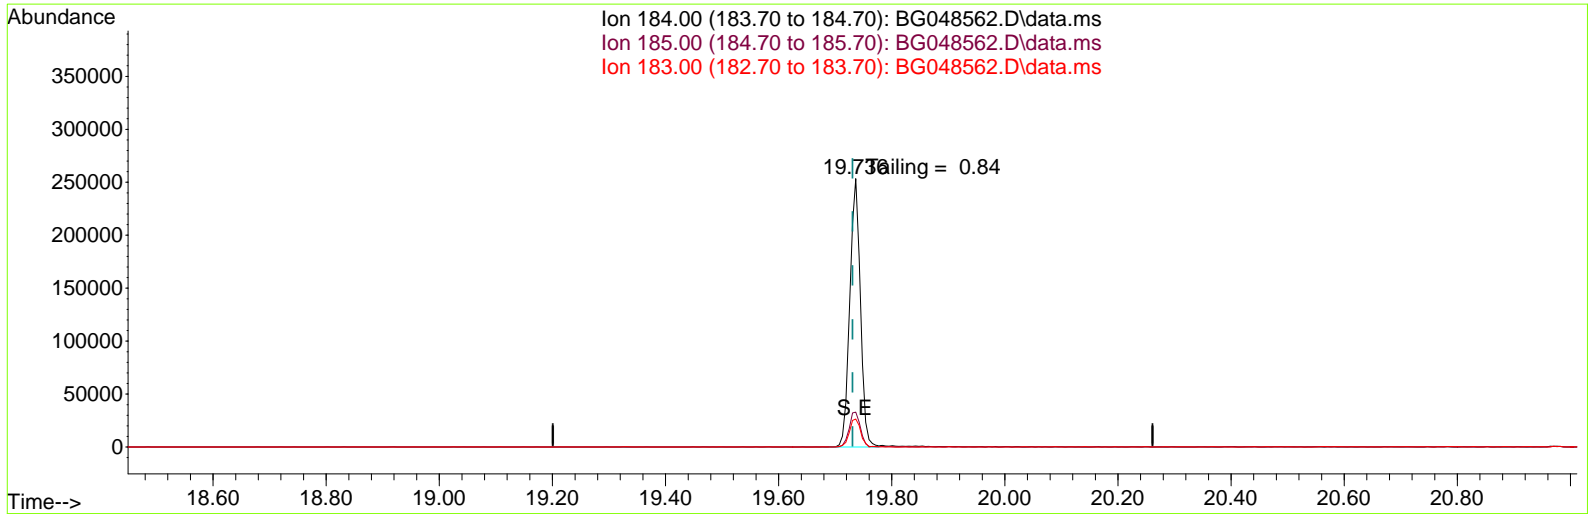

TIC: BG048562.D\data.ms

(77) Benzidine

19.736min (+ 0.005) 89987.22 ng

response 332149

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.00
183.00	11.50	10.43
0.00	0.00	0.00