
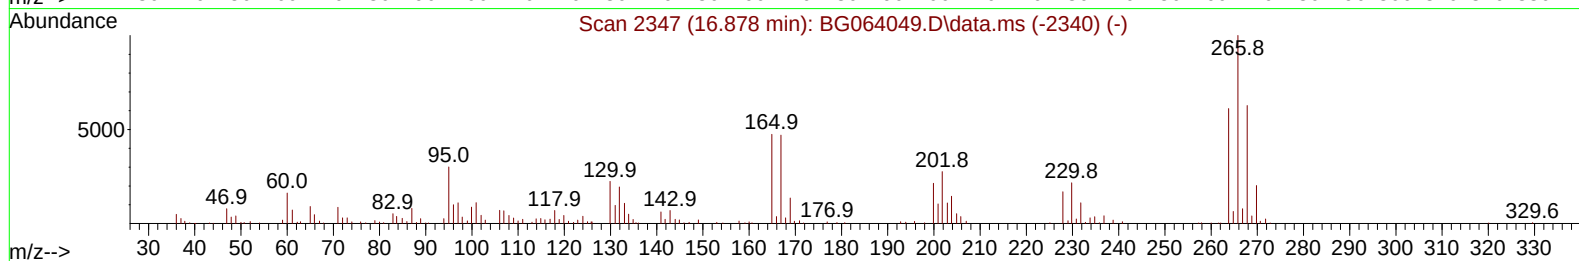
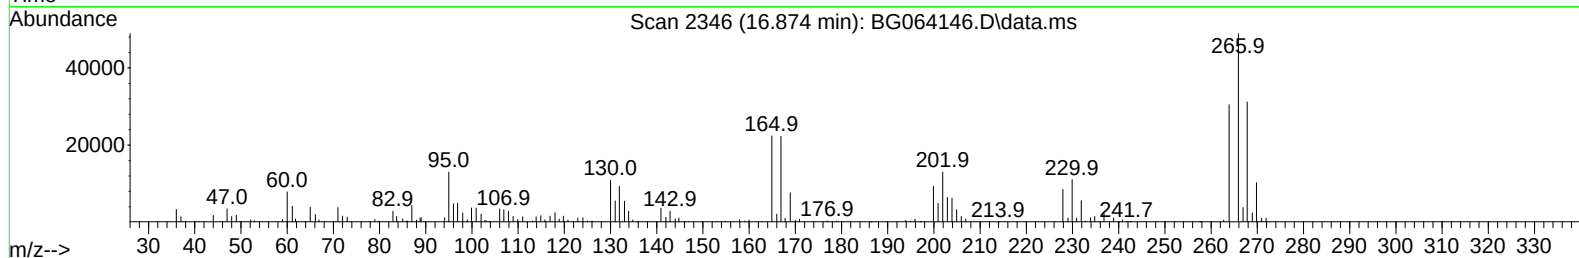


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040225\
Data File : BG064146.D
Acq On : 2 Apr 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 12:56:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

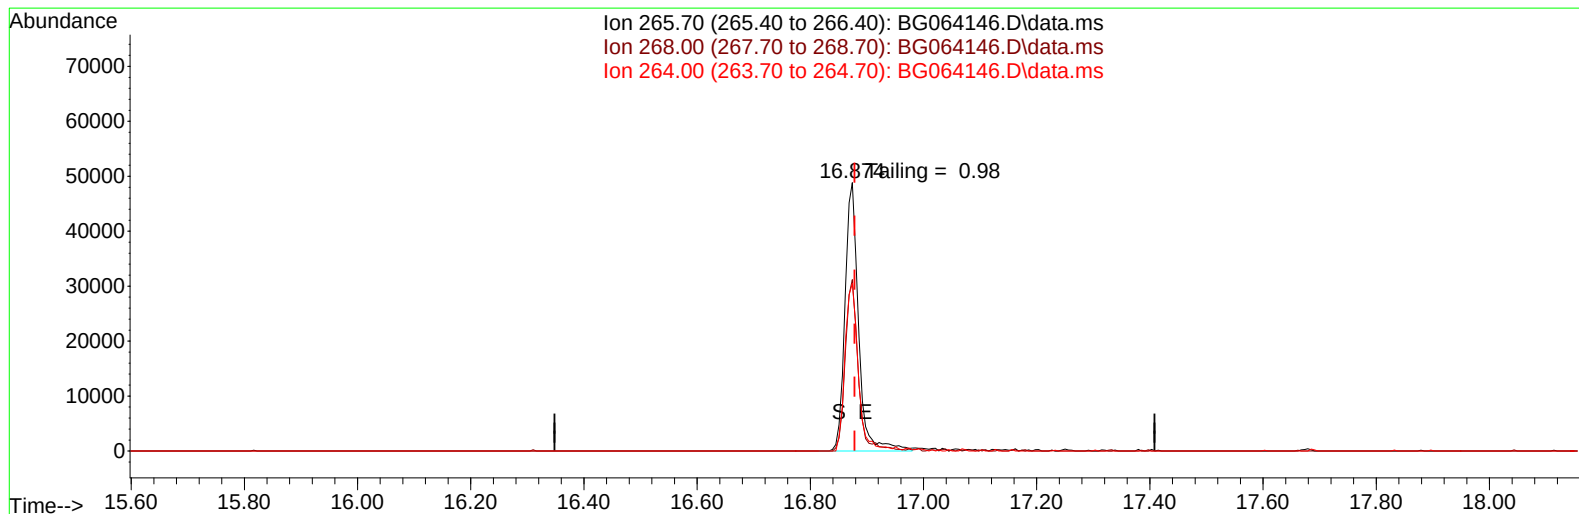

TIC: BG064146.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.004) 161654.29 ng

response 81711

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.88
264.00	61.10	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040225\
Data File : BG064146.D
Acq On : 2 Apr 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 12:56:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

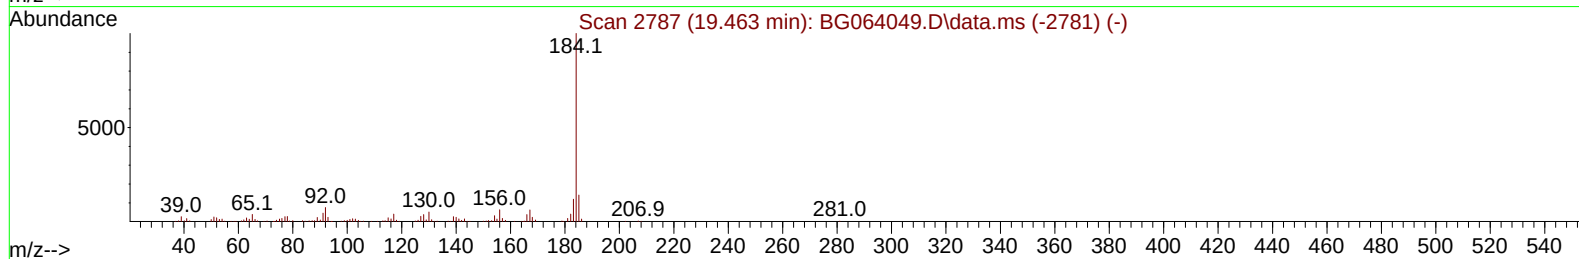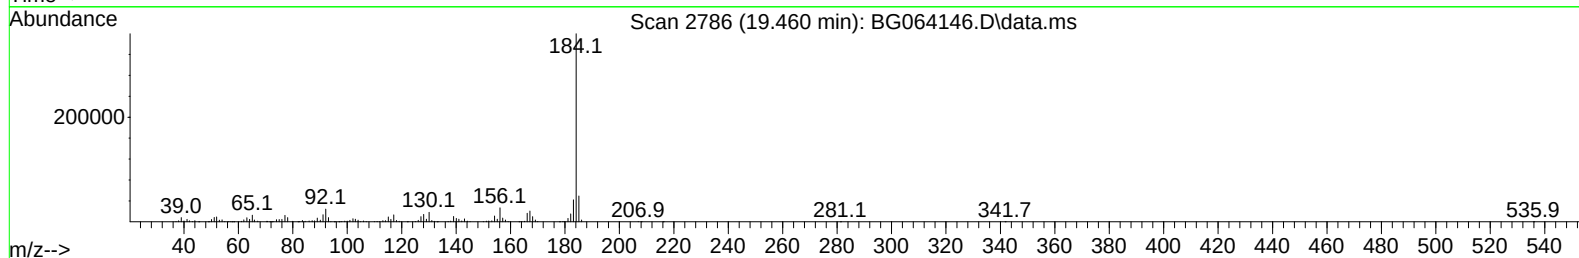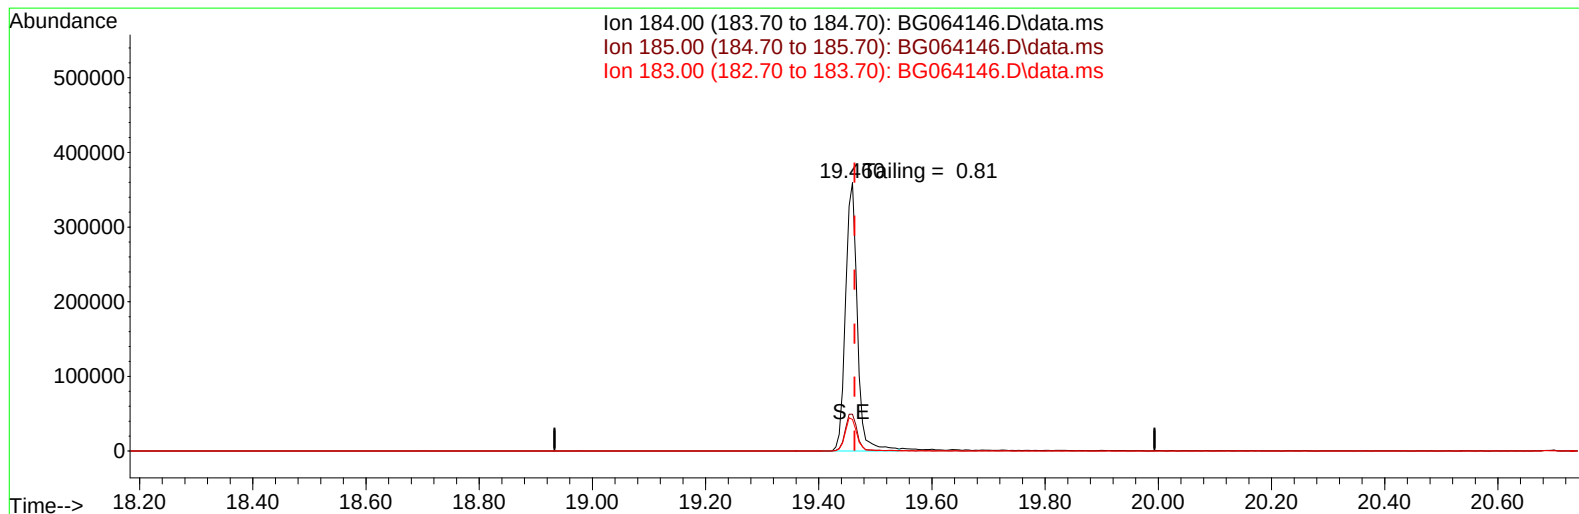

TIC: BG064146.D\data.ms

(77) Benzidine**19.460min (-0.003) 440472.91 ng****response 518440**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.70
183.00	11.90	11.74
0.00	0.00	0.00