
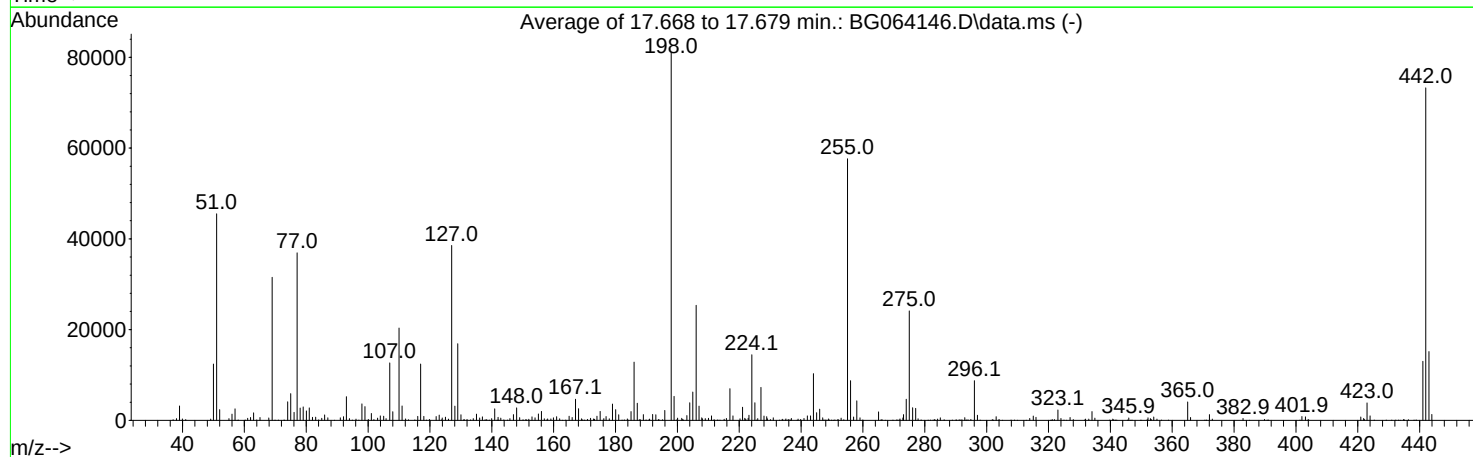


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040225\
Data File : BG064146.D
Acq On : 2 Apr 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

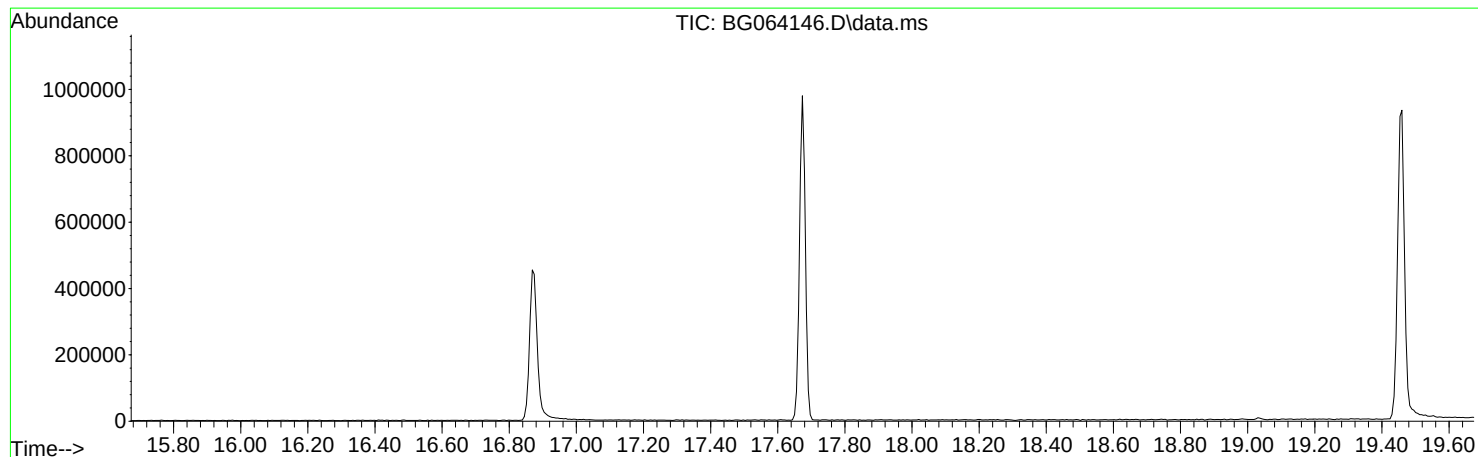

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	45533	PASS
68	69	0.00	2	1.7	525	PASS
69	198	0.00	100	38.9	31523	PASS
70	69	0.00	2	0.2	63	PASS
127	198	10	80	47.6	38552	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81067	PASS
199	198	5	9	6.5	5301	PASS
275	198	10	60	29.7	24117	PASS
365	198	1	100	5.0	4056	PASS
441	198	0.01	100	16.0	13005	PASS
442	442	50	100	100.0	73283	PASS
443	442	15	24	20.7	15181	PASS