


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040317\
 Data File : BG026538.D
 Acq On : 3 Apr 2017 16:59
 Operator : SJ/MA
 Sample : DFTPP24
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP24

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG032717MA.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 04 16:17:25 2017

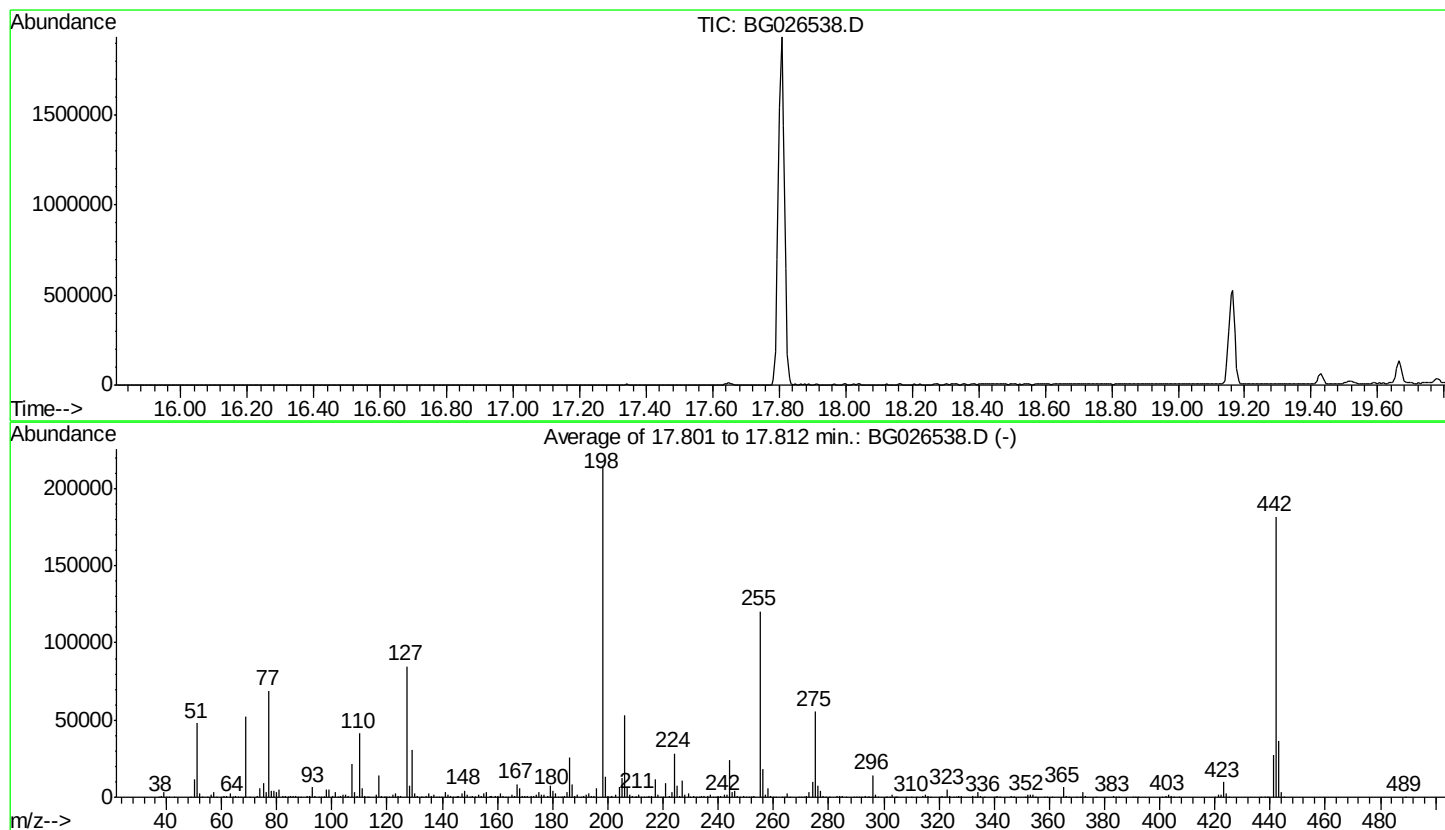

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.3	47946	PASS
68	69	0.00	2	0.7	348	PASS
69	198	0.00	100	24.5	52621	PASS
70	69	0.00	2	0.5	267	PASS
127	198	10	80	39.5	84994	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	214912	PASS
199	198	5	9	6.4	13654	PASS
275	198	10	60	25.8	55424	PASS
365	198	1	100	3.0	6503	PASS
441	442	0.01	100	15.2	27672	PASS
442	198	50	100	84.6	181909	PASS
443	442	15	24	19.9	36173	PASS

m/z	Abundance
37.00	206.0
38.10	578.0
39.20	3196.0
40.10	394.0
41.00	163.0
44.10	613.0
49.00	535.0
50.10	12297.0
51.10	53848.0
52.10	3011.0
53.10	236.0
55.00	359.0
56.10	1997.0
57.10	3731.0
58.00	236.0
60.10	174.0
61.10	777.0
62.10	819.0
63.10	2318.0
64.00	336.0
65.10	1420.0
67.10	173.0
68.10	1046.0
69.00	57440.0
70.10	327.0
73.10	568.0
74.10	5801.0
75.10	10176.0
76.10	4148.0
77.10	74680.0
78.10	4710.0
79.10	4364.0
80.00	4006.0
81.00	5296.0
82.10	1235.0
83.00	1304.0
84.00	381.0
85.00	1115.0
86.10	1510.0
87.10	599.0
88.00	325.0
88.90	190.0
91.10	1293.0
92.10	1378.0
93.10	6815.0
94.00	729.0
96.10	821.0
97.00	240.0
98.10	5792.0
99.10	6235.0
100.20	541.0
101.00	3325.0
102.20	241.0
103.00	1040.0
104.10	1949.0
105.00	2215.0
106.00	460.0
107.10	21856.0
108.10	3283.0
109.10	904.0
110.00	43400.0
111.10	7159.0
112.10	731.0
113.10	173.0
116.00	1701.0
117.10	14555.0
118.00	1351.0
118.90	184.0
119.20	232.0
119.90	429.0
122.00	1560.0
123.10	2050.0
124.00	1022.0
125.10	721.0
127.10	85056.0
128.10	7122.0
129.00	30768.0
130.00	2716.0
131.10	635.0
132.10	562.0
133.00	154.0
134.10	756.0
135.10	2967.0
136.10	898.0
137.10	2197.0
138.10	338.0
139.00	185.0
141.10	3226.0
142.10	1456.0
143.00	666.0
144.00	423.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

145.20	261.0
146.00	653.0
147.10	2079.0
148.10	4418.0
149.10	1435.0
150.10	372.0
151.10	534.0
152.00	413.0
153.10	1330.0
154.00	1307.0
155.10	2488.0
156.10	4129.0
157.20	1261.0
158.10	642.0
159.10	504.0
160.00	1115.0
161.00	2253.0
162.10	463.0
163.10	205.0
164.10	210.0
165.10	1278.0
166.00	955.0
167.10	8594.0
168.10	6814.0
169.00	1114.0
170.00	661.0
171.00	574.0
172.00	953.0
173.00	972.0
174.10	1876.0
175.10	3409.0
176.10	1244.0
177.00	1668.0
178.00	398.0
179.00	6804.0
180.00	4424.0
181.10	2261.0
182.00	425.0
183.50	266.0
184.10	543.0
185.10	3013.0
186.10	23976.0
187.10	7570.0
188.10	1161.0
189.10	1568.0
190.10	323.0
191.10	714.0
192.00	1410.0
193.10	2569.0
194.00	692.0
195.10	533.0
196.10	5674.0
198.00	202880.0
199.00	13889.0
200.00	1126.0
201.60	642.0
203.00	928.0
204.10	6535.0
205.10	11985.0
206.10	49592.0
207.10	7523.0
208.10	1573.0
209.00	654.0
210.10	729.0
211.00	1961.0
212.10	429.0
212.90	169.0
215.00	675.0
216.00	785.0
217.00	11500.0
218.00	1594.0
219.10	172.0
221.10	8694.0
223.10	3281.0
224.10	26328.0
225.10	6443.0
226.10	927.0
227.10	9172.0
228.00	1376.0
229.10	3038.0
230.00	265.0
231.00	1175.0
232.10	299.0
233.00	184.0
234.10	623.0
235.00	734.0
236.10	443.0
237.10	1320.0
238.10	312.0
239.00	432.0
240.10	546.0
241.10	762.0
242.10	1255.0
243.10	1490.0
244.10	21992.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

245.10	2521.0
246.00	3960.0
247.00	1100.0
249.00	989.0
251.00	200.0
253.10	934.0
255.10	109848.0
256.10	16528.0
257.10	1657.0
258.10	5566.0
259.10	1346.0
260.00	238.0
260.90	257.0
265.00	2332.0
266.10	405.0
269.90	200.0
271.00	292.0
272.00	654.0
273.00	2864.0
274.00	8673.0
275.10	49496.0
276.10	6960.0
277.00	3504.0
278.00	753.0
283.00	309.0
284.20	264.0
285.00	621.0
286.10	186.0
289.10	322.0
290.00	223.0
292.10	328.0
293.00	842.0
294.10	320.0
294.90	348.0
296.00	12306.0
297.10	1724.0
300.80	164.0
302.10	228.0
303.10	1315.0
304.00	491.0
308.00	259.0
310.10	153.0
314.10	670.0
315.00	1273.0
316.10	859.0
316.90	163.0
320.20	154.0
321.10	434.0
322.10	173.0
323.10	4557.0
324.00	885.0
327.00	560.0
328.00	498.0
332.00	236.0
333.00	268.0
334.10	3200.0
335.10	702.0
336.20	196.0
340.00	279.0
341.00	525.0
342.10	205.0
346.10	994.0
346.90	159.0
352.00	1212.0
353.10	923.0
354.10	1307.0
355.10	269.0
365.10	4629.0
366.00	671.0
370.10	241.0
371.00	210.0
372.10	2443.0
373.00	473.0
383.00	391.0
384.10	187.0
385.00	191.0
390.00	158.0
391.20	192.0
401.00	186.0
402.10	688.0
403.10	998.0
404.10	613.0
421.00	1522.0
422.10	1666.0
423.10	7981.0
424.10	2296.0
425.10	362.0
441.10	19136.0
442.10	134848.0
443.10	28984.0
444.10	2145.0
488.80	193.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

m/z	Abundance
37.10	238.0
38.10	585.0
39.10	3327.0
40.10	254.0
43.00	213.0
44.00	758.0
49.10	406.0
50.10	13067.0
51.10	56104.0
52.10	3036.0
55.10	506.0
56.10	1914.0
57.10	4221.0
58.10	237.0
61.10	871.0
62.00	717.0
63.10	2785.0
64.00	376.0
65.10	1430.0
66.10	185.0
67.00	154.0
69.00	61440.0
70.00	474.0
73.20	737.0
74.10	6844.0
75.10	11389.0
76.10	3709.0
77.10	81912.0
78.10	4468.0
79.10	5189.0
80.00	3676.0
81.10	5279.0
82.00	1591.0
83.00	1457.0
84.20	244.0
85.10	1346.0
86.00	1412.0
87.10	1113.0
87.90	334.0
88.90	166.0
91.00	1340.0
92.00	1405.0
93.00	7763.0
94.10	724.0
95.30	301.0
96.00	498.0
97.20	240.0
98.10	6093.0
99.00	5819.0
100.10	747.0
101.10	3641.0
102.00	349.0
103.10	1091.0
104.10	1663.0
105.10	1598.0
106.10	939.0
107.10	25896.0
108.10	3757.0
110.10	49320.0
111.10	7102.0
112.00	858.0
112.90	153.0
113.40	153.0
116.10	1491.0
117.10	16568.0
118.00	1492.0
120.00	538.0
120.90	203.0
122.10	1427.0
123.10	2789.0
124.00	1233.0
125.00	1155.0
127.10	103056.0
128.10	8875.0
129.10	34536.0
130.10	3122.0
131.10	628.0
132.20	432.0
133.00	201.0
134.00	1362.0
135.10	2946.0
136.10	1084.0
137.10	1865.0
138.00	440.0
139.00	184.0
139.90	370.0
141.00	4134.0
142.10	1781.0
143.00	1182.0
144.00	271.0
144.90	354.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

146.00	619.0
147.10	3082.0
148.00	4934.0
149.00	2065.0
150.00	320.0
151.10	696.0
151.70	416.0
152.00	407.0
153.10	1482.0
154.10	1207.0
155.10	2900.0
156.00	4214.0
157.10	830.0
158.00	840.0
159.10	796.0
160.00	1427.0
161.00	2909.0
162.10	736.0
163.00	316.0
164.10	363.0
165.00	1795.0
166.10	1461.0
167.10	9496.0
168.10	6907.0
169.10	1221.0
170.00	527.0
171.00	444.0
172.00	969.0
173.10	989.0
174.00	2079.0
175.10	4926.0
176.10	1554.0
177.00	1578.0
178.10	604.0
179.00	8815.0
180.10	5203.0
181.10	2522.0
182.00	566.0
183.90	627.0
185.00	3808.0
186.10	30392.0
187.10	10285.0
188.10	904.0
189.10	1705.0
190.10	206.0
191.10	1027.0
192.00	2510.0
193.10	2153.0
194.10	814.0
194.90	391.0
196.10	7590.0
198.00	255424.0
199.00	15542.0
200.00	1249.0
200.80	255.0
201.50	1651.0
203.10	1809.0
204.10	7026.0
205.10	13883.0
206.10	63208.0
207.10	8911.0
208.10	2015.0
208.90	654.0
210.30	1108.0
211.00	2692.0
213.00	189.0
214.10	156.0
215.00	437.0
215.90	1093.0
217.00	13478.0
218.10	2111.0
221.10	11558.0
222.10	1758.0
223.10	3585.0
224.10	34544.0
225.10	8819.0
226.10	839.0
227.00	13891.0
228.00	1988.0
229.00	2884.0
230.00	740.0
231.10	1190.0
232.00	202.0
233.00	498.0
234.10	922.0
235.00	1085.0
236.00	899.0
237.10	1608.0
239.10	610.0
240.10	508.0
241.00	751.0
242.10	1581.0
243.10	1799.0
244.10	27544.0
245.10	4084.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

246.00	4102.0
247.10	514.0
248.00	257.0
249.00	1059.0
250.00	181.0
251.00	479.0
251.80	256.0
253.10	656.0
255.10	143488.0
256.10	22696.0
257.00	1719.0
258.00	7419.0
259.00	1538.0
260.00	381.0
260.90	275.0
264.00	323.0
265.00	3139.0
266.00	370.0
269.00	166.0
271.00	359.0
272.00	424.0
273.00	4819.0
274.00	11875.0
275.10	65456.0
276.10	9316.0
277.10	5205.0
277.90	879.0
279.00	174.0
281.00	237.0
283.00	608.0
284.10	612.0
285.10	1050.0
286.10	272.0
289.10	229.0
292.10	421.0
293.10	1375.0
294.10	548.0
296.10	17736.0
297.10	2823.0
298.00	208.0
301.00	358.0
302.00	429.0
303.10	1807.0
304.00	542.0
307.90	368.0
310.00	251.0
311.90	155.0
314.10	954.0
315.00	1528.0
316.10	1305.0
316.90	204.0
321.10	522.0
322.10	324.0
323.10	5063.0
324.10	1226.0
325.20	253.0
326.30	175.0
327.00	1147.0
328.00	610.0
332.10	637.0
333.00	524.0
334.10	4385.0
335.10	996.0
336.20	186.0
341.10	1135.0
342.10	272.0
346.00	974.0
347.10	204.0
351.10	182.0
352.10	1855.0
353.10	1627.0
354.10	1768.0
355.00	350.0
358.00	191.0
365.00	8093.0
366.00	1035.0
367.10	165.0
369.90	196.0
371.00	161.0
372.10	3644.0
373.10	760.0
377.00	186.0
383.10	1076.0
384.10	463.0
390.00	461.0
391.00	409.0
392.00	207.0
402.10	1444.0
403.10	1765.0
404.10	584.0
404.90	159.0
407.10	232.0
420.00	189.0
421.10	1652.0
422.10	2032.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

423.10	10019.0
424.10	2396.0
425.10	389.0
436.50	180.0
437.90	158.0
439.50	211.0
441.10	31936.0
442.10	209920.0
443.10	42040.0
444.10	4316.0
445.00	405.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

m/z	Abundance
38.10	407.0
39.10	2446.0
39.90	240.0
44.10	741.0
50.10	8746.0
51.10	33888.0
52.10	1513.0
55.10	457.0
56.10	1258.0
57.10	3226.0
58.10	168.0
61.00	484.0
62.10	573.0
63.10	1956.0
63.90	226.0
65.10	670.0
69.00	38984.0
73.10	454.0
74.10	4099.0
75.10	6655.0
76.10	2423.0
77.10	51072.0
78.10	3810.0
79.00	2640.0
80.00	2654.0
81.10	4348.0
82.00	883.0
83.00	970.0
84.00	272.0
85.20	510.0
86.00	827.0
87.10	408.0
88.00	382.0
91.00	884.0
92.10	955.0
93.00	4957.0
94.10	373.0
96.30	262.0
98.10	4383.0
99.00	3434.0
100.10	504.0
101.00	2782.0
102.00	344.0
103.00	867.0
104.00	1522.0
105.00	1291.0
106.10	503.0
107.10	17312.0
108.00	2225.0
109.10	815.0
110.00	31384.0
111.00	4449.0
112.00	504.0
113.00	278.0
116.00	825.0
117.00	11204.0
118.00	810.0
119.00	196.0
122.00	1360.0
123.00	1642.0
124.10	848.0
125.00	1038.0
127.10	66872.0
128.10	5536.0
129.00	25880.0
130.10	2048.0
131.00	564.0
132.10	207.0
132.80	198.0
134.00	1027.0
135.00	2818.0
136.00	680.0
137.10	1086.0
138.10	355.0
140.00	477.0
141.10	2851.0
142.10	1160.0
142.90	684.0
144.90	323.0
146.10	408.0
147.00	1859.0
148.00	3799.0
149.00	772.0
150.20	259.0
151.00	473.0
151.70	488.0
153.00	1223.0
154.00	745.0
155.10	2455.0
156.00	2733.0
157.10	542.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

158.00	581.0
159.00	375.0
160.00	952.0
161.10	1712.0
162.00	441.0
163.00	234.0
164.00	368.0
165.00	1391.0
166.00	992.0
167.10	7159.0
168.00	4489.0
169.00	1127.0
170.00	184.0
171.00	406.0
172.00	630.0
173.10	835.0
174.10	1918.0
175.00	2396.0
176.00	1069.0
177.10	1626.0
178.10	421.0
179.00	5864.0
180.10	4013.0
181.00	1891.0
182.10	342.0
183.10	252.0
184.10	592.0
185.00	2820.0
186.10	24080.0
187.10	6542.0
188.10	598.0
189.00	1065.0
190.10	181.0
191.00	740.0
192.10	1815.0
193.10	2033.0
194.00	579.0
195.10	544.0
196.00	5222.0
198.00	186432.0
199.00	11532.0
200.10	880.0
201.50	760.0
203.00	1323.0
204.10	6528.0
205.10	11110.0
206.10	45848.0
207.10	6452.0
208.00	1257.0
209.00	423.0
209.80	375.0
211.00	1268.0
212.10	362.0
215.10	621.0
216.00	973.0
217.00	10959.0
218.00	1328.0
219.00	182.0
220.00	324.0
221.10	8073.0
223.00	2495.0
224.10	24656.0
225.10	6596.0
226.10	778.0
227.00	10358.0
228.00	1350.0
229.00	1790.0
229.80	259.0
231.10	785.0
231.90	189.0
233.10	243.0
234.00	472.0
235.10	900.0
236.10	476.0
237.10	939.0
238.00	179.0
239.00	301.0
240.00	484.0
241.00	657.0
242.10	1318.0
243.10	1969.0
244.10	21864.0
245.10	2424.0
246.00	3844.0
247.10	721.0
249.00	786.0
251.10	166.0
252.10	442.0
253.10	655.0
255.10	108256.0
256.10	15806.0
257.10	1354.0
258.00	5778.0
259.10	910.0
260.00	259.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

263.00	163.0
264.00	222.0
265.10	2230.0
266.00	548.0
271.10	276.0
272.00	624.0
273.00	2927.0
274.10	9500.0
275.10	51320.0
276.10	7370.0
277.00	3645.0
278.10	821.0
280.10	164.0
283.00	788.0
284.10	481.0
285.10	604.0
289.00	316.0
290.10	170.0
290.90	163.0
293.00	816.0
294.10	261.0
294.80	406.0
296.00	12653.0
297.00	1586.0
301.10	202.0
302.10	180.0
303.10	1978.0
304.20	642.0
305.00	176.0
310.00	196.0
314.00	751.0
315.00	1190.0
316.00	879.0
321.10	416.0
322.10	270.0
323.10	4911.0
324.10	861.0
326.90	666.0
328.00	534.0
332.00	505.0
333.00	378.0
334.10	3180.0
335.10	925.0
341.10	716.0
346.00	1175.0
346.90	422.0
352.10	1362.0
353.10	1515.0
354.00	2064.0
359.10	241.0
360.90	215.0
365.00	6789.0
366.10	927.0
371.00	701.0
372.10	2950.0
373.00	341.0
376.80	152.0
383.10	763.0
384.00	346.0
390.10	205.0
391.10	294.0
392.00	216.0
401.00	524.0
402.10	1256.0
403.00	1403.0
404.00	407.0
421.10	1427.0
422.10	1238.0
423.10	10765.0
424.10	2940.0
425.10	488.0
439.10	185.0
441.10	31944.0
442.10	200960.0
443.10	37496.0
444.10	3462.0
445.10	270.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

Scan 2498 (17.765 min): BG026538.D
DFTPP24

m/z	Abundance
39.90	171.0
44.10	746.0
70.90	250.0
85.90	161.0
96.30	153.0
106.90	153.0
129.80	162.0
207.10	602.0
208.10	172.0
281.00	175.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24