
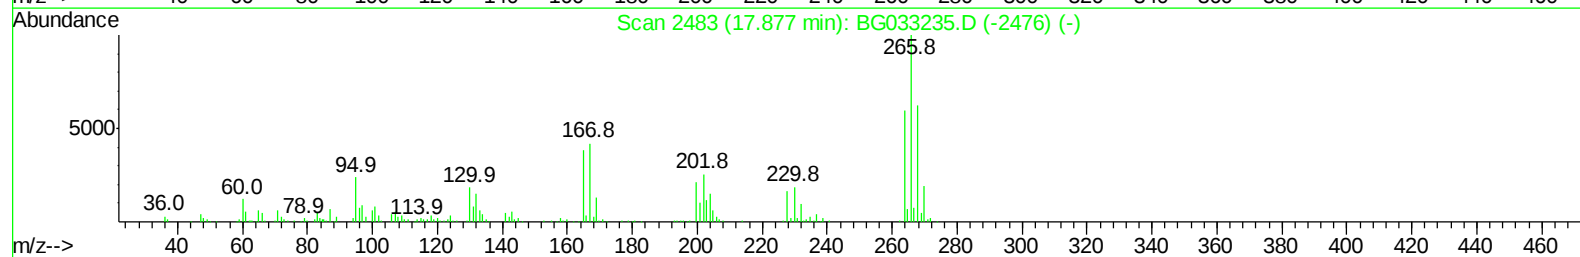
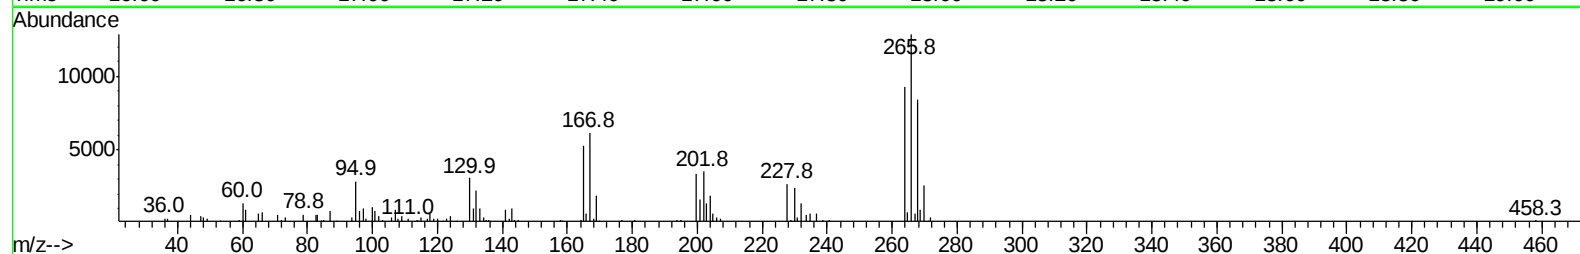


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040318\
Data File : BG033515.D
Acq On : 3 Apr 2018 8:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 04:56:24 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 14:50:26 2018
Response via : Initial Calibration

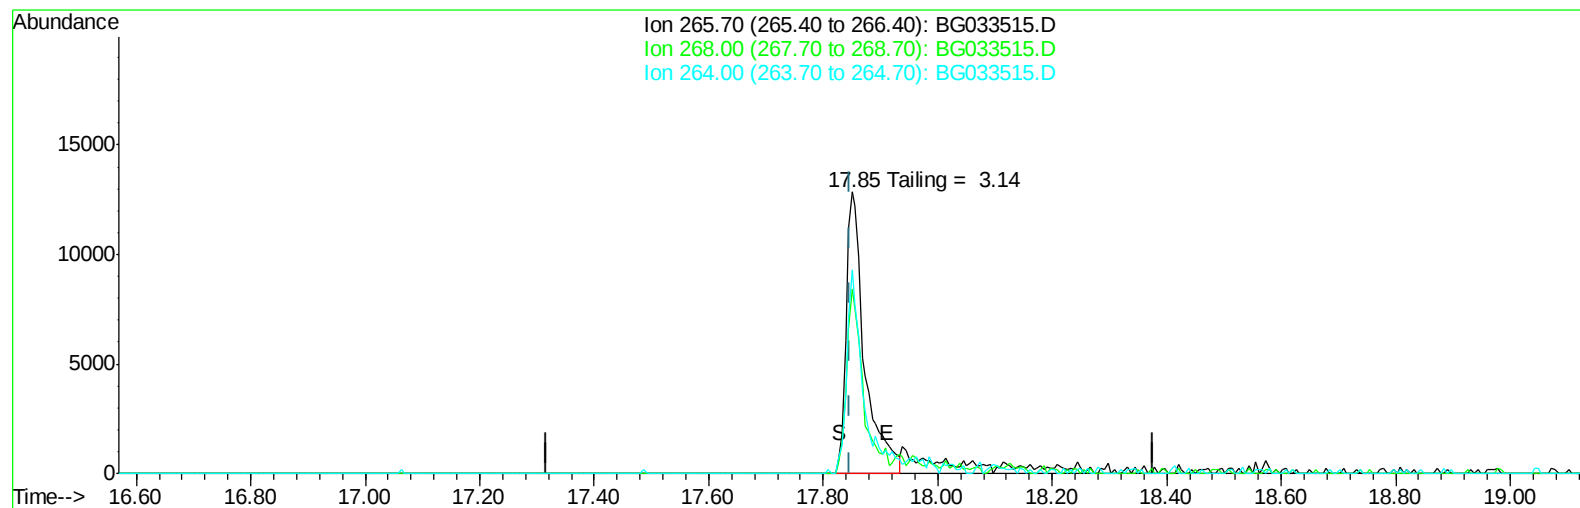

TIC: BG033515.D

(69) Pentachlorophenol (C)




17.850min (+0.003) 21525.52ng

response 28749

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	72.90
264.00	62.00	72.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040318\
Data File : BG033515.D
Acq On : 3 Apr 2018 8:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 04:56:24 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 14:50:26 2018
Response via : Initial Calibration

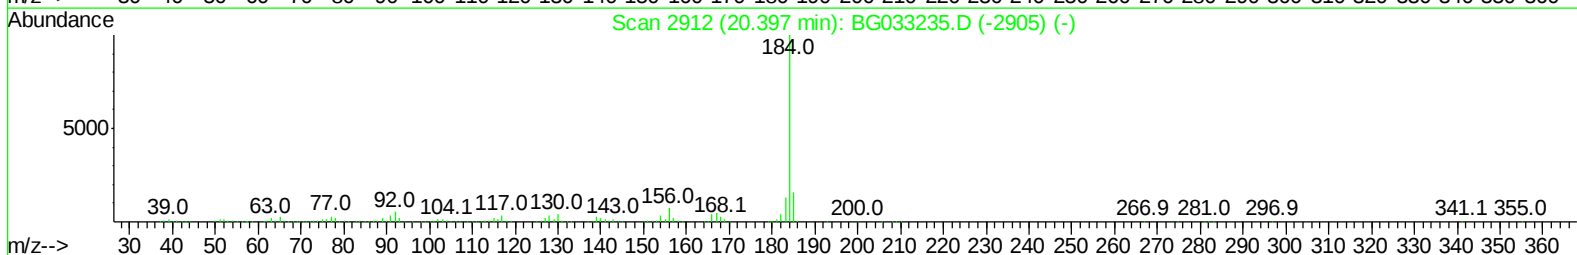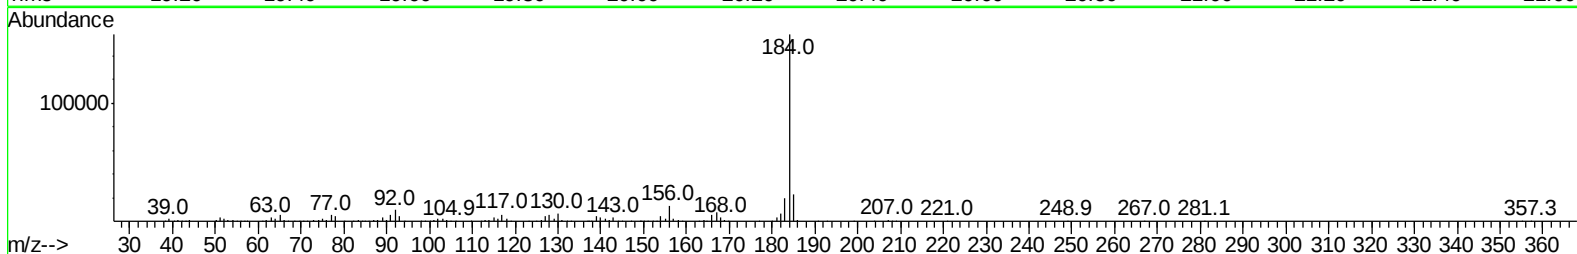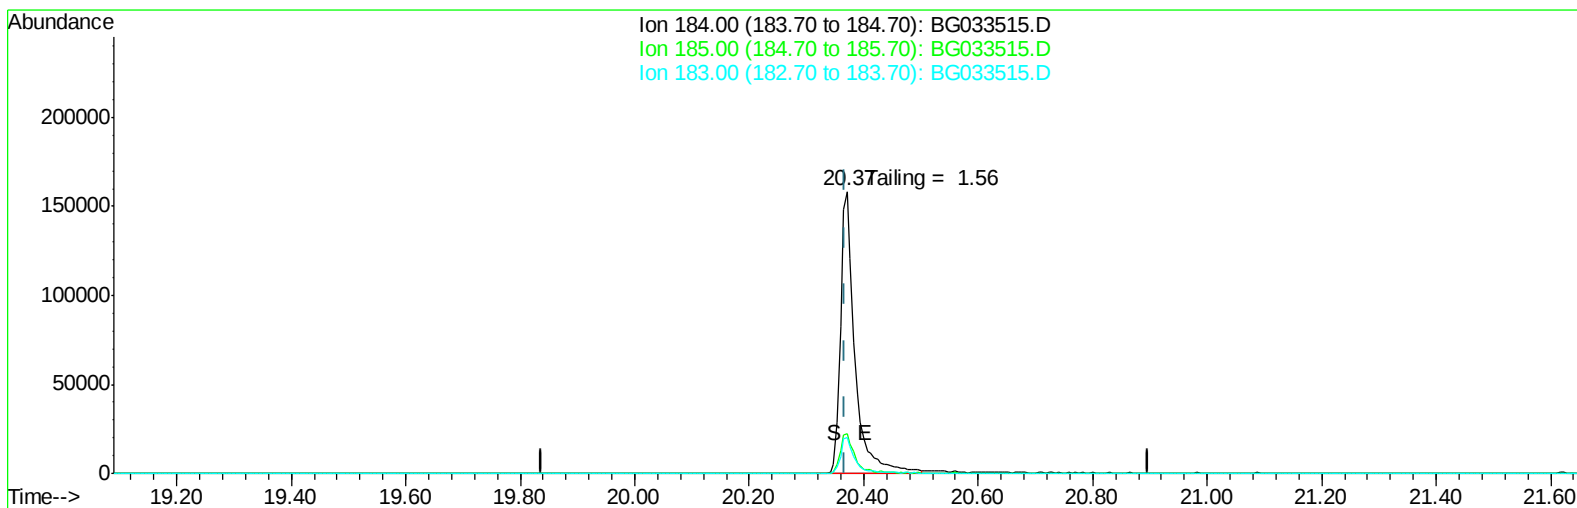

TIC: BG033515.D

(76) Benzidine

20.371min (+0.003) 181489.85ng

response 280539

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.32
183.00	13.30	12.75
0.00	0.00	0.00