
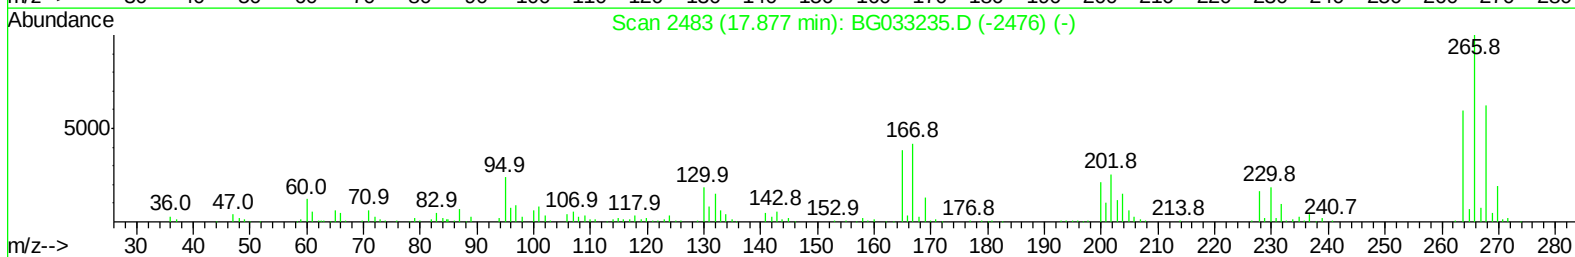
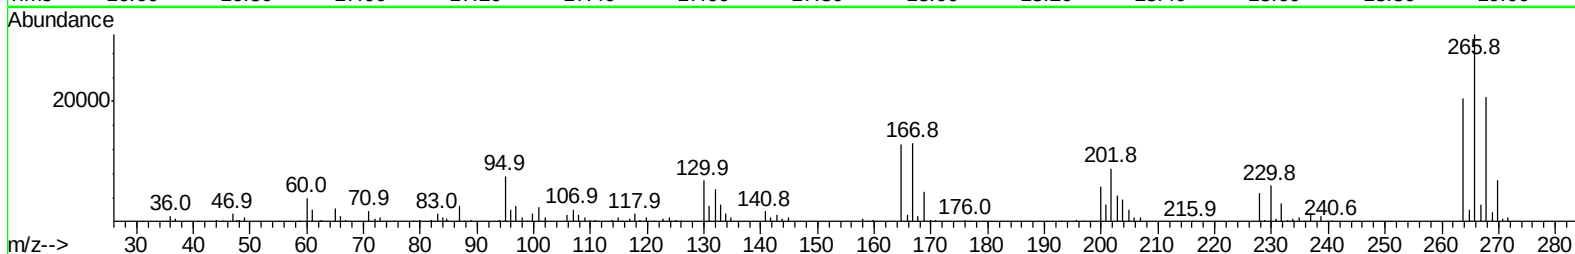


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040318\
Data File : BG033534.D
Acq On : 3 Apr 2018 21:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 04:57:33 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 14:50:26 2018
Response via : Initial Calibration

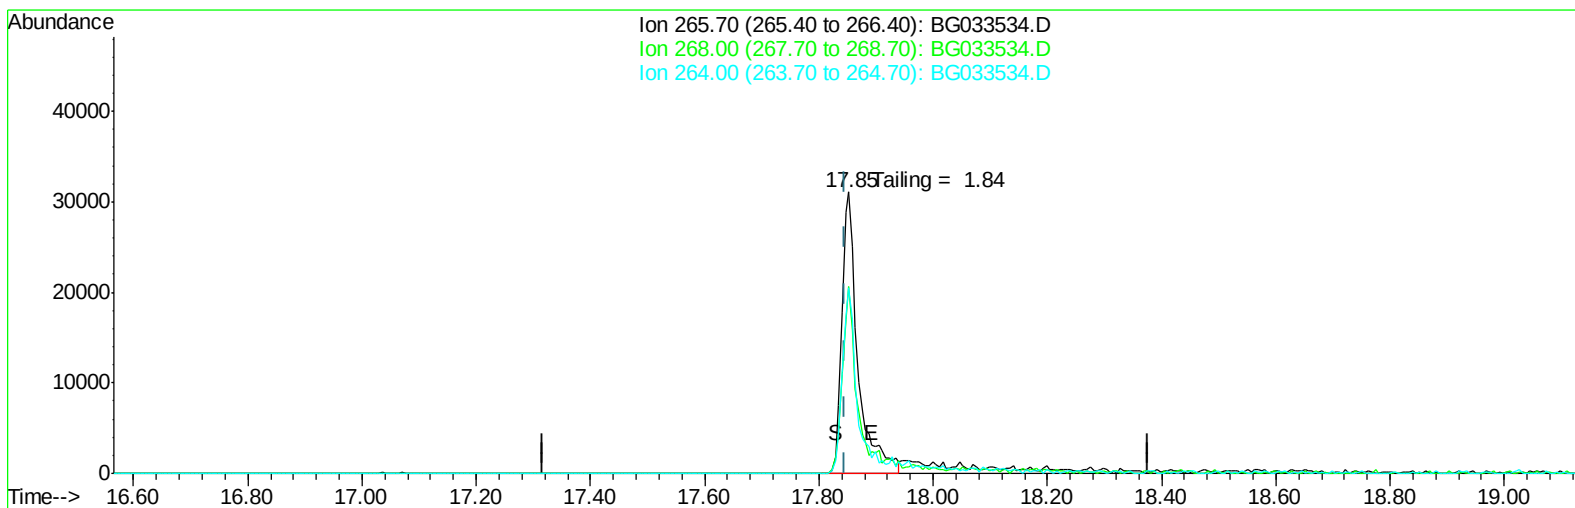

TIC: BG033534.D

(69) Pentachlorophenol (C)




17.852min (+0.005) 10609.68ng

response 61915

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.60
264.00	62.00	65.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040318\
Data File : BG033534.D
Acq On : 3 Apr 2018 21:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 04:57:33 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 14:50:26 2018
Response via : Initial Calibration

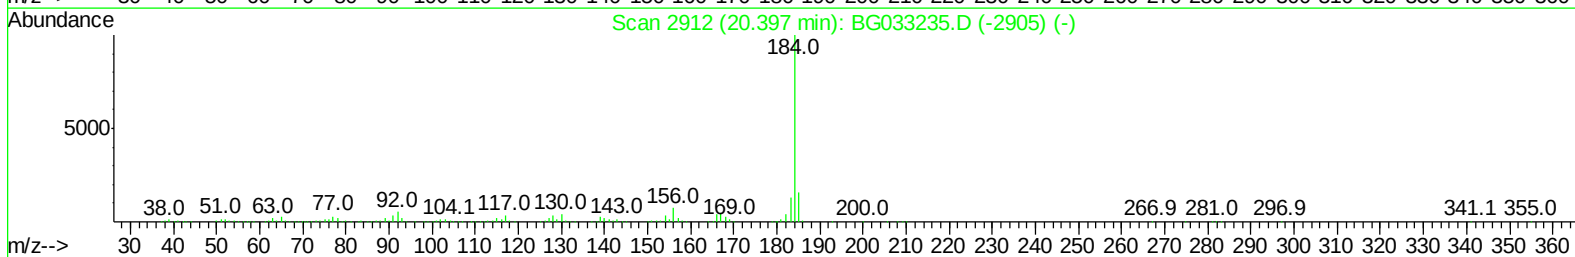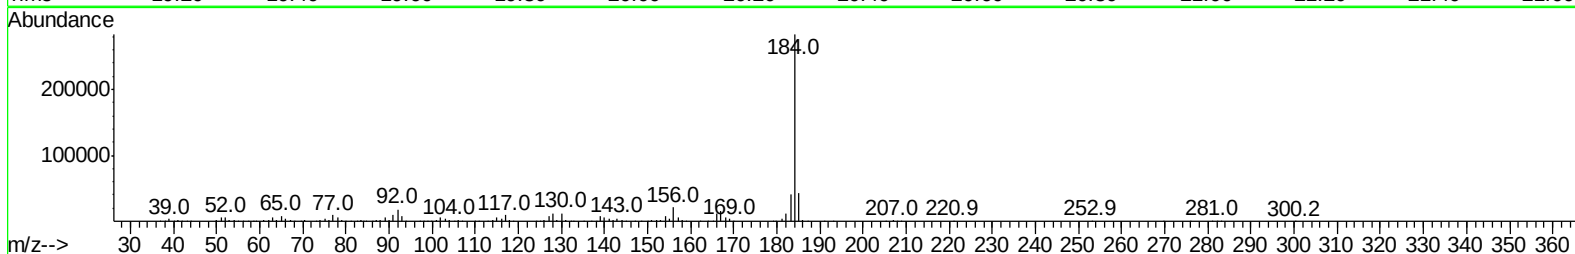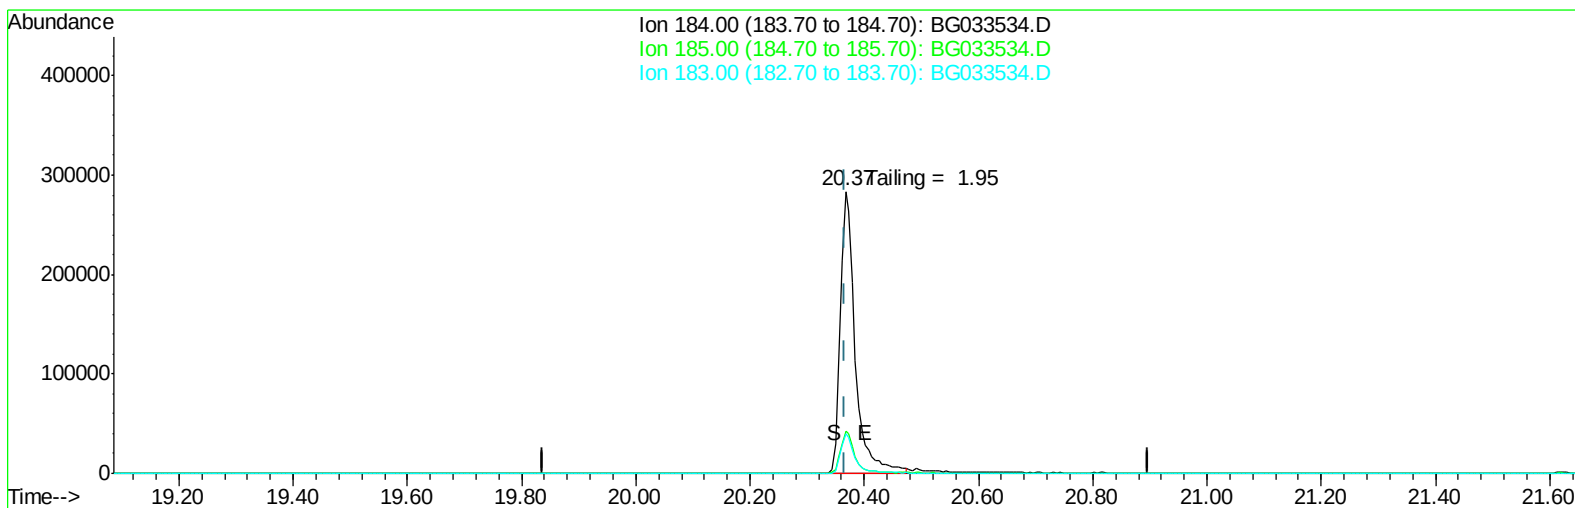

TIC: BG033534.D

(76) Benzidine

20.367min (-0.001) 0.00ng

response 516473

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.91
183.00	13.30	14.19
0.00	0.00	0.00