

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040318\
 Data File : BG033529.D
 Acq On : 3 Apr 2018 17:13
 Operator : SJ/JU
 Sample : J2131-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 4540-2

Quant Time: Apr 04 12:02:24 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 03 14:50:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	31622	20.00	ng	0.00
21) Naphthalene-d8	11.74	136	140600	20.00	ng	0.00
38) Acenaphthene-d10	15.48	164	111204	20.00	ng	0.00
63) Phenanthrene-d10	18.21	188	307630	20.00	ng	0.00
75) Chrysene-d12	22.56	240	314264	20.00	ng	0.00
86) Perylene-d12	26.33	264	316593	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	308558	182.97	ng	0.00
7) Phenol-d6	7.98	99	421367	145.42	ng	0.00
23) Nitrobenzene-d5	10.06	82	335092	109.50	ng	0.00
41) 2,4,6-Tribromophenol	16.96	330	248593	149.47	ng	0.00
44) 2-Fluorobiphenyl	14.11	172	831950	108.00	ng	0.00
78) Terphenyl-d14	20.73	244	1613564	109.81	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040318\
Data File : BG033529.D
Acq On : 3 Apr 2018 17:13
Operator : SJ/JU
Sample : J2131-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
4540-2

Quant Time: Apr 04 12:02:24 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 03 14:50:26 2018
Response via : Initial Calibration

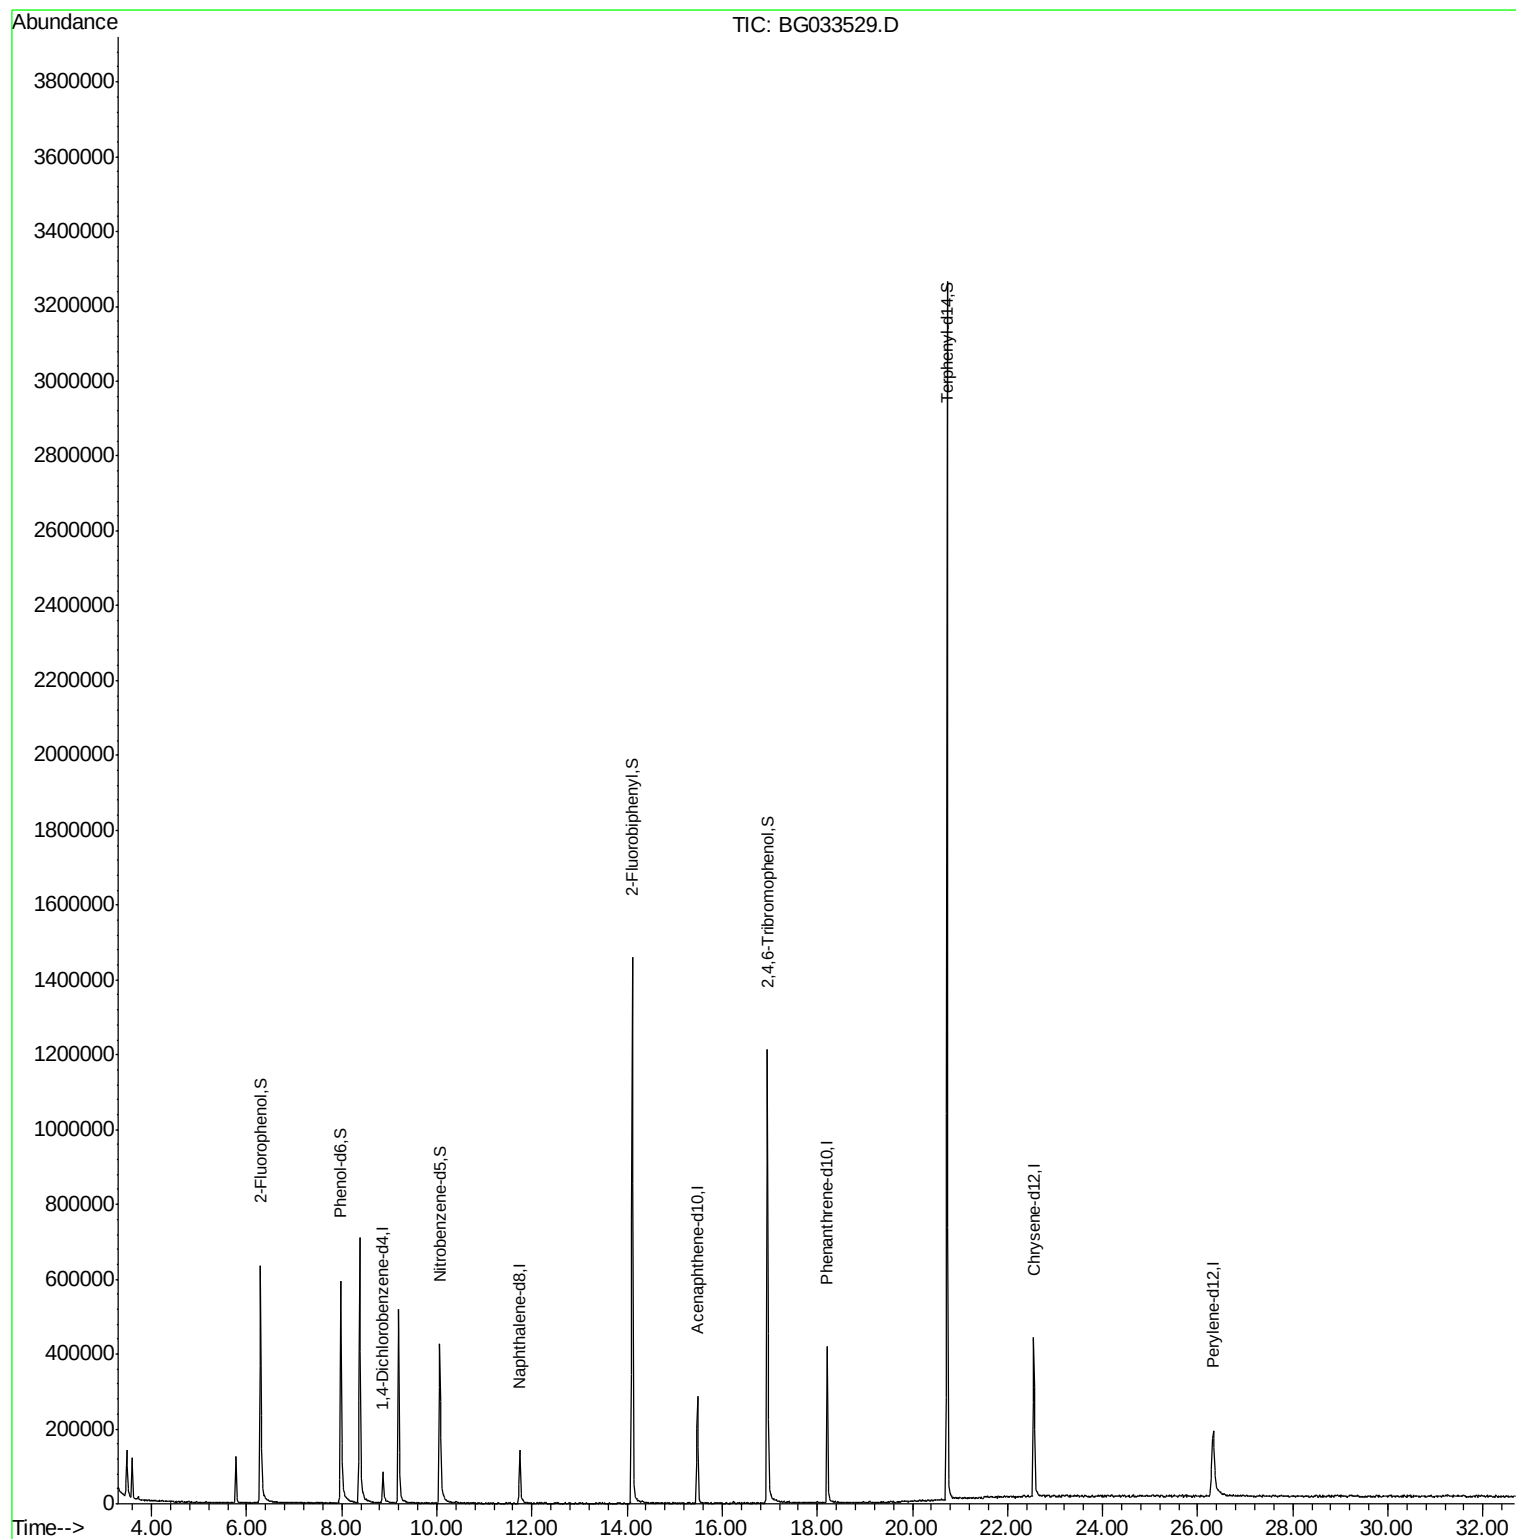

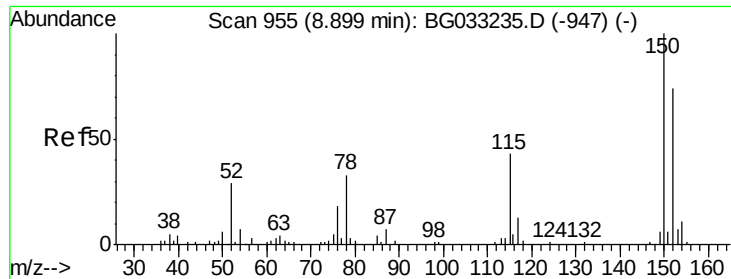


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.87 min Scan# 949
Delta R.T. -0.00 min
Lab File: BG033529.D
Acq: 3 Apr 2018 17:13

Instrument :
BNA_G
ClientSampleId :
4540-2

Tot Ion:152 Resp: 31622
Ion Ratio Lower Upper
152 100
150 147.7 126.6 189.8
115 61.0 53.0 79.4

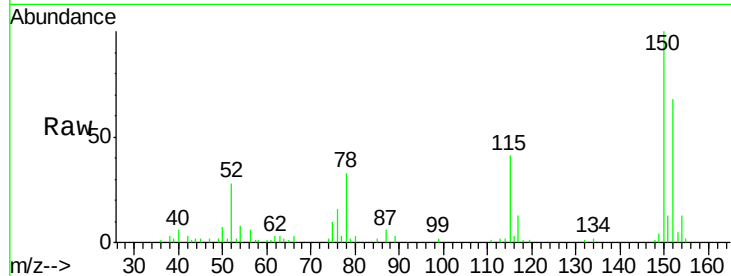


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

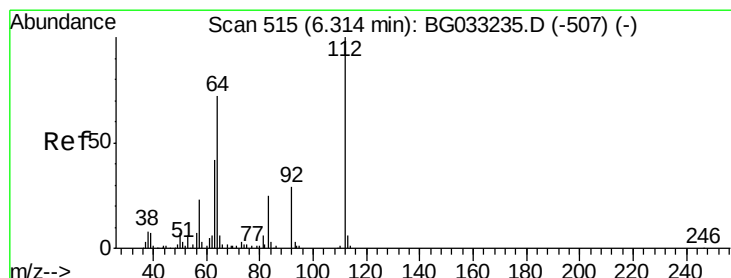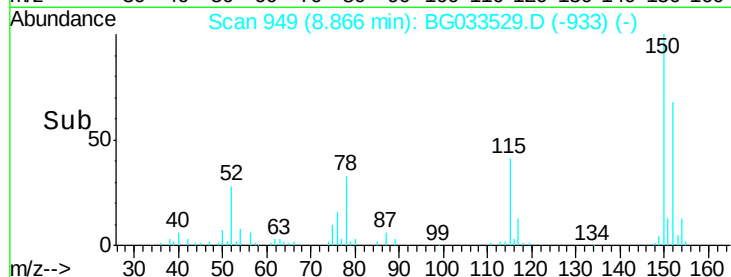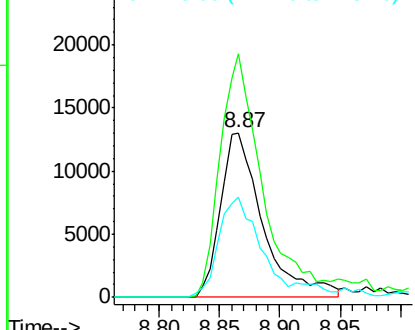



#5


2-Fluorophenol
Concen: 182.969 ng
RT: 6.29 min Scan# 511
Delta R.T. 0.00 min
Lab File: BG033529.D
Acq: 3 Apr 2018 17:13

Tgt Ion:112 Resp: 308558
Ion Ratio Lower Upper
112 100
64 71.6 56.3 84.5
63 40.1 30.1 45.1

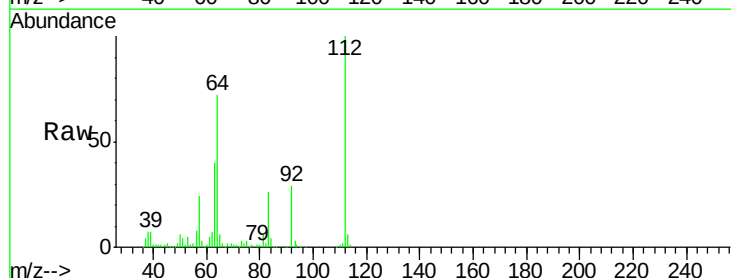

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

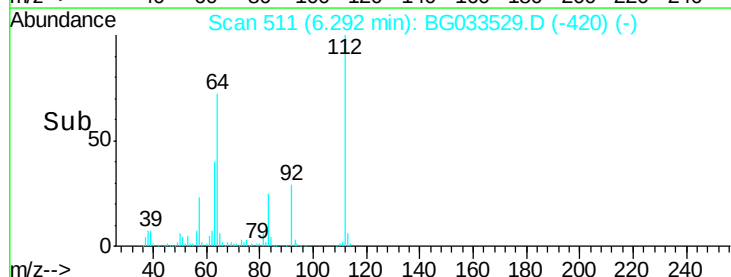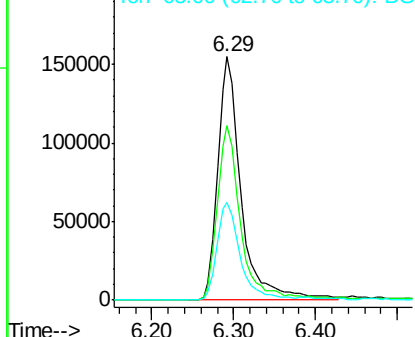

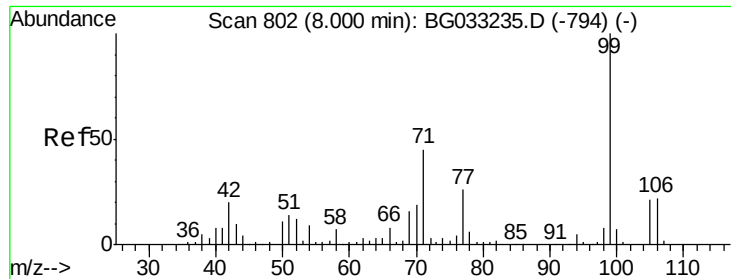

#7

Phenol-d6

Concen: 145.420 ng

RT: 7.98 min Scan# 798

Delta R.T. -0.00 min

Lab File: BG033529.D

Acq: 3 Apr 2018 17:13

Instrument :

BNA_G

ClientSampleId :

4540-2


Tot Ion: 99 Resp: 421367

Ion Ratio Lower Upper




99 100

42 20.7 14.1 21.1

71 43.7 26.1 39.1#

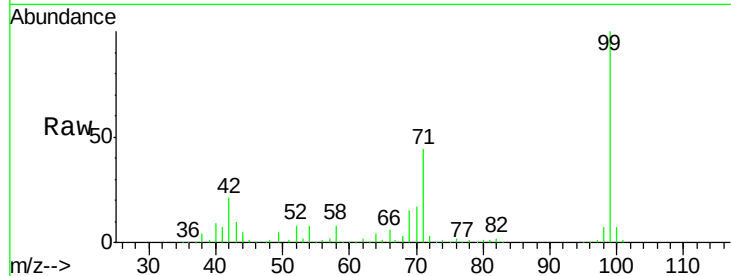

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

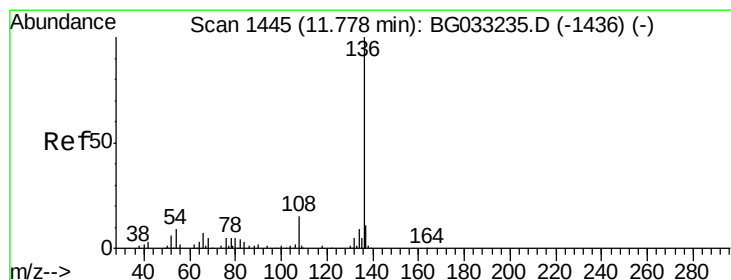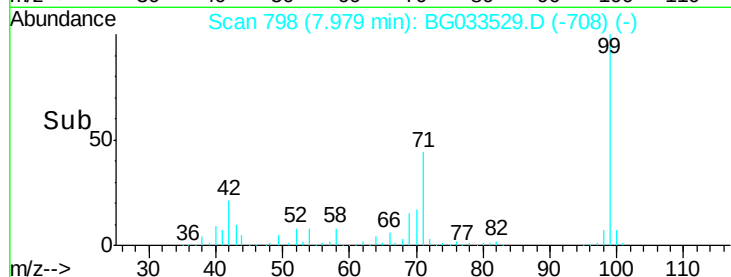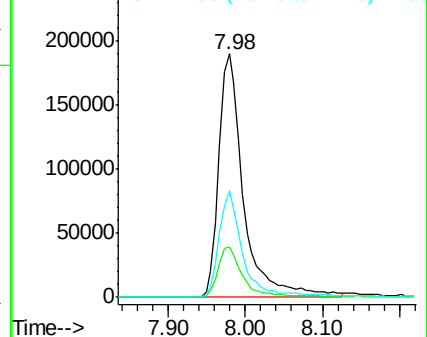

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.74 min Scan# 1439

Delta R.T. -0.00 min

Lab File: BG033529.D

Acq: 3 Apr 2018 17:13

Tgt Ion: 136 Resp: 140600


Ion Ratio Lower Upper

136 100



137 9.9 9.2 13.8


54 10.5 10.3 15.5

68 5.6 4.5 6.7

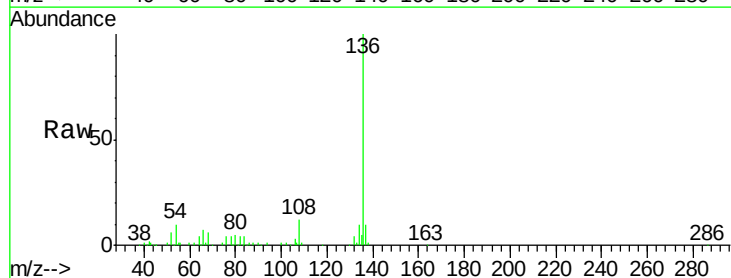

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



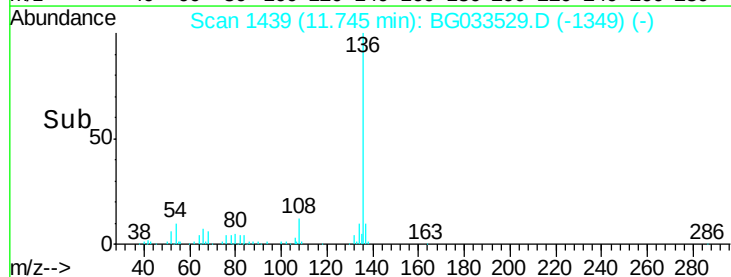
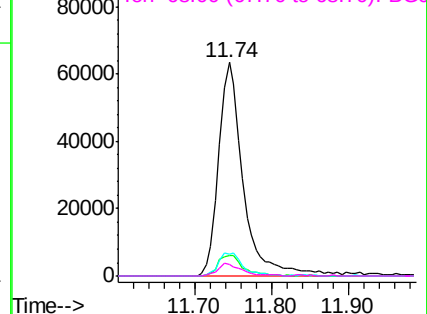


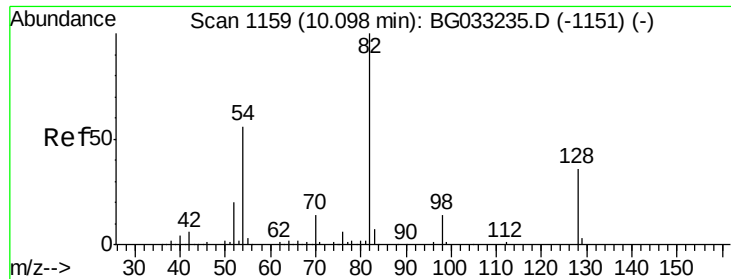

#23
 Nitrobenzene-d5
 Concen: 109.499 ng
 RT: 10.06 min Scan# 1153
 Delta R.T. 0.00 min
 Lab File: BG033529.D
 Acq: 3 Apr 2018 17:13




Instrument :
 BNA_G
 ClientSampleId :
 4540-2


Tot Ion	82	Resp	335092
Ion Ratio	Lower	Upper	
82	100		
128	36.4	29.7	44.5
54	58.0	43.1	64.7

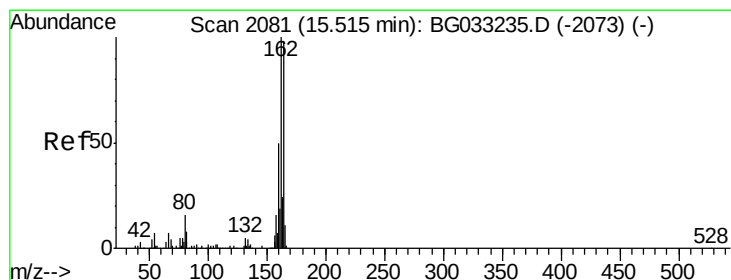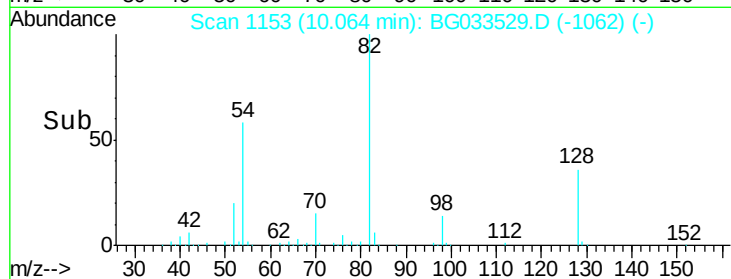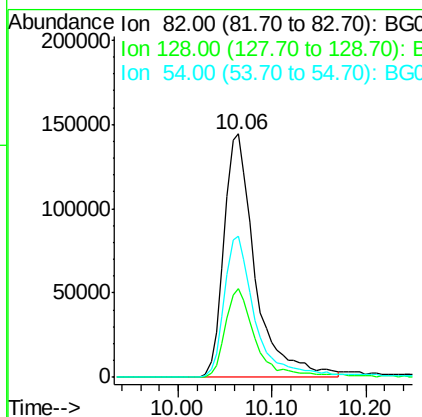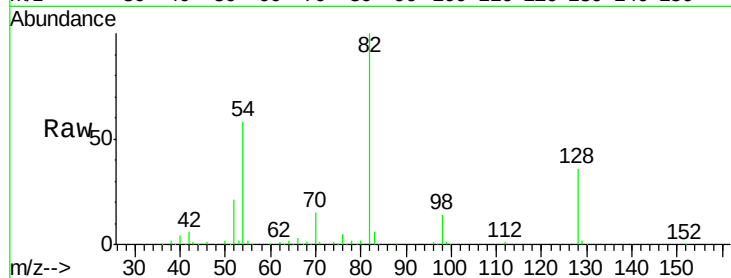

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.48 min Scan# 2075
 Delta R.T. 0.00 min
 Lab File: BG033529.D
 Acq: 3 Apr 2018 17:13

Tgt Ion	164	Resp	111204
Ion Ratio	Lower	Upper	
164	100		
162	98.5	78.8	118.2
160	44.5	35.4	53.0

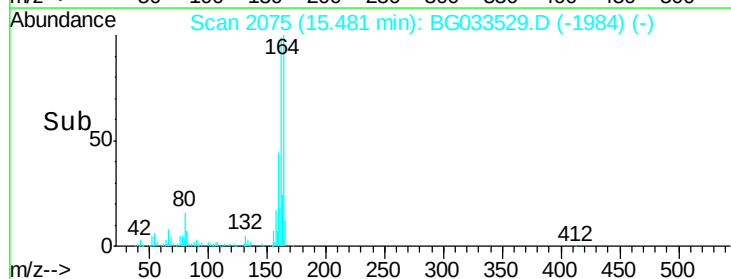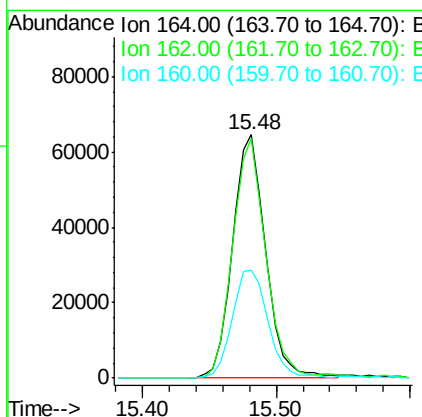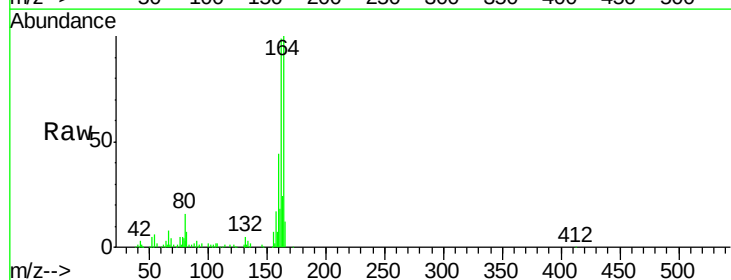


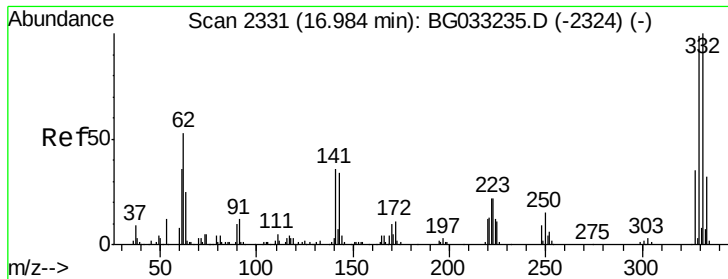




#41
 2,4,6-Tribromophenol
 Concen: 149.468 ng
 RT: 16.96 min Scan# 2326
 Delta R.T. 0.00 min
 Lab File: BG033529.D
 Acq: 3 Apr 2018 17:13

Instrument :
 BNA_G
 ClientSampleId :
 4540-2

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.0	115.6
141	38.0	25.2	37.8#

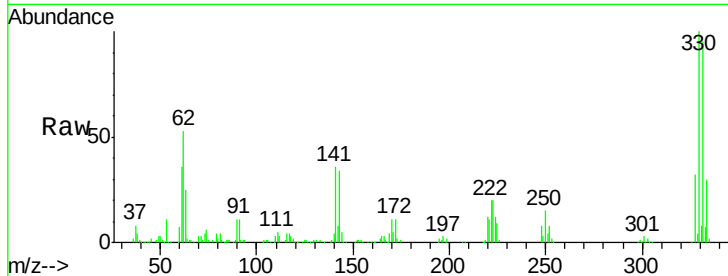


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

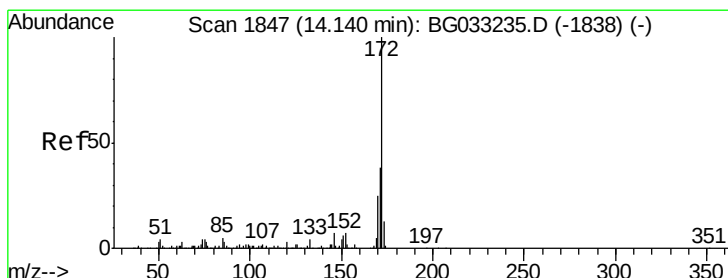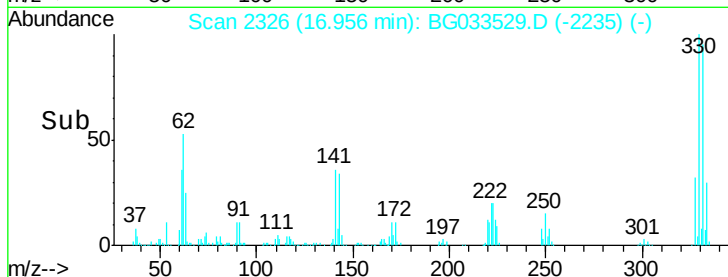
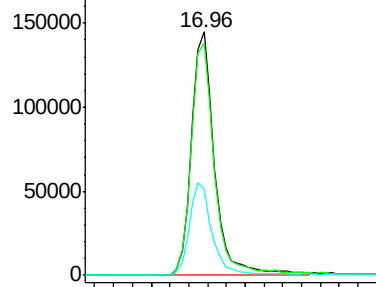



#44
 2-Fluorobiphenyl
 Concen: 108.003 ng
 RT: 14.11 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: BG033529.D
 Acq: 3 Apr 2018 17:13

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.9	30.0	45.0
170	25.6	19.5	29.3

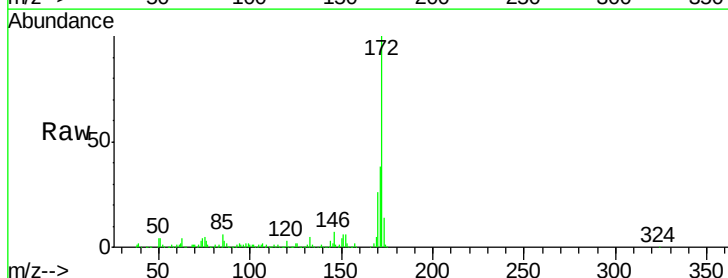

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

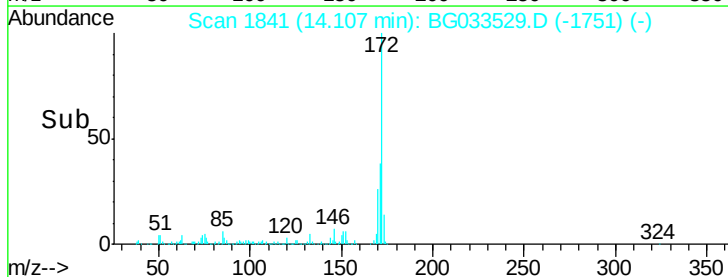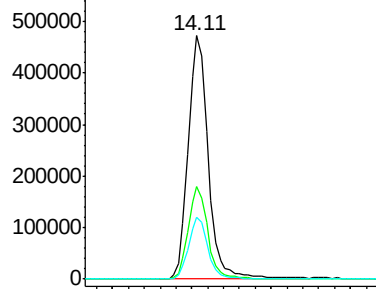

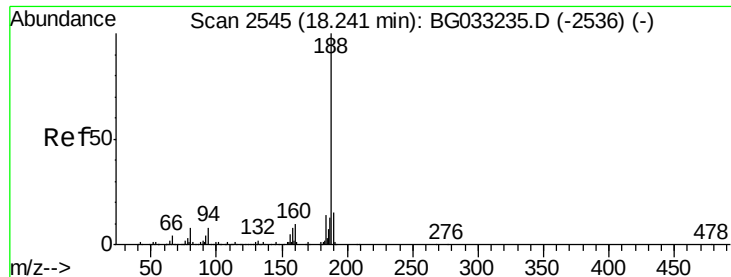

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.21 min Scan# 2539

Delta R.T. -0.00 min

Lab File: BG033529.D

Acq: 3 Apr 2018 17:13

Instrument :

BNA_G

ClientSampleId :

4540-2


Tot Ion:188 Resp: 307630

Ion Ratio Lower Upper

188 100

94 6.1 6.9 10.3#




80 8.4 7.7 11.5

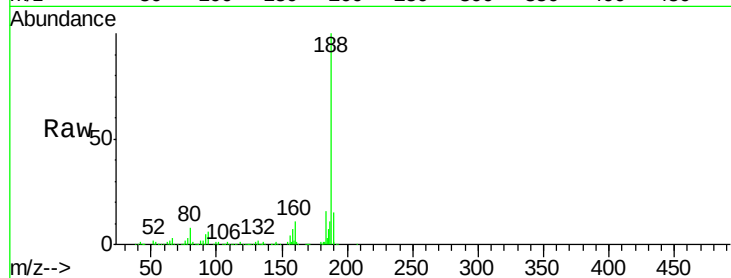

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

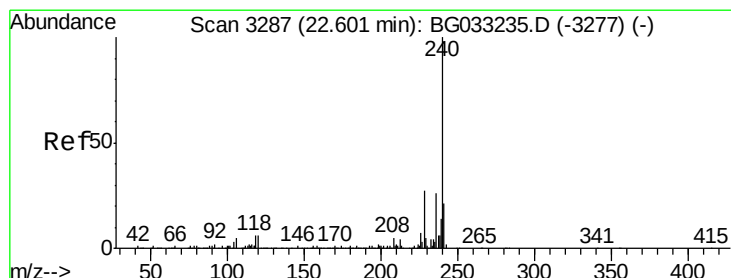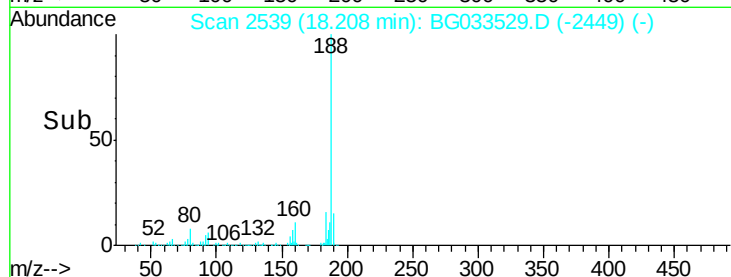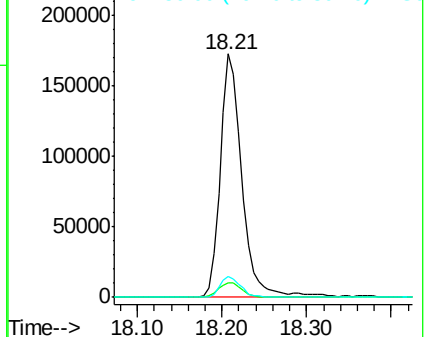

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.56 min Scan# 3279

Delta R.T. 0.00 min

Lab File: BG033529.D

Acq: 3 Apr 2018 17:13


Tgt Ion:240 Resp: 314264

Ion Ratio Lower Upper

240 100

120 7.3 6.8 10.2



236 26.1 20.9 31.3

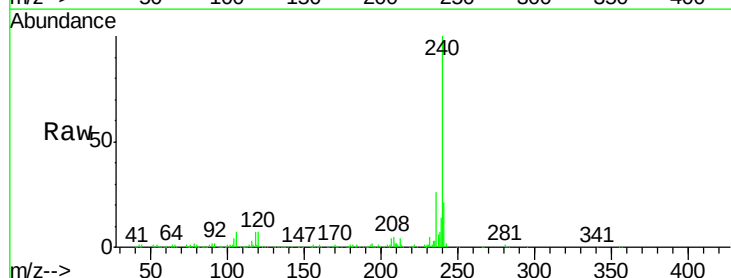


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

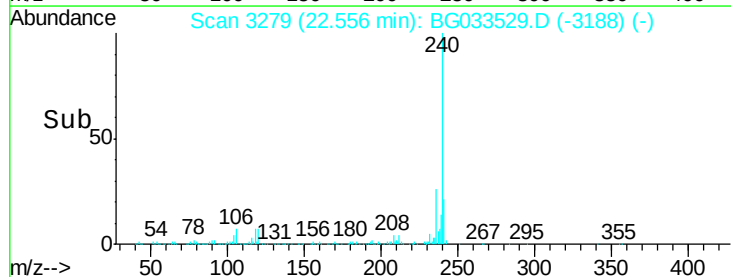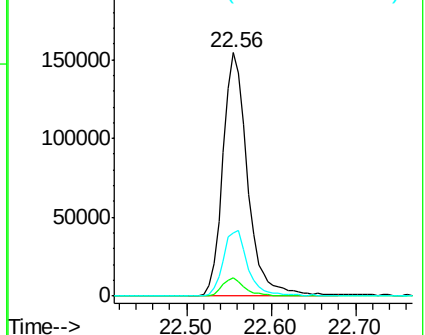

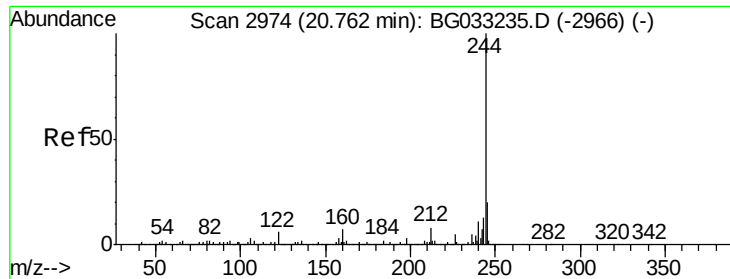

#78

Terphenyl-d14

Concen: 109.805 ng

RT: 20.73 min Scan# 2968

Delta R.T. -0.00 min

Lab File: BG033529.D

Acq: 3 Apr 2018 17:13

Instrument :

BNA_G

ClientSampleId :

4540-2


Tot Ion:244 Resp: 1613564

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#




122 7.6 7.0 10.4

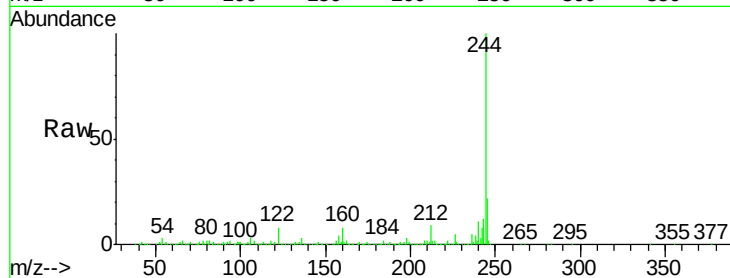

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

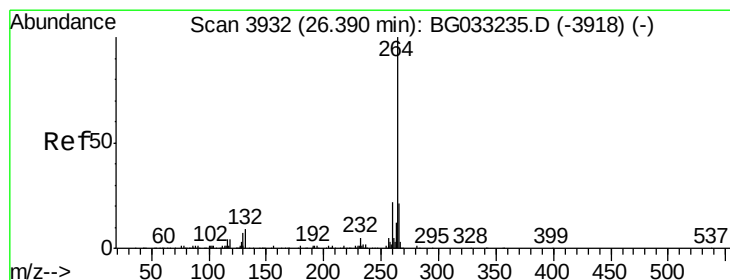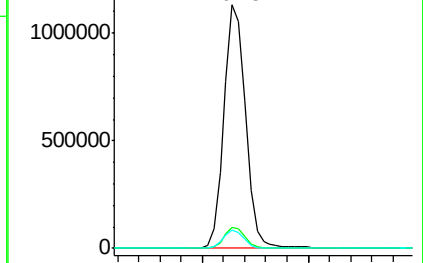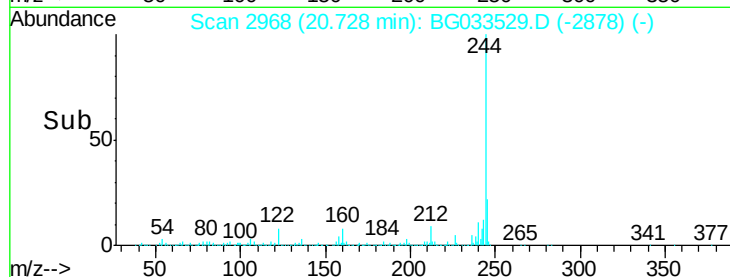

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.33 min Scan# 3921

Delta R.T. 0.01 min

Lab File: BG033529.D

Acq: 3 Apr 2018 17:13


Tgt Ion:264 Resp: 316593

Ion Ratio Lower Upper

264 100

260 21.1 17.4 26.0

265 21.9 17.7 26.5

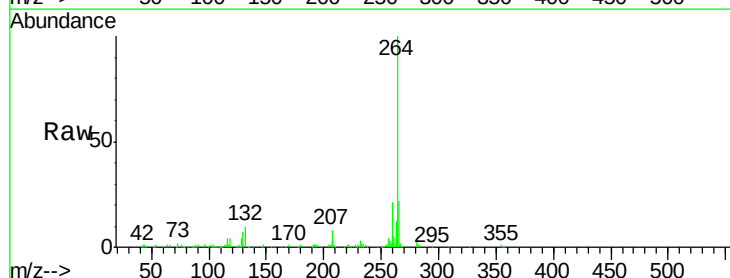

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

