


Data Path : Z:\HPCHEM1\BNA G\Data\BG040318\
 Data File : BG033515.D
 Acq On : 3 Apr 2018 8:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 03 14:50:26 2018

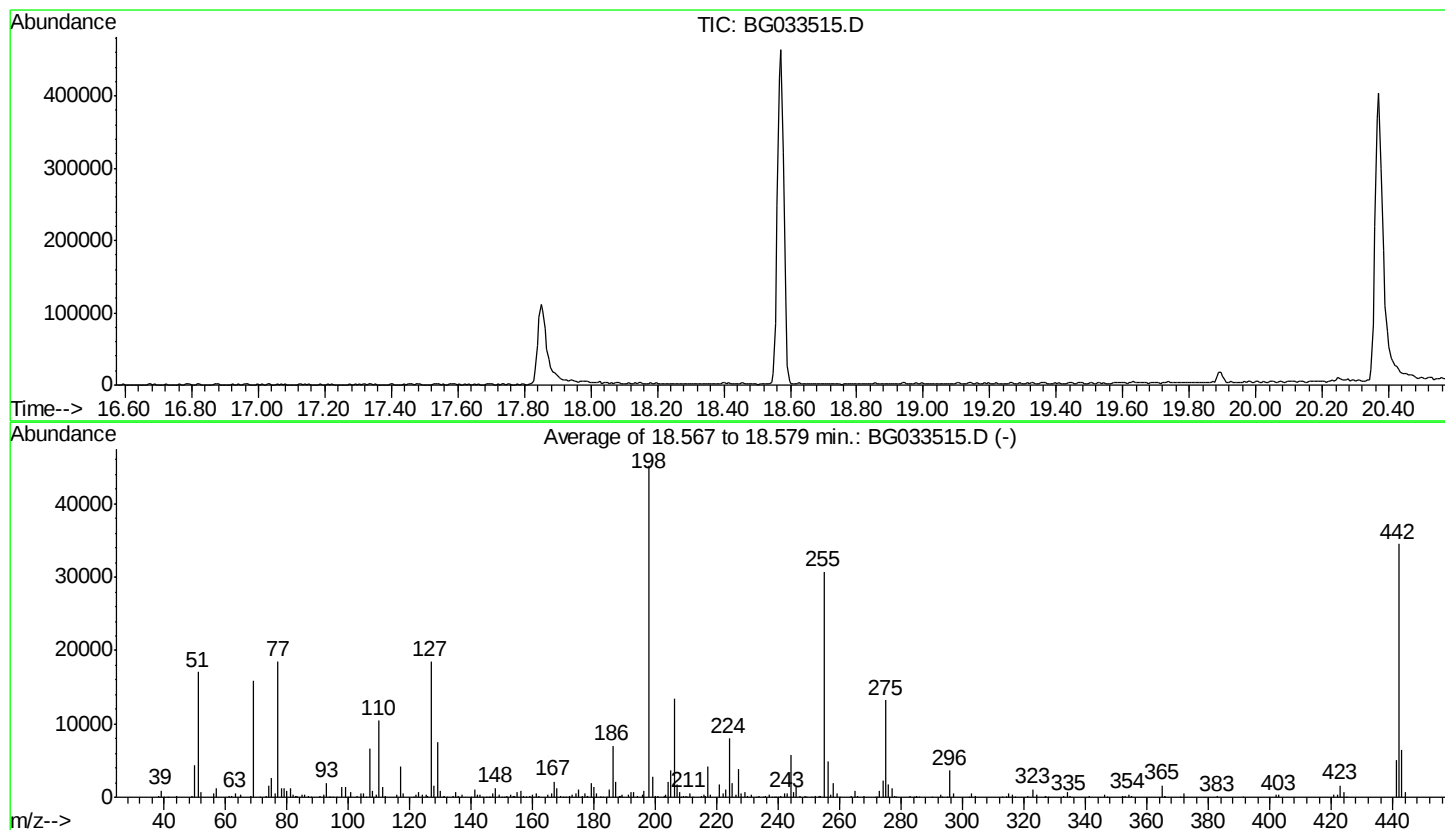

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	17071	PASS
68	69	0.00	2	0.8	133	PASS
69	198	0.00	100	35.0	15809	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	18478	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45210	PASS
199	198	5	9	6.2	2816	PASS
275	198	10	60	29.2	13192	PASS
365	198	1	100	3.5	1599	PASS
441	443	0.01	100	80.0	5134	PASS
442	198	50	100	76.4	34538	PASS
443	442	15	24	18.6	6416	PASS