
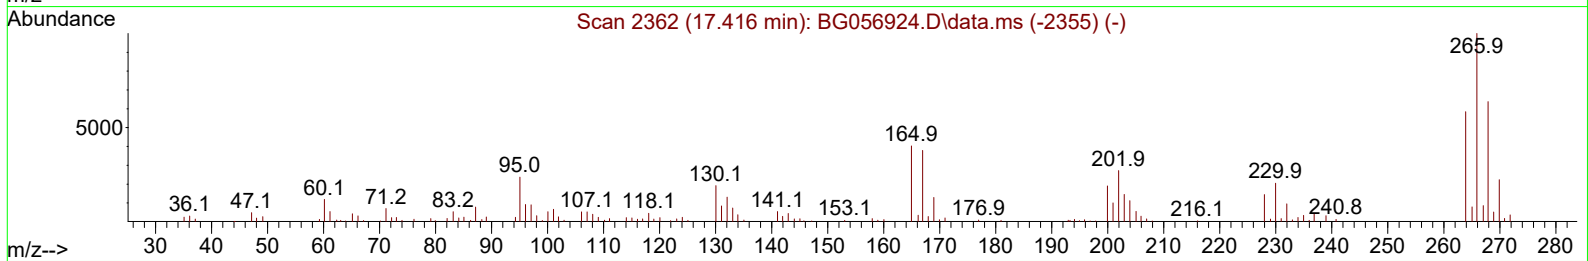
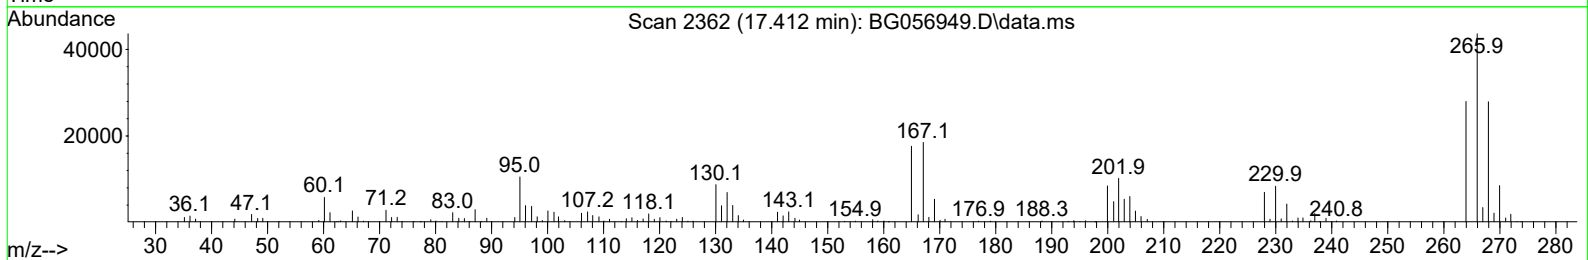


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040323\
Data File : BG056949.D
Acq On : 3 Apr 2023 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 06:47:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

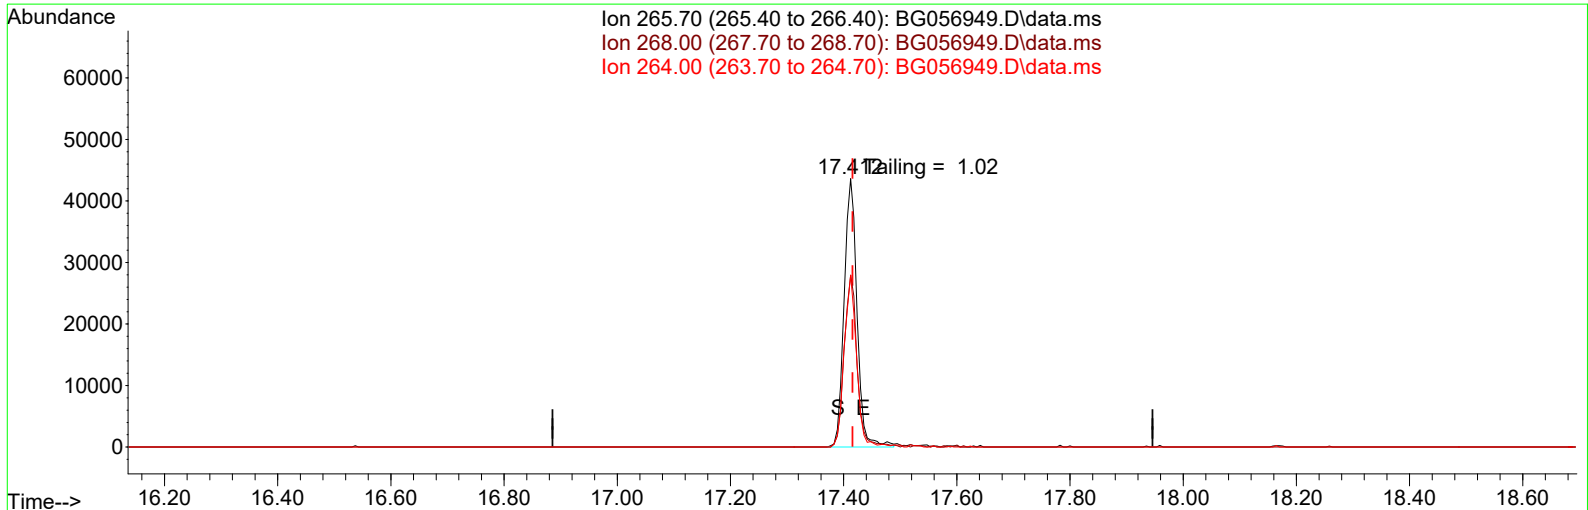

TIC: BG056949.D\data.ms

(70) Pentachlorophenol (C)




17.412min (-0.003) 138927.92 ng

response 68277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.99
264.00	58.50	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040323\
 Data File : BG056949.D
 Acq On : 3 Apr 2023 9:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 06:47:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 03:23:11 2023
 Response via : Initial Calibration

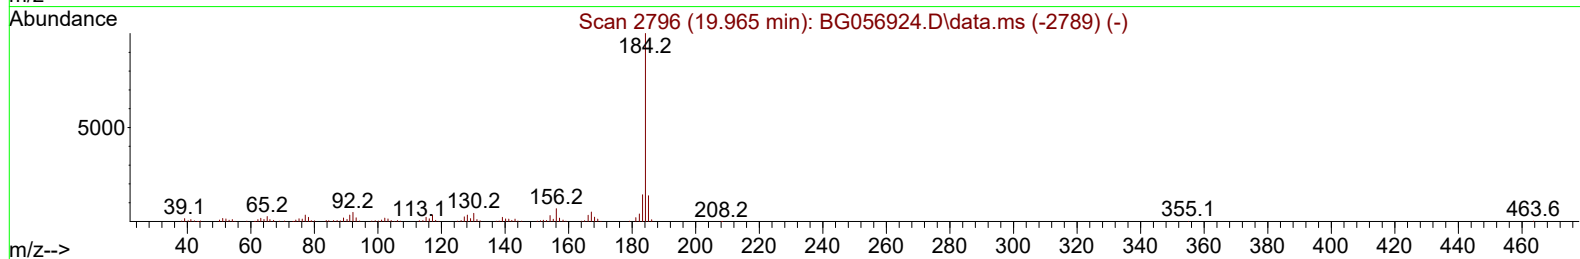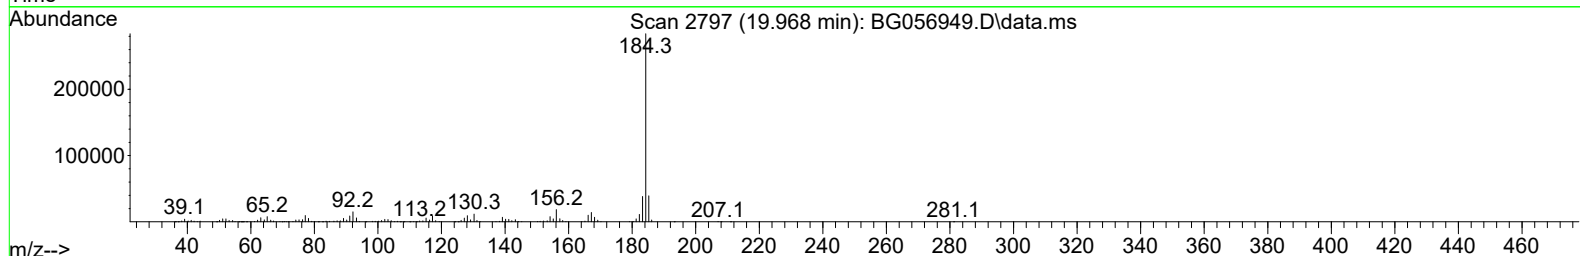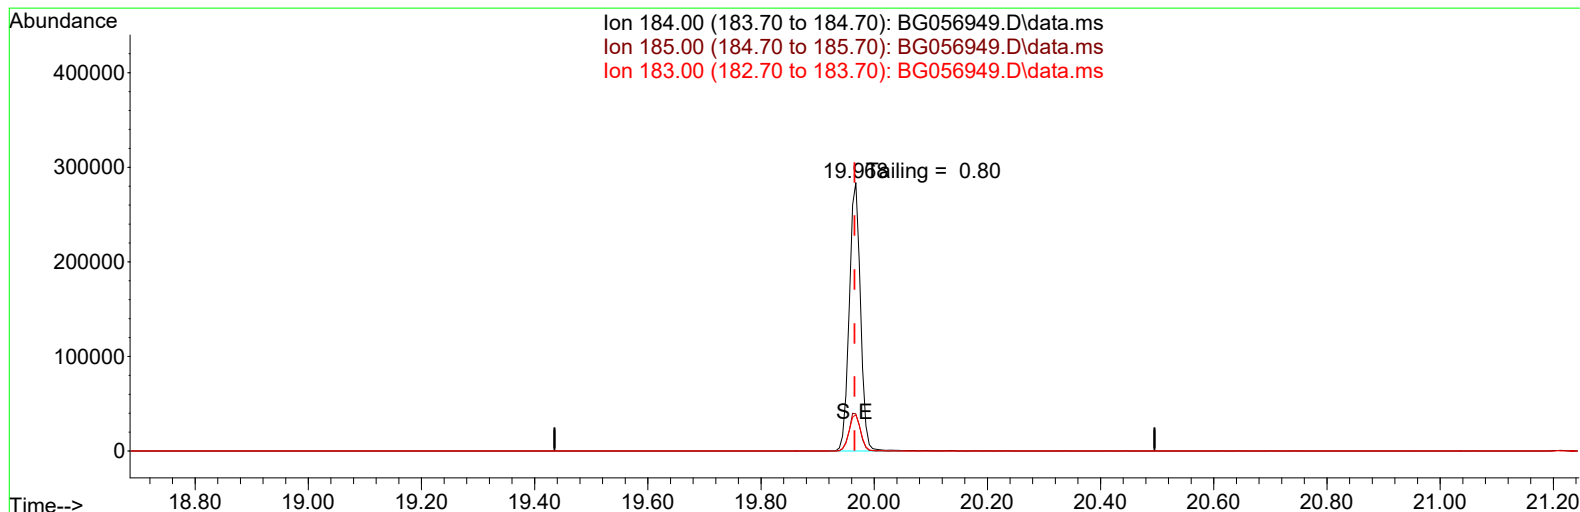

TIC: BG056949.D\data.ms

(77) Benzidine**19.968min (+ 0.003) 100088.10 ng****response 391210**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.86
183.00	14.20	13.49
0.00	0.00	0.00