


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040323\
Data File : BG056949.D
Acq On : 3 Apr 2023 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 03:23:11 2023

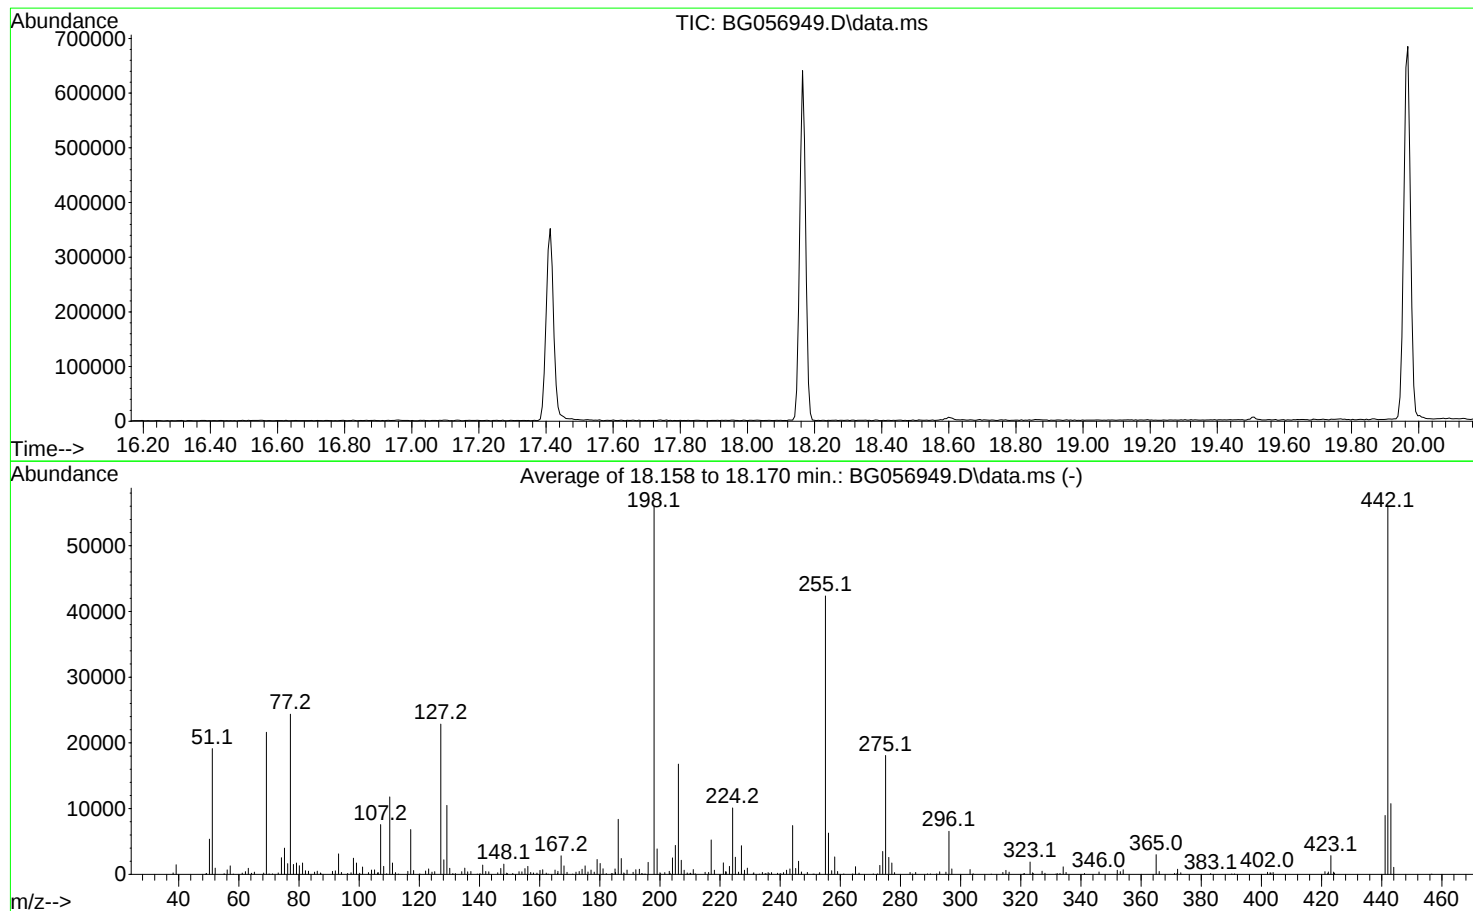




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	19144	PASS
68	69	0.00	2	0.9	190	PASS
69	198	0.00	100	38.6	21627	PASS
70	69	0.00	2	0.3	64	PASS
127	198	10	80	40.8	22859	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55960	PASS
199	198	5	9	6.9	3878	PASS
275	198	10	60	32.3	18090	PASS
365	198	1	100	5.3	2989	PASS
441	198	0.01	100	16.0	8958	PASS
442	442	50	100	100.0	55869	PASS
443	442	15	24	19.3	10768	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040323\
Data File : BG056949.D
Acq On : 3 Apr 2023 9:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 04 06:47:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

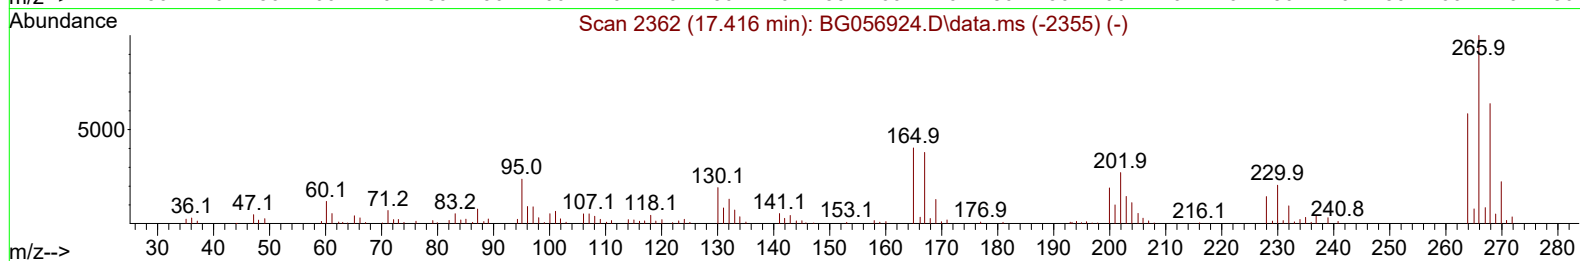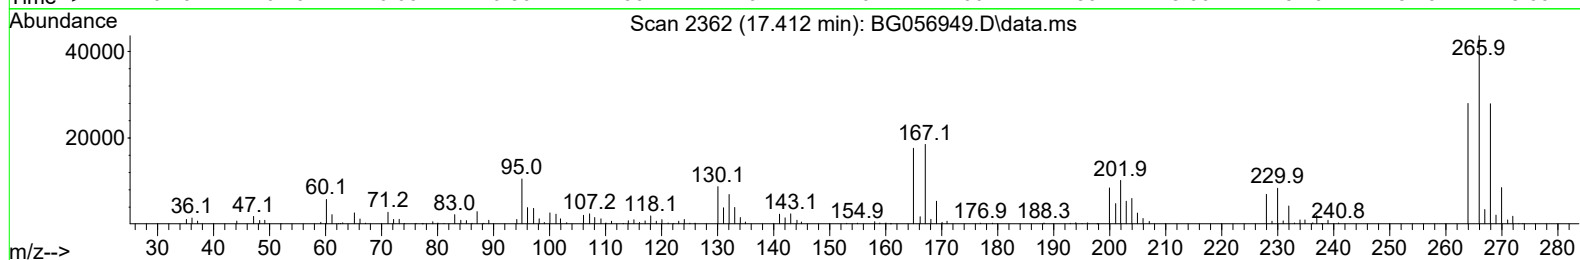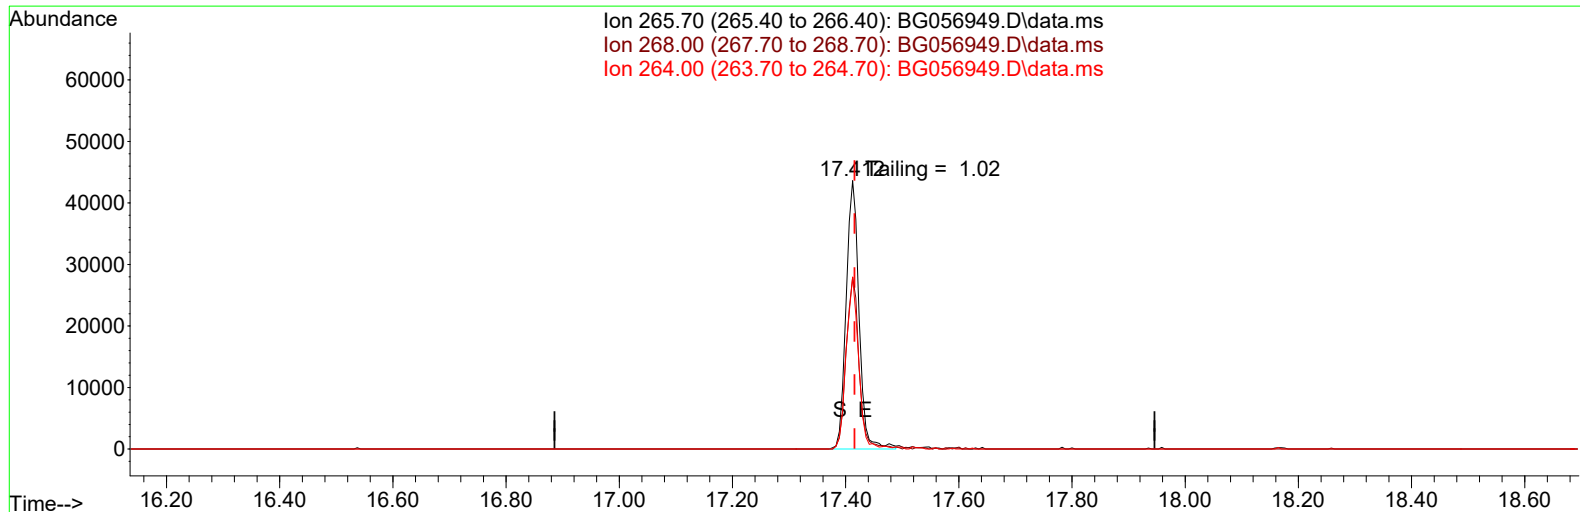

TIC: BG056949.D\data.ms

(70) Pentachlorophenol (C)

17.412min (-0.003) 138927.92 ng




response 68277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.99
264.00	58.50	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040323\
 Data File : BG056949.D
 Acq On : 3 Apr 2023 9:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 04 06:47:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 03:23:11 2023
 Response via : Initial Calibration

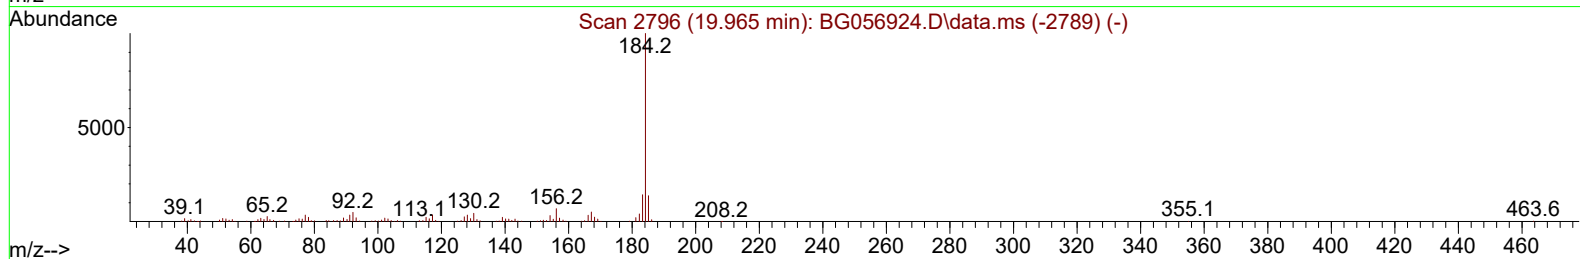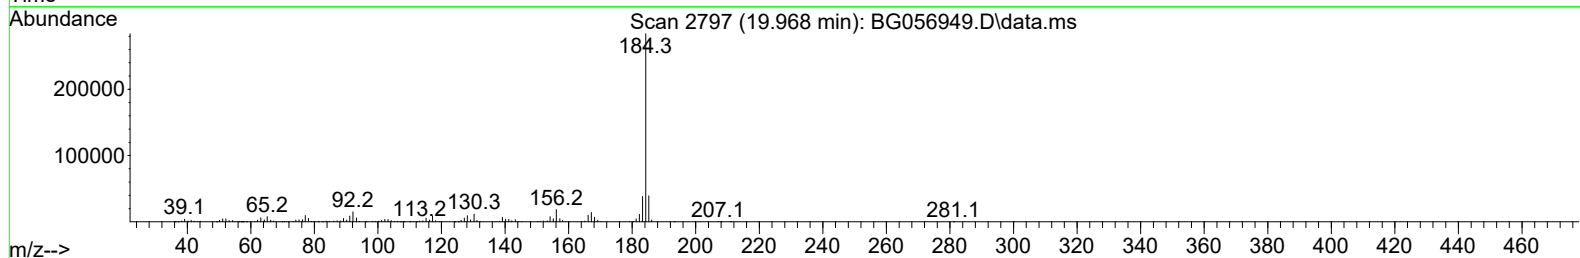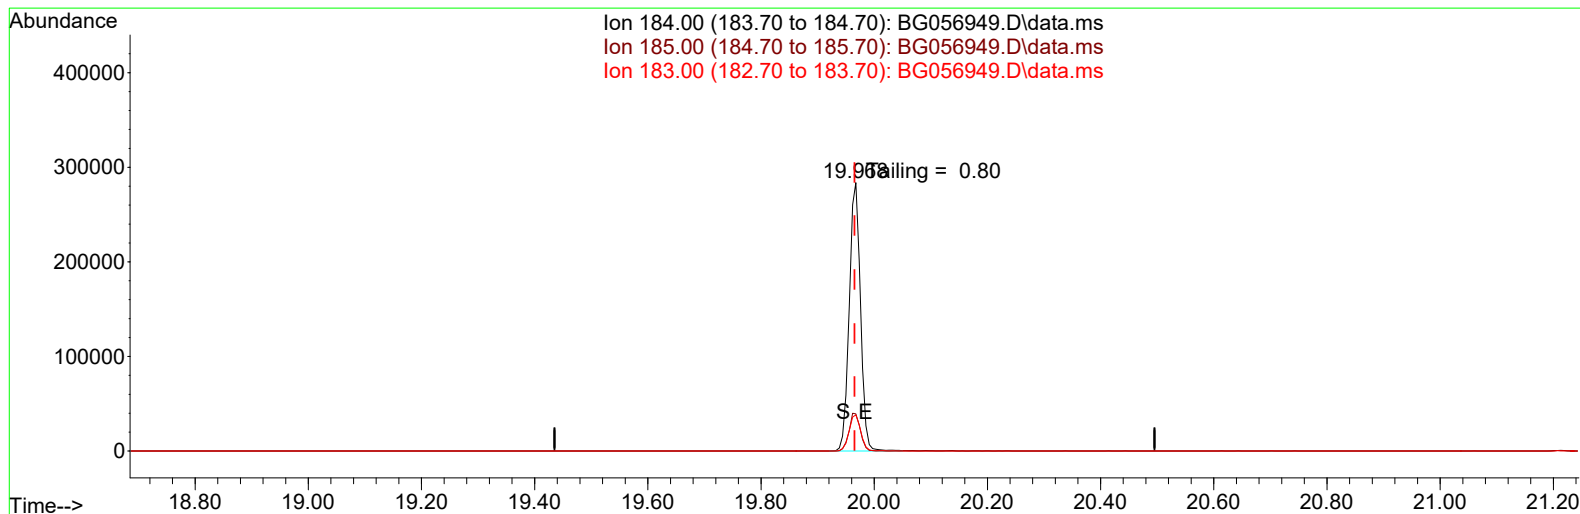

TIC: BG056949.D\data.ms

(77) Benzidine**19.968min (+ 0.003) 100088.10 ng****response 391210**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.86
183.00	14.20	13.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2023	BNA_G	BG056949.D
Compound Name	Response	Retention Time
DDT	184354	21.213
DDD	3793	20.749
DDE	111	20.232
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3904	188258	2.07

Instrument :
BNA_G
ClientSampleId :
DFTPP