
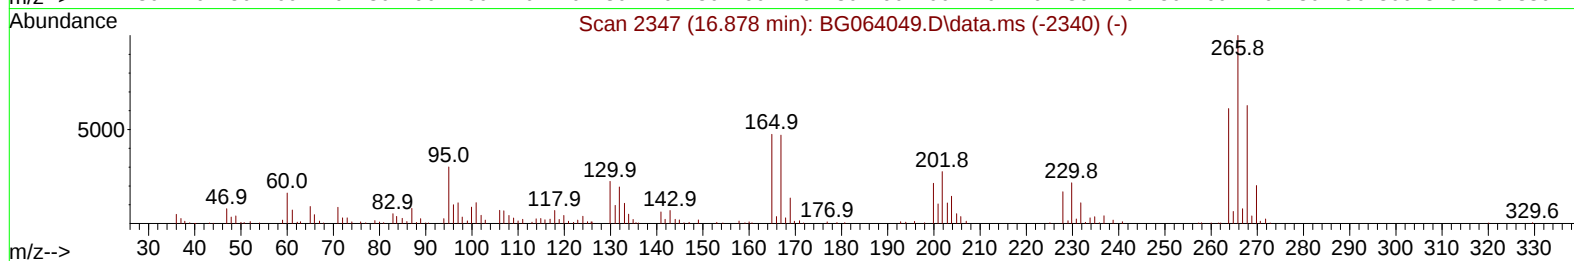
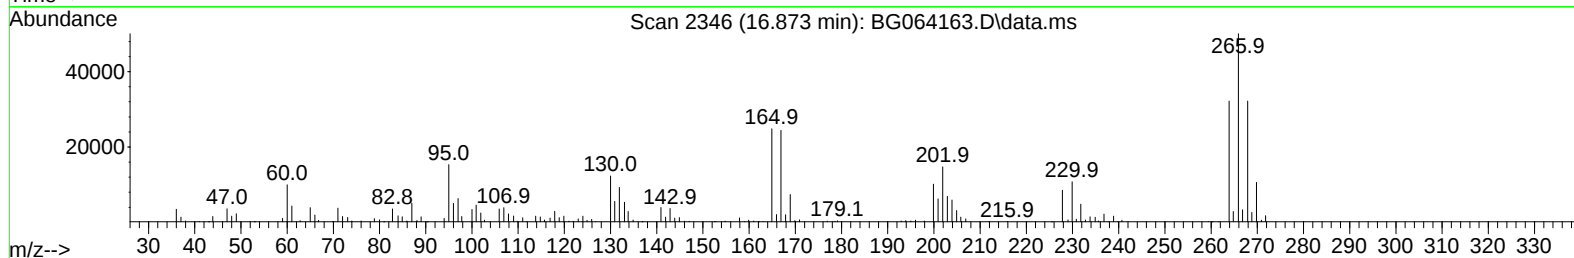


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064163.D
Acq On : 3 Apr 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 13:51:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

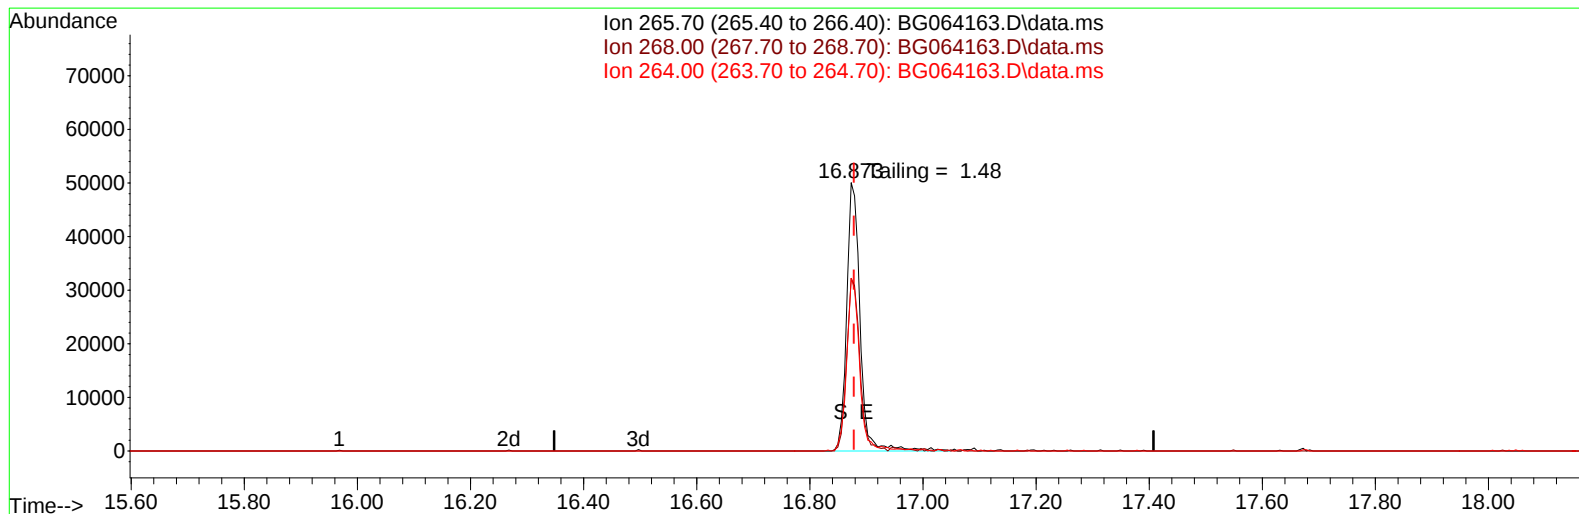

TIC: BG064163.D\data.ms

(70) Pentachlorophenol (C)




16.873min (-0.005) 143328.78 ng m

response 82652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	64.32
264.00	61.10	64.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064163.D
Acq On : 3 Apr 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 13:51:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

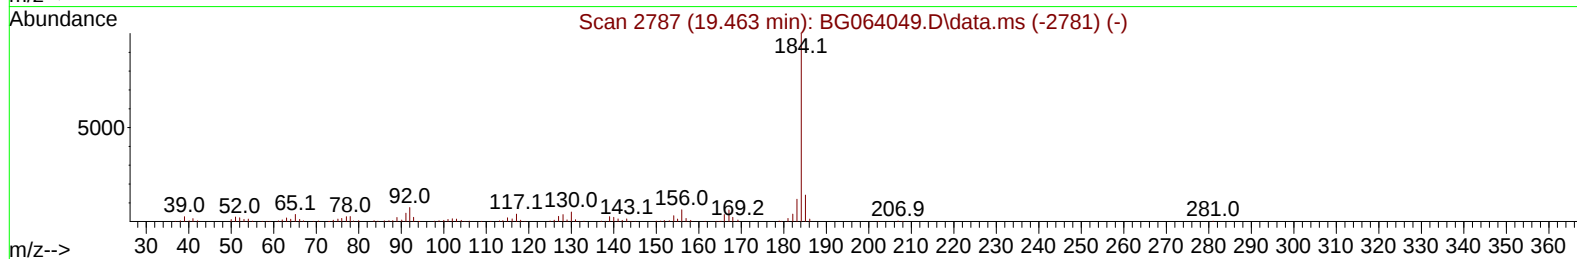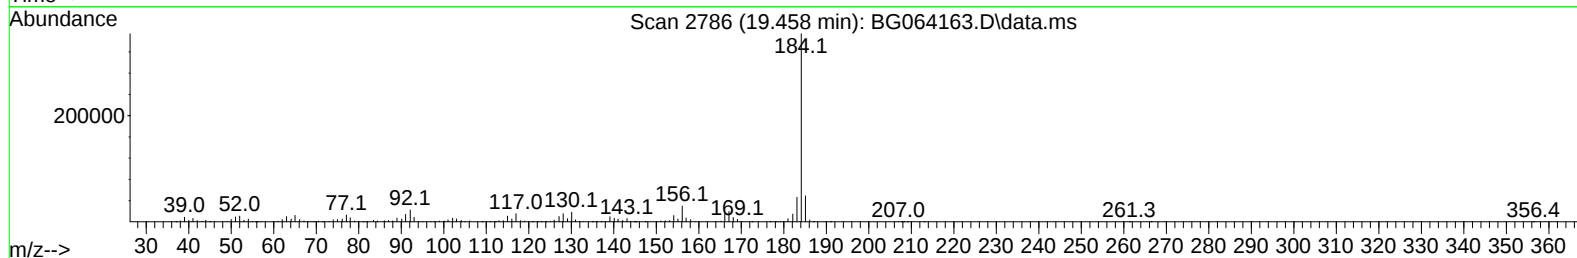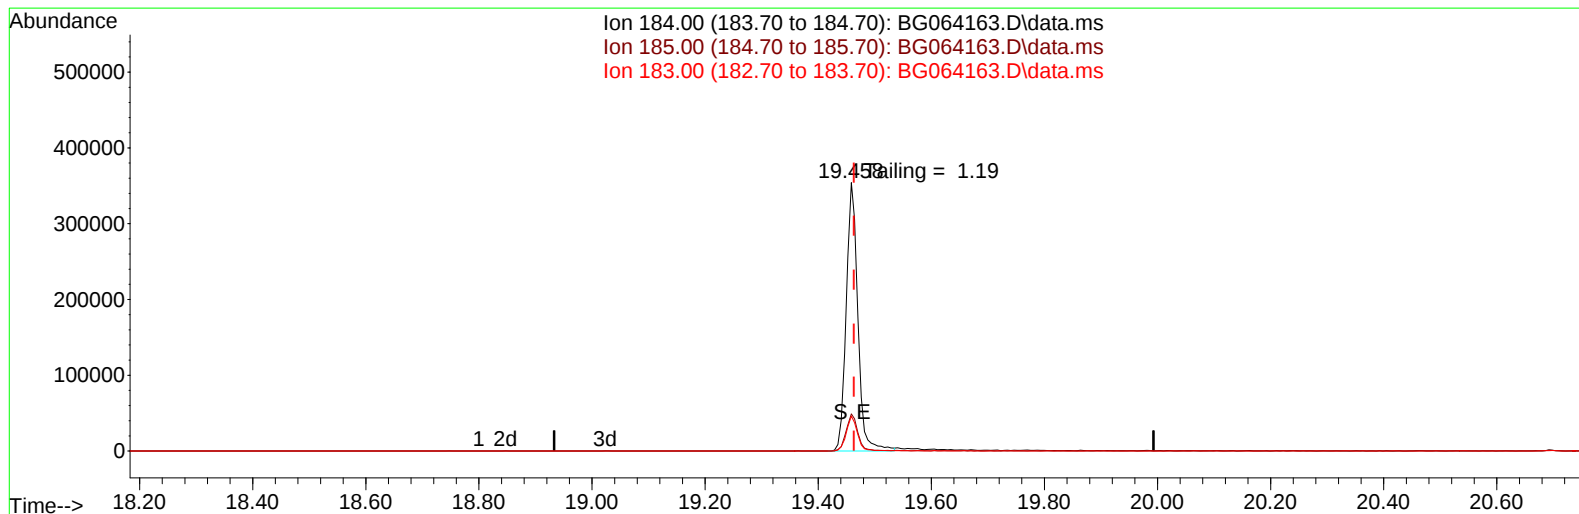

TIC: BG064163.D\data.ms

(77) Benzidine

19.458min (-0.005) 9423.30 ng m

response 527163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.84
183.00	11.90	13.02
0.00	0.00	0.00