
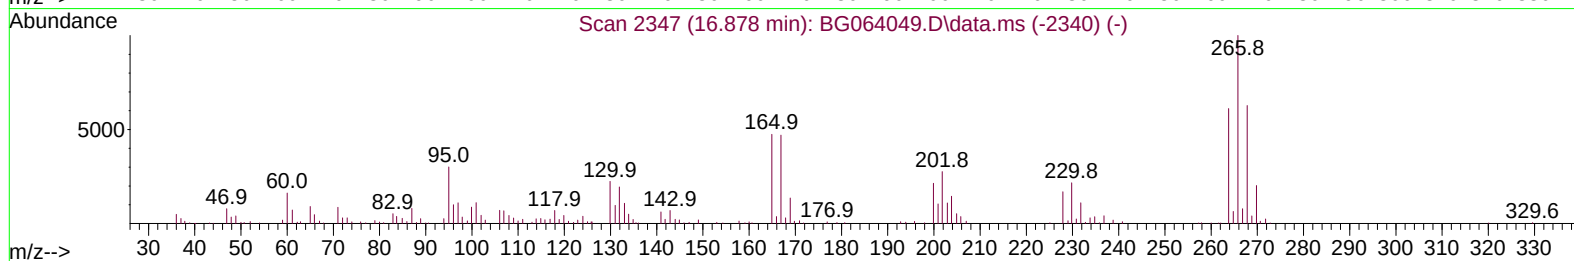
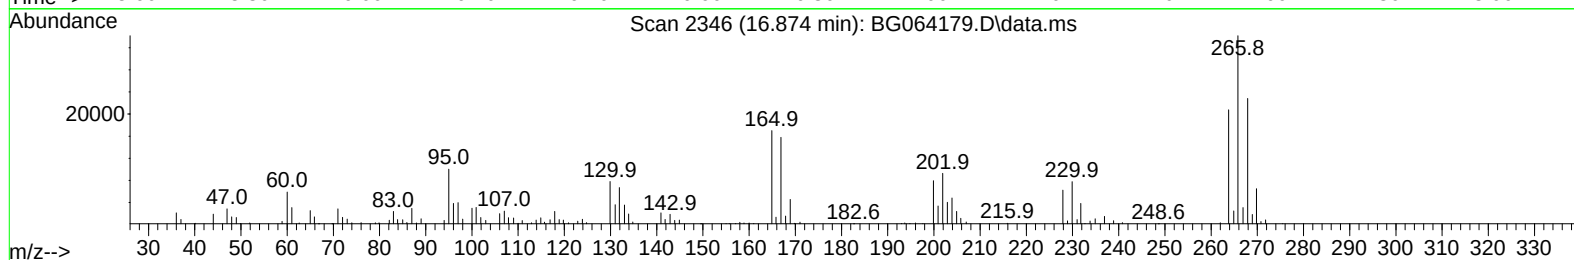


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\  
Data File : BG064179.D  
Acq On    : 3 Apr 2025 23:21  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Apr 04 02:44:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

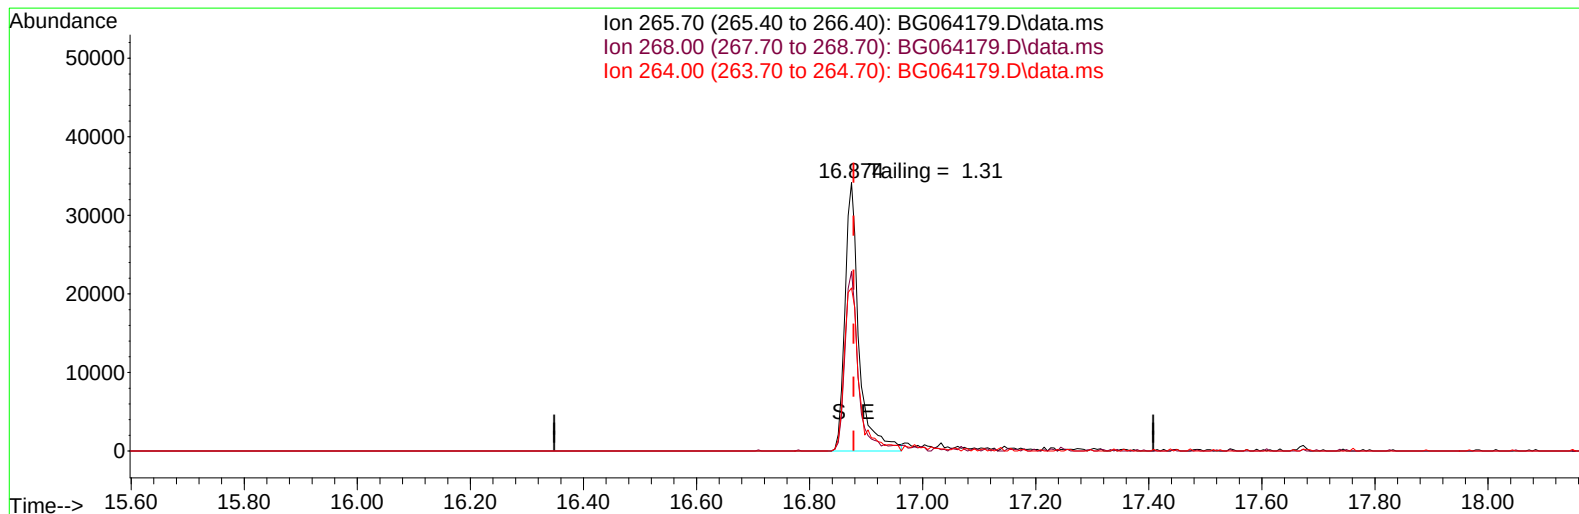

TIC: BG064179.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.004) 11250.31 ng

response **58869**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	66.82
264.00	61.10	60.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064179.D
Acq On : 3 Apr 2025 23:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 02:44:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

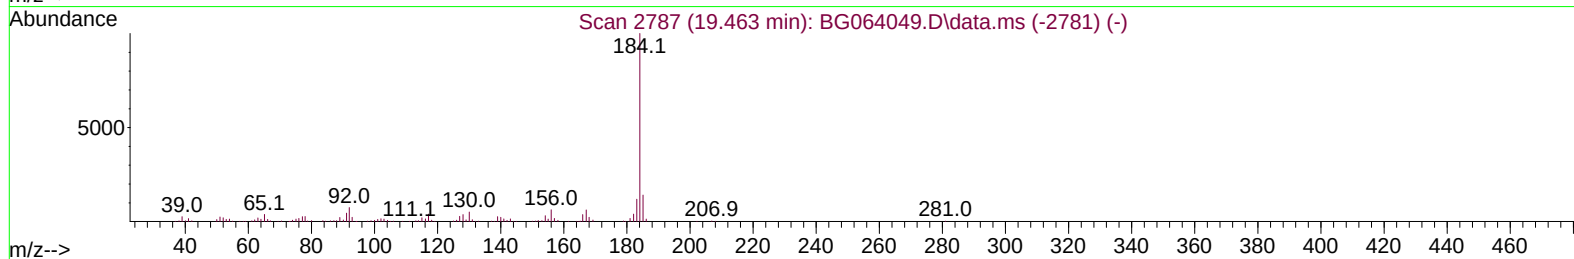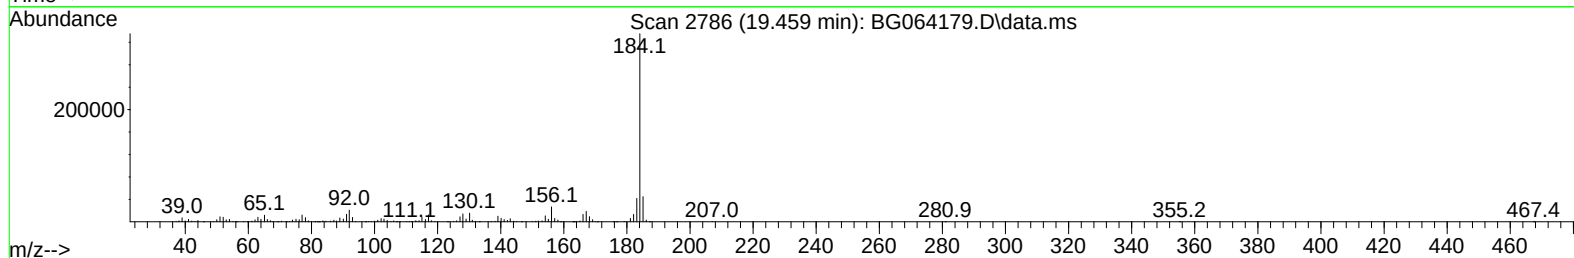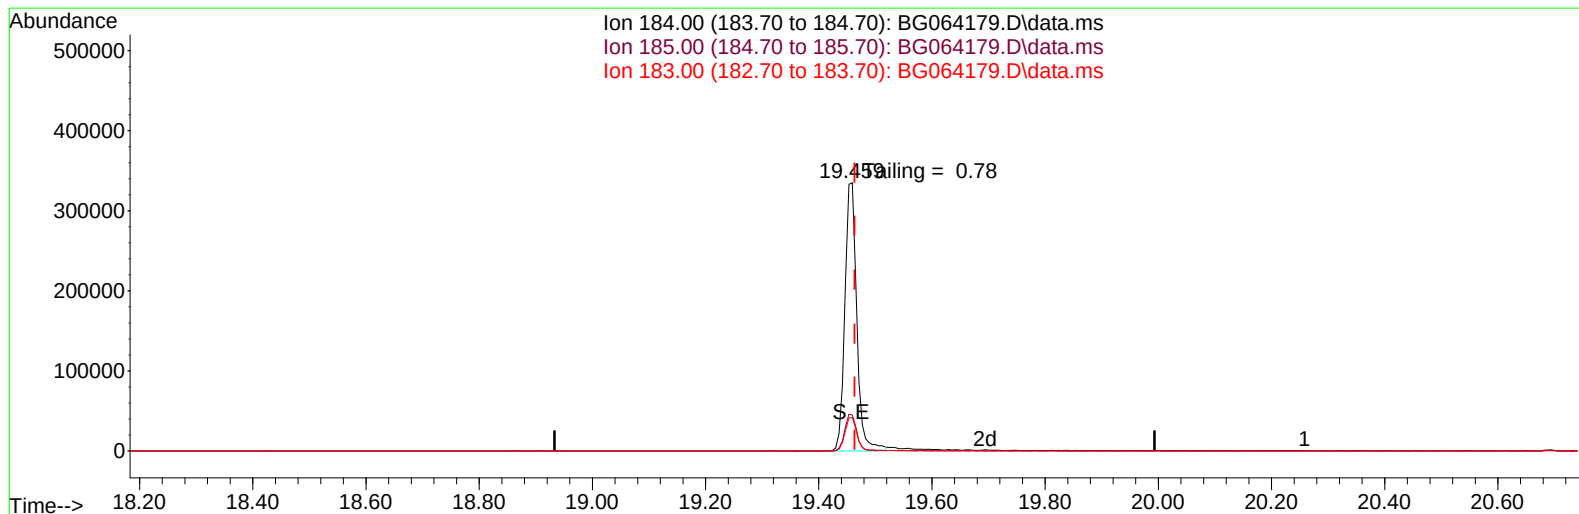

TIC: BG064179.D\data.ms

(77) Benzidine

19.459min (-0.004) 641088.64 ng m

response 497126

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.43
183.00	11.90	12.45
0.00	0.00	0.00