
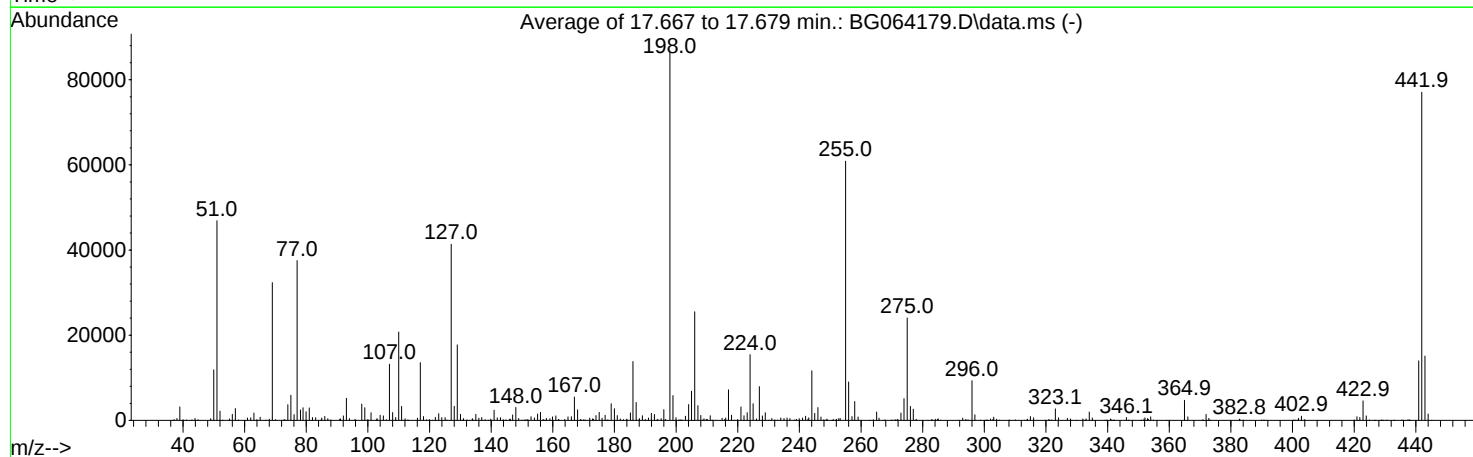


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064179.D
Acq On : 3 Apr 2025 23:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

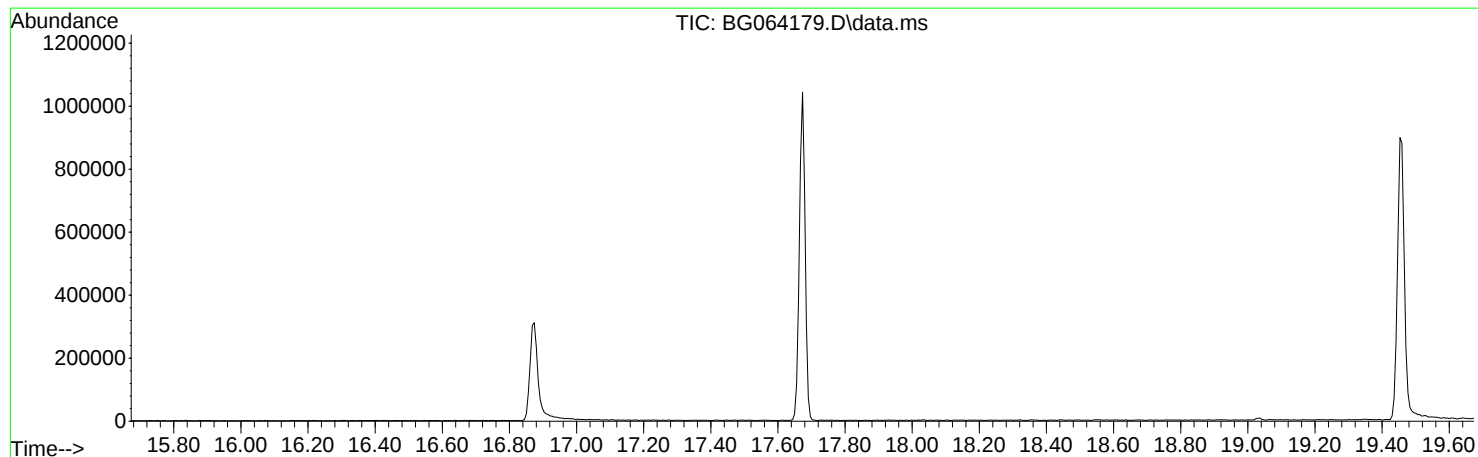




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	46909	PASS
68	69	0.00	2	1.0	316	PASS
69	198	0.00	100	37.5	32360	PASS
70	69	0.00	2	0.6	187	PASS
127	198	10	80	47.9	41387	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86392	PASS
199	198	5	9	6.8	5835	PASS
275	198	10	60	27.9	24064	PASS
365	198	1	100	5.4	4701	PASS
441	198	0.01	100	16.2	13982	PASS
442	442	50	100	100.0	77088	PASS
443	442	15	24	19.6	15115	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\  
Data File : BG064179.D  
Acq On    : 3 Apr 2025 23:21  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 04 02:44:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

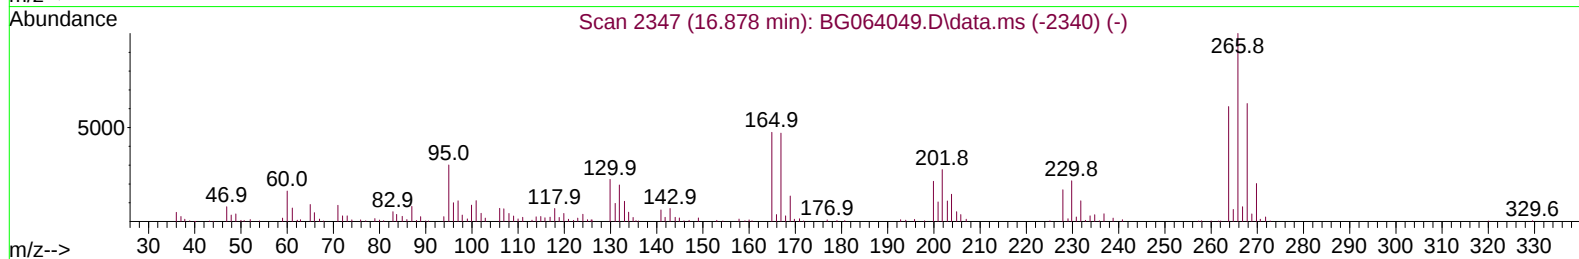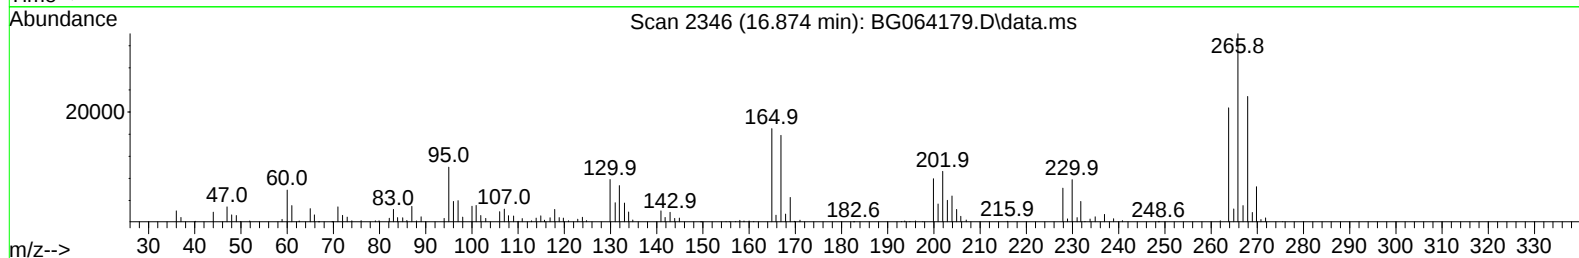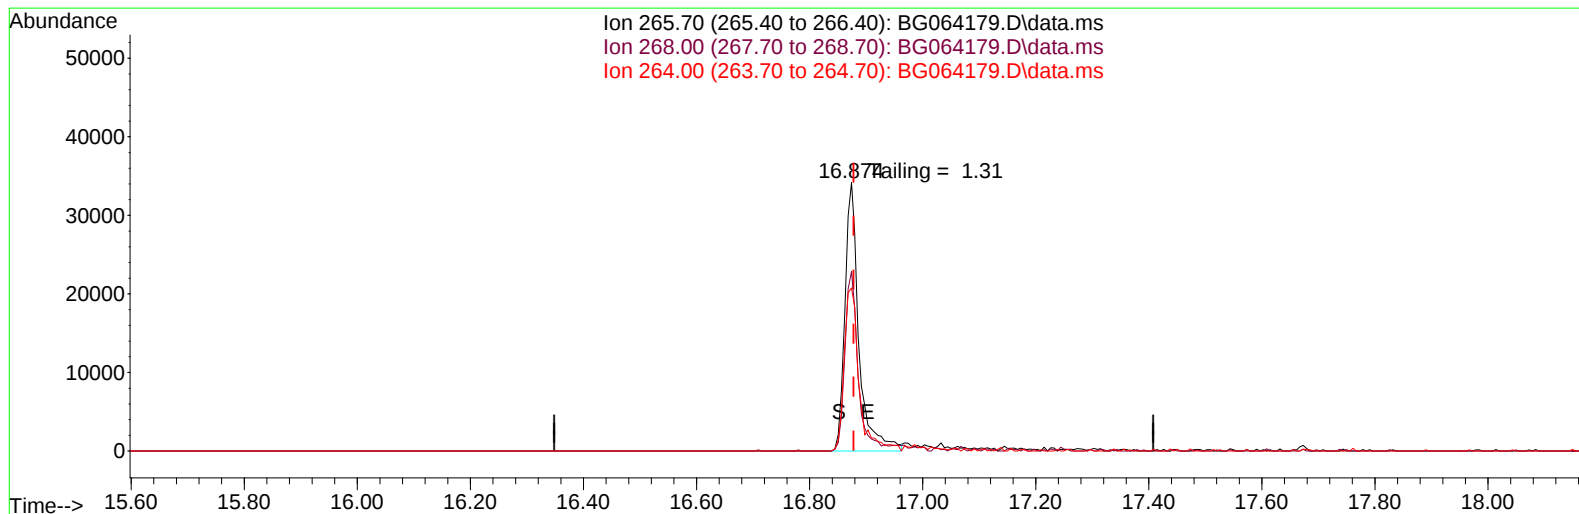

TIC: BG064179.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.004) 11250.31 ng




response **58869**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	66.82
264.00	61.10	60.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064179.D
Acq On : 3 Apr 2025 23:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 04 02:44:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

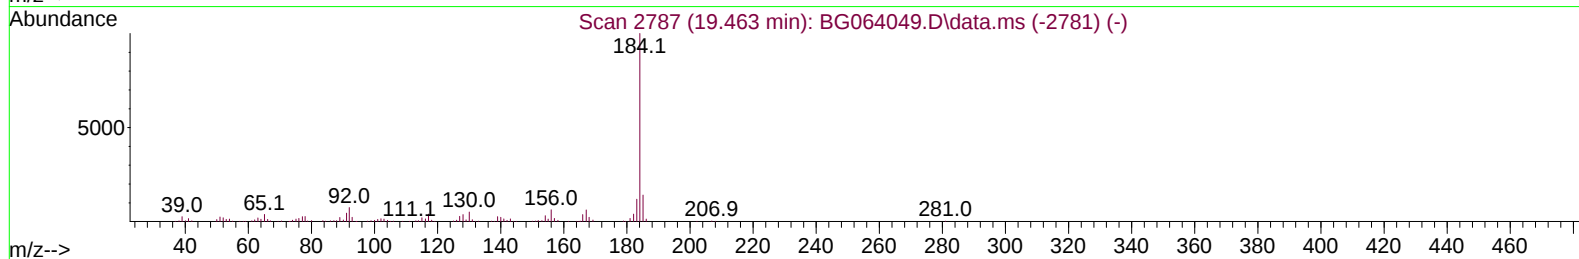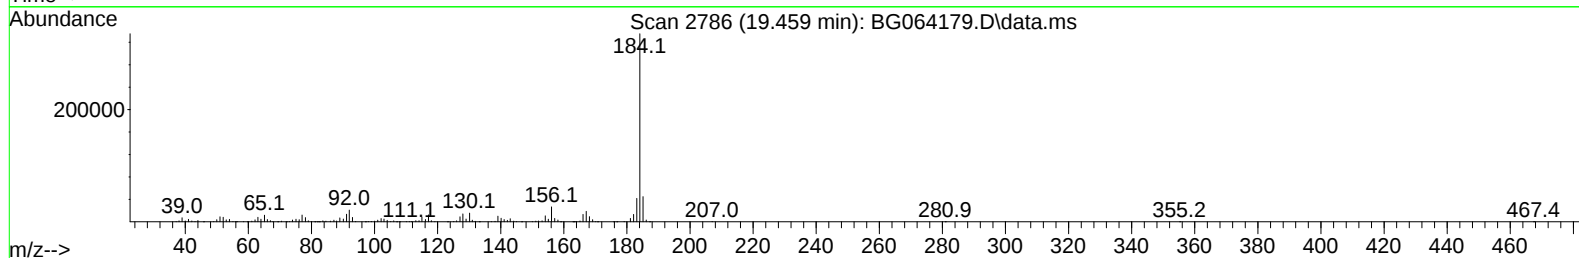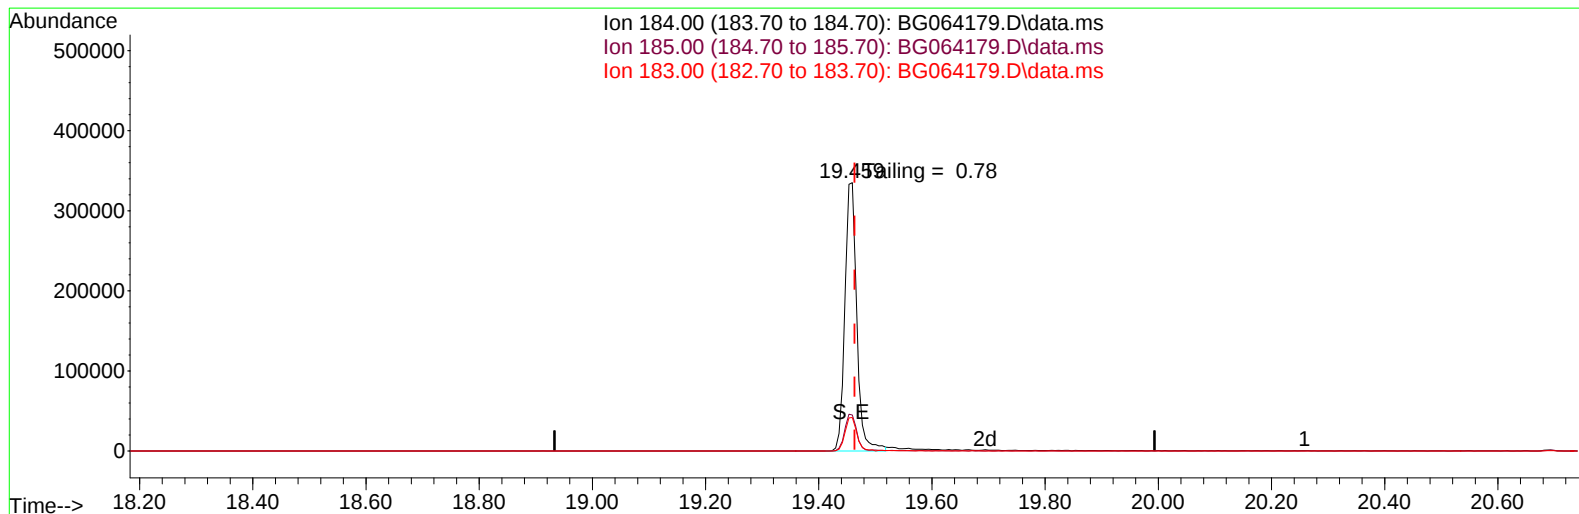

TIC: BG064179.D\data.ms

(77) Benzidine

19.459min (-0.004) 641088.64 ng m

response 497126

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.43
183.00	11.90	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2025	BNA_G	<u>BG064179.D</u>
Compound Name	Response	Retention Time
DDT	263327	20.693
DDD	9632	20.252
DDE	3585	19.753
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13217	276544	4.78

Instrument :
BNA_G
ClientSampleId :
DFTPP