
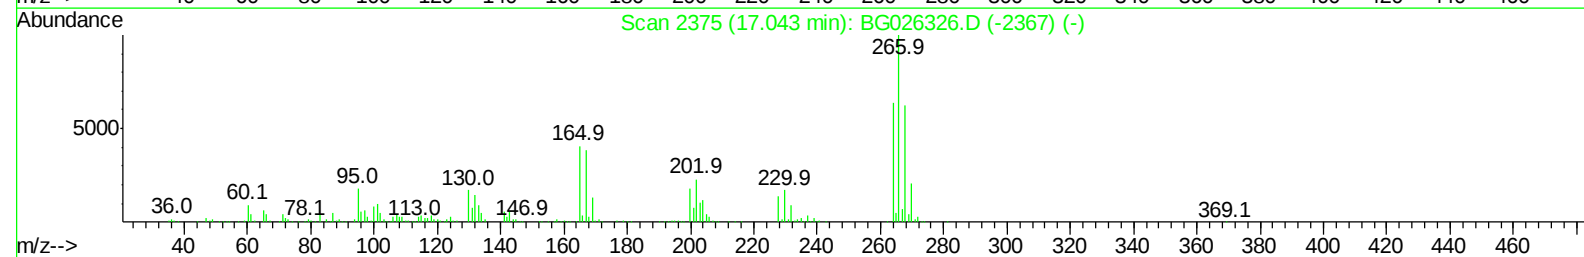
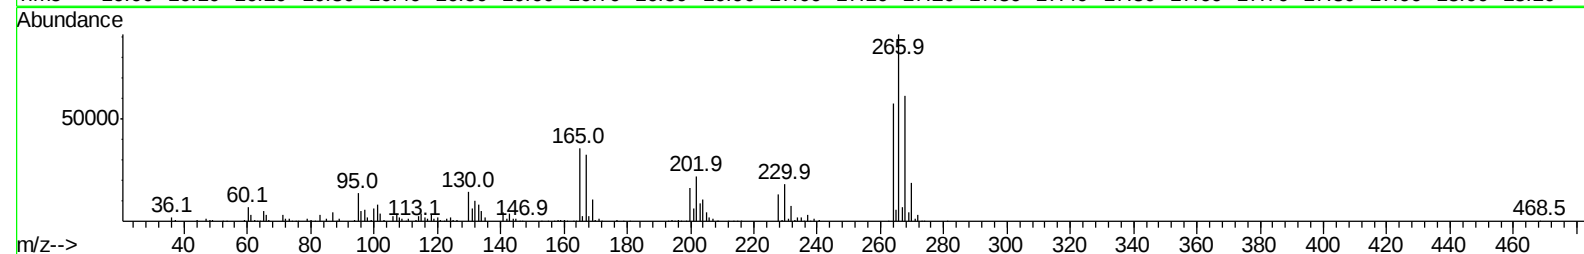


Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
Data File : BG026543.D
Acq On : 4 Apr 2017 14:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 05:30:19 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

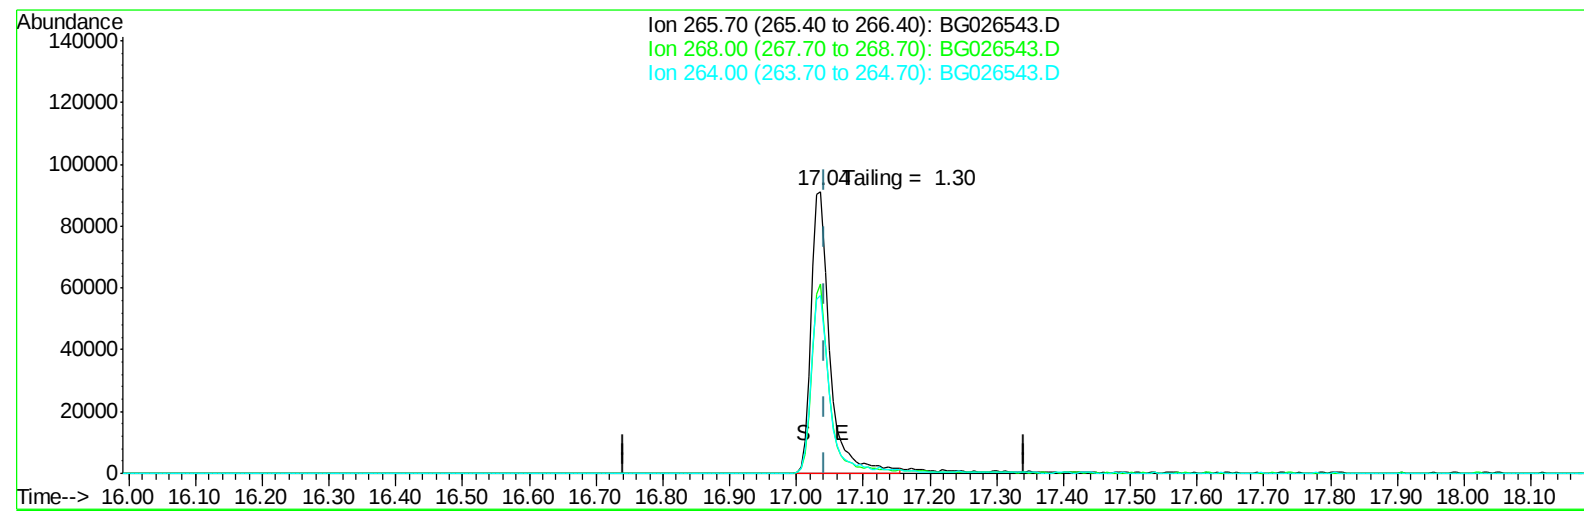

TIC: BG026543.D

(69) Pentachlorophenol (C)




17.037min (-0.006) 0.00ng

response 176404

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	67.33
264.00	62.60	63.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
 Data File : BG026543.D
 Acq On : 4 Apr 2017 14:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 05:30:19 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 17:43:27 2017
 Response via : Initial Calibration

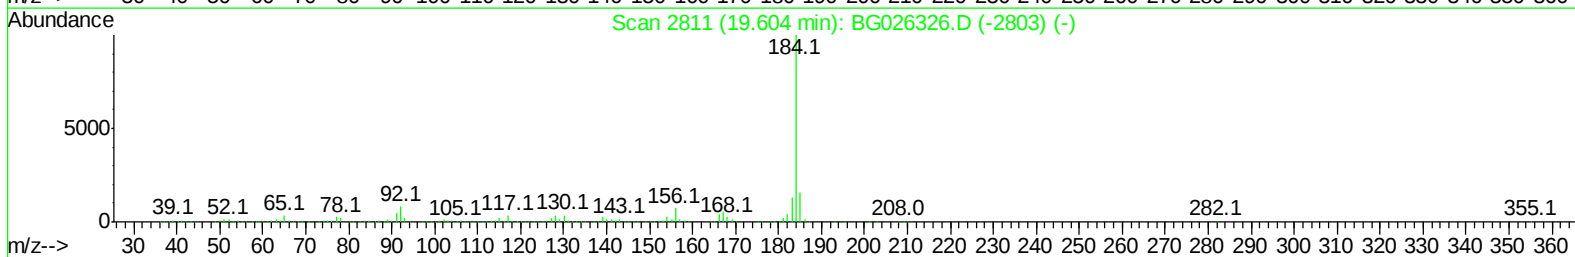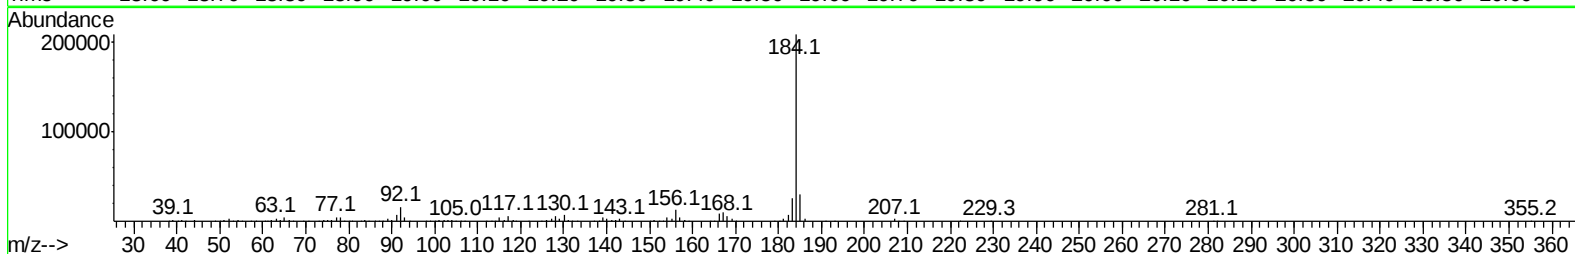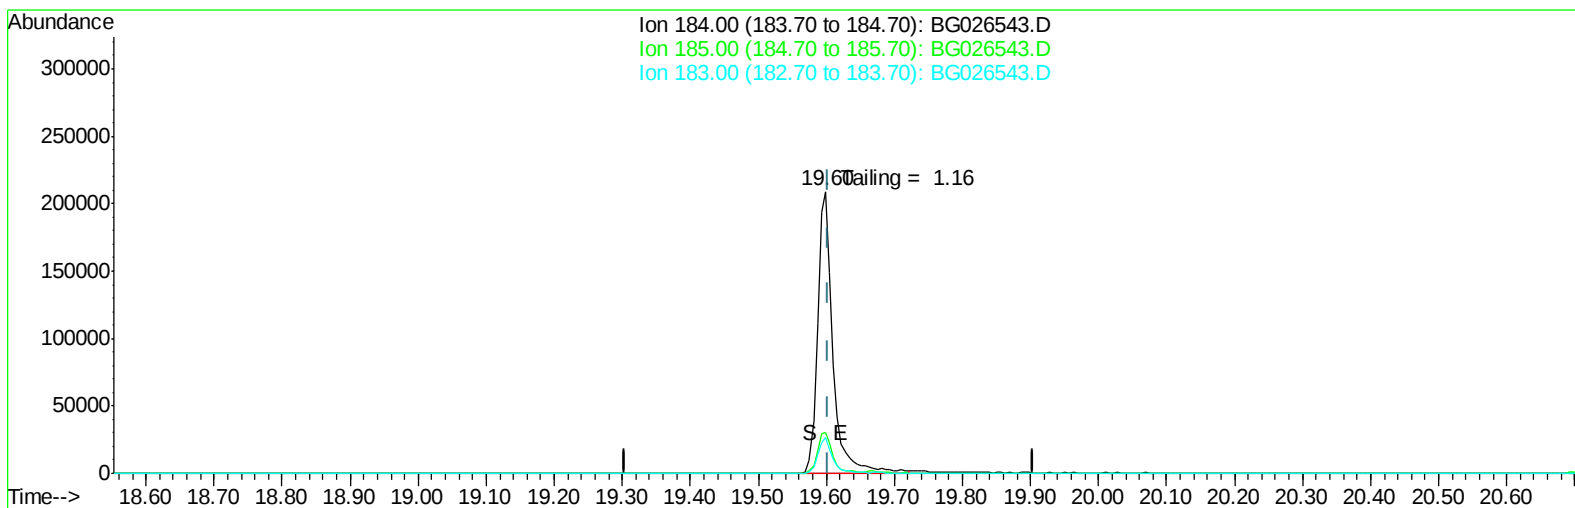

TIC: BG026543.D

(76) Benzidine

19.599min (-0.006) 11349.40ng

response 329091

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.38
183.00	13.80	12.65
0.00	0.00	0.00