

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
Data File : BG026549.D
Acq On : 4 Apr 2017 18:36
Operator : SJ/MA
Sample : I2484-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
033017-PRRT-F-D-M

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.613	423	430	444	rBV	652284	1075607	10.98%	2.748%
2	7.205	694	701	712	rBV	365627	682603	6.97%	1.744%
3	7.575	756	764	777	rBV	1213719	2106291	21.50%	5.382%
4	8.040	834	843	855	rBV	457407	794295	8.11%	2.030%
5	8.363	890	898	909	rBV	1727998	3028157	30.91%	7.738%
6	9.197	1033	1040	1053	rBV	1259020	2255808	23.03%	5.764%
7	10.842	1309	1320	1329	rBV	610558	1137241	11.61%	2.906%
8	13.275	1726	1734	1747	rBV	3977355	6246357	63.77%	15.961%
9	14.644	1961	1967	1978	rBV2	927430	1546445	15.79%	3.952%
10	16.124	2212	2219	2235	rBV	1997956	3026861	30.90%	7.734%
11	17.382	2426	2433	2445	rBV	1242655	1982263	20.24%	5.065%
12	19.978	2868	2875	2888	rBV	7401794	9795454	100.00%	25.030%
13	21.624	3149	3155	3165	rBV	1663282	2692373	27.49%	6.880%
14	24.802	3685	3696	3711	rBV	978835	2765248	28.23%	7.066%


Sum of corrected areas: 39135003

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
Data File : BG026549.D
Acq On : 4 Apr 2017 18:36
Operator : SJ/MA
Sample : I2484-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
033017-PRRT-F-D-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

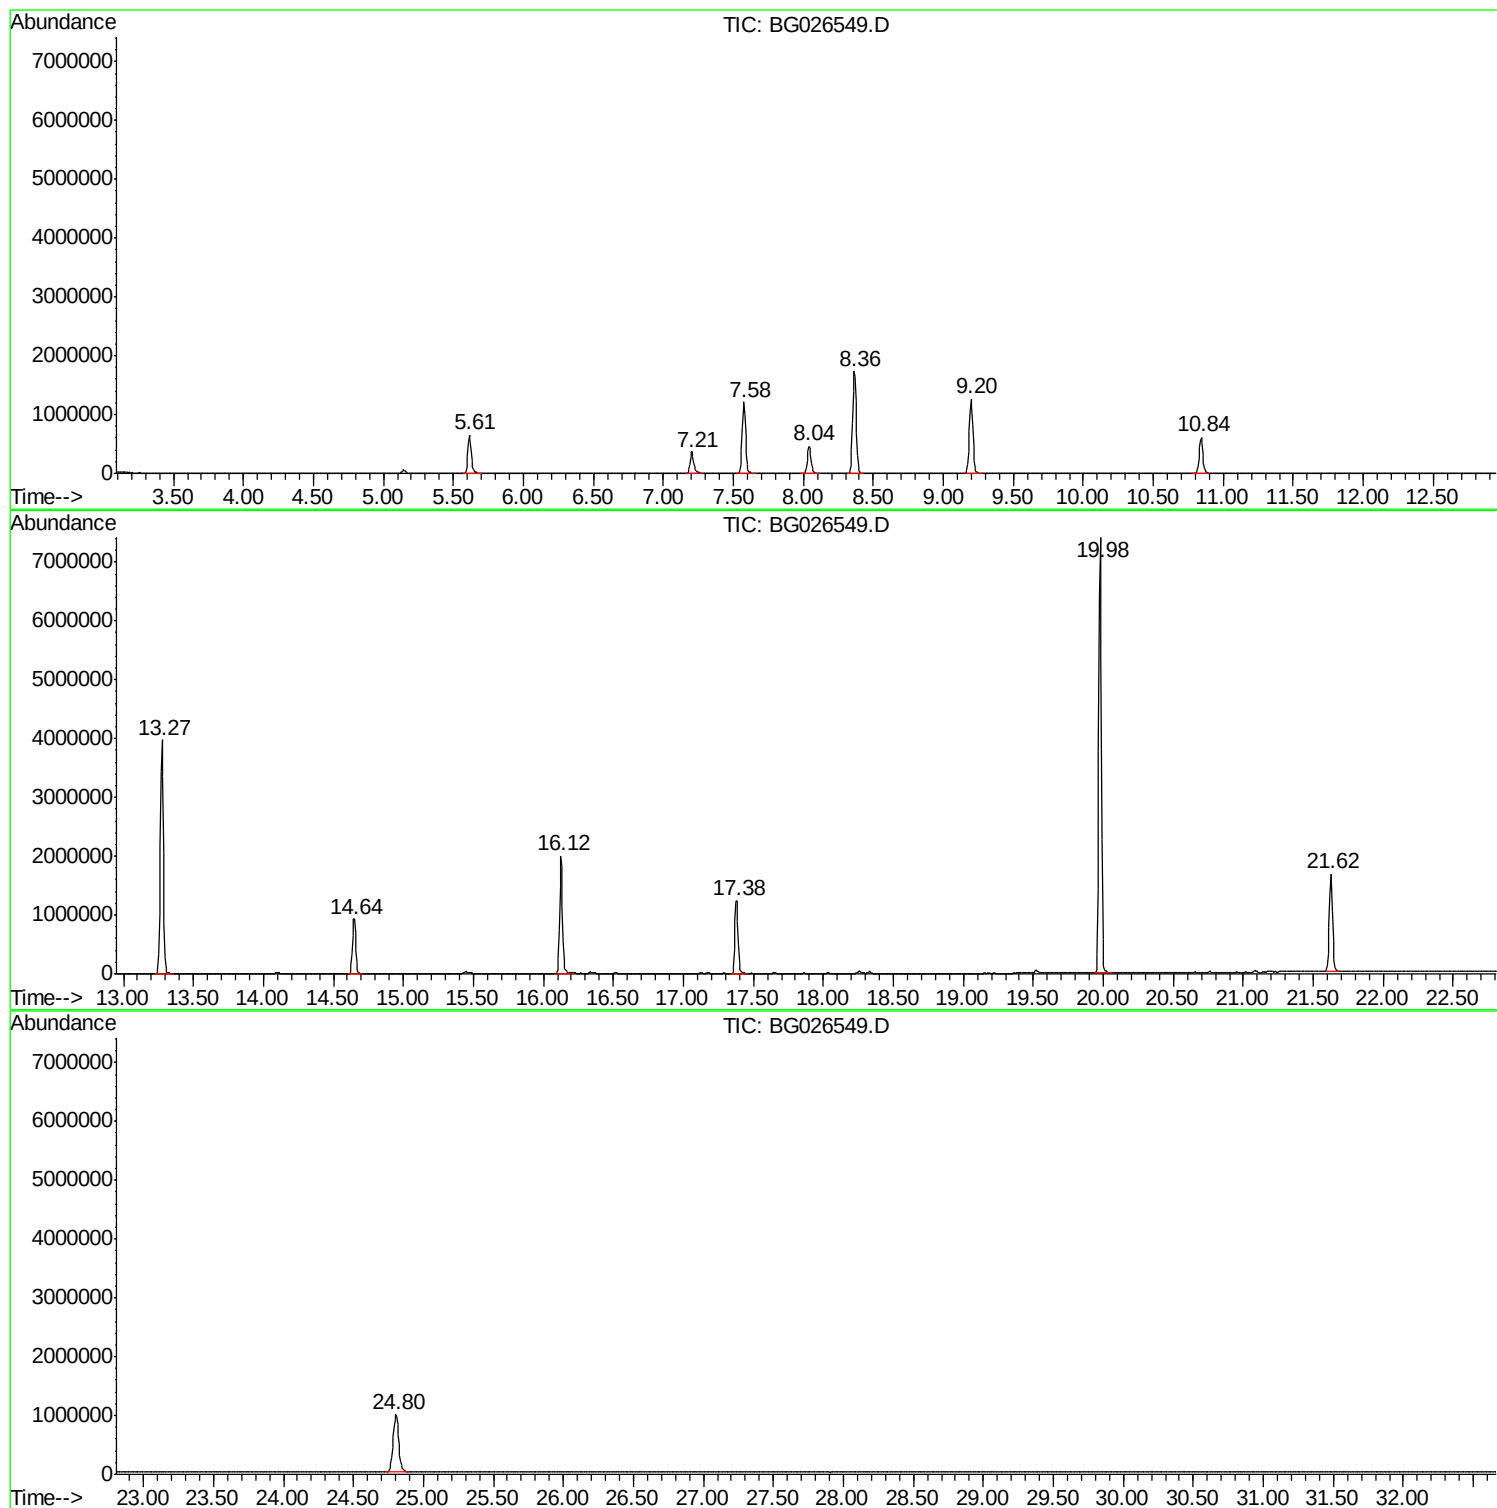

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
Data File : BG026549.D
Acq On : 4 Apr 2017 18:36
Operator : SJ/MA
Sample : I2484-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
033017-PRRT-F-D-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	53.04 ng	2106290	1,4-Dichlorobenzene-d4	8.04

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	38	
2	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38	
3	Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	12	
4	Amphetaminil	250	C17H18N2	017590-01-1	12	
5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9	

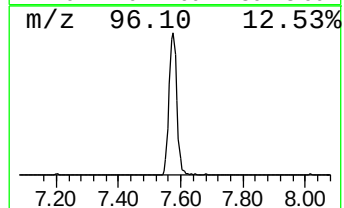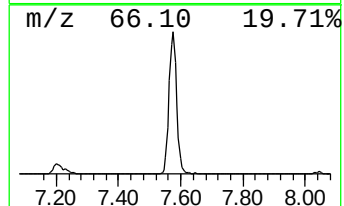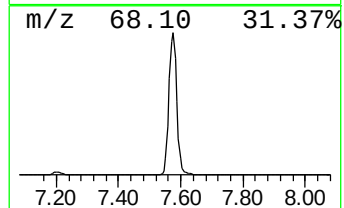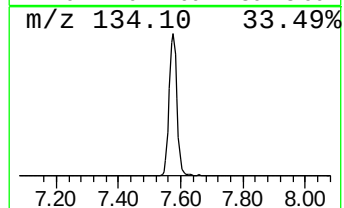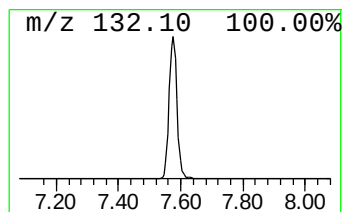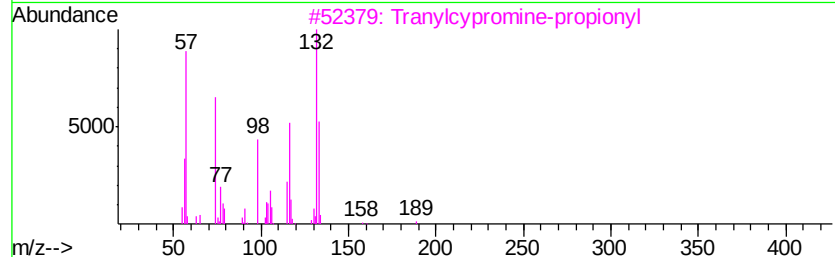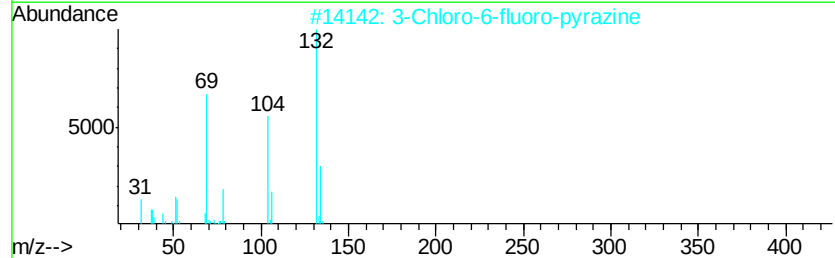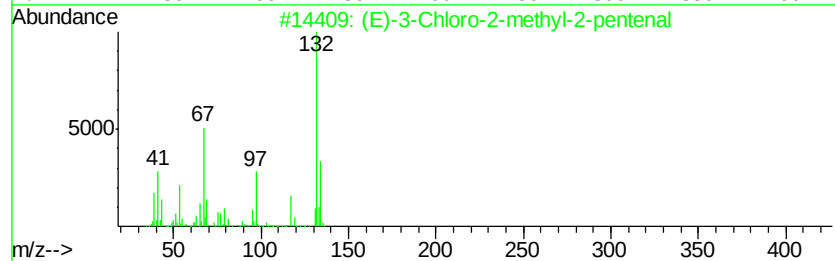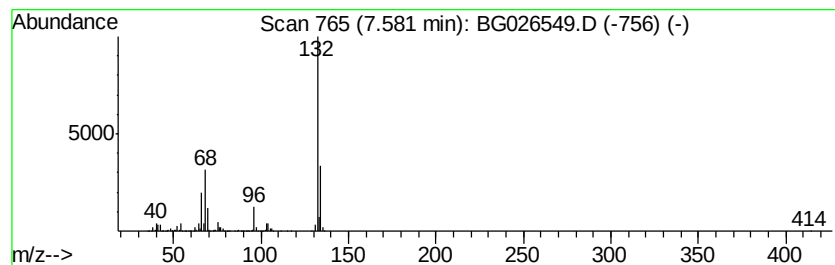

Data Path : Z:\HPCHEM1\BNA_G\Data\BG040417\
Data File : BG026549.D
Acq On : 4 Apr 2017 18:36
Operator : SJ/MA
Sample : I2484-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
033017-PRRT-F-D-M

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	53.0	ng	2106290	1	8.04	794295	20.0