

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
 Data File : BG026552.D
 Acq On : 4 Apr 2017 20:35
 Operator : SJ/MA
 Sample : I2485-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 032917-DSDC-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.617	423	430	443	rBV	705829	1191038	10.51%	2.692%
2	7.203	692	700	712	rBV	498182	933220	8.24%	2.109%
3	7.574	756	763	775	rBV	1371719	2390940	21.11%	5.404%
4	8.044	836	843	851	rBV	516438	884110	7.80%	1.998%
5	8.367	889	898	907	rBV	2047559	3556554	31.40%	8.038%
6	9.201	1032	1040	1050	rBV	1400036	2569142	22.68%	5.806%
7	10.840	1309	1319	1331	rBV	696151	1257033	11.10%	2.841%
8	13.273	1726	1733	1747	rBV	4449624	7147917	63.10%	16.154%
9	14.648	1957	1967	1978	rBV2	1051085	1700695	15.01%	3.844%
10	16.128	2212	2219	2236	rBV	2172925	3355265	29.62%	7.583%
11	17.380	2425	2432	2445	rBV	1388959	2157577	19.05%	4.876%
12	19.977	2868	2874	2884	rBV	8329207	11328353	100.00%	25.602%
13	21.628	3147	3155	3167	rBV	1679132	2871069	25.34%	6.489%
14	24.801	3683	3695	3710	rBV2	1001686	2904734	25.64%	6.565%


Sum of corrected areas: 44247647

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
Data File : BG026552.D
Acq On : 4 Apr 2017 20:35
Operator : SJ/MA
Sample : I2485-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032917-DSDC-F-D-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

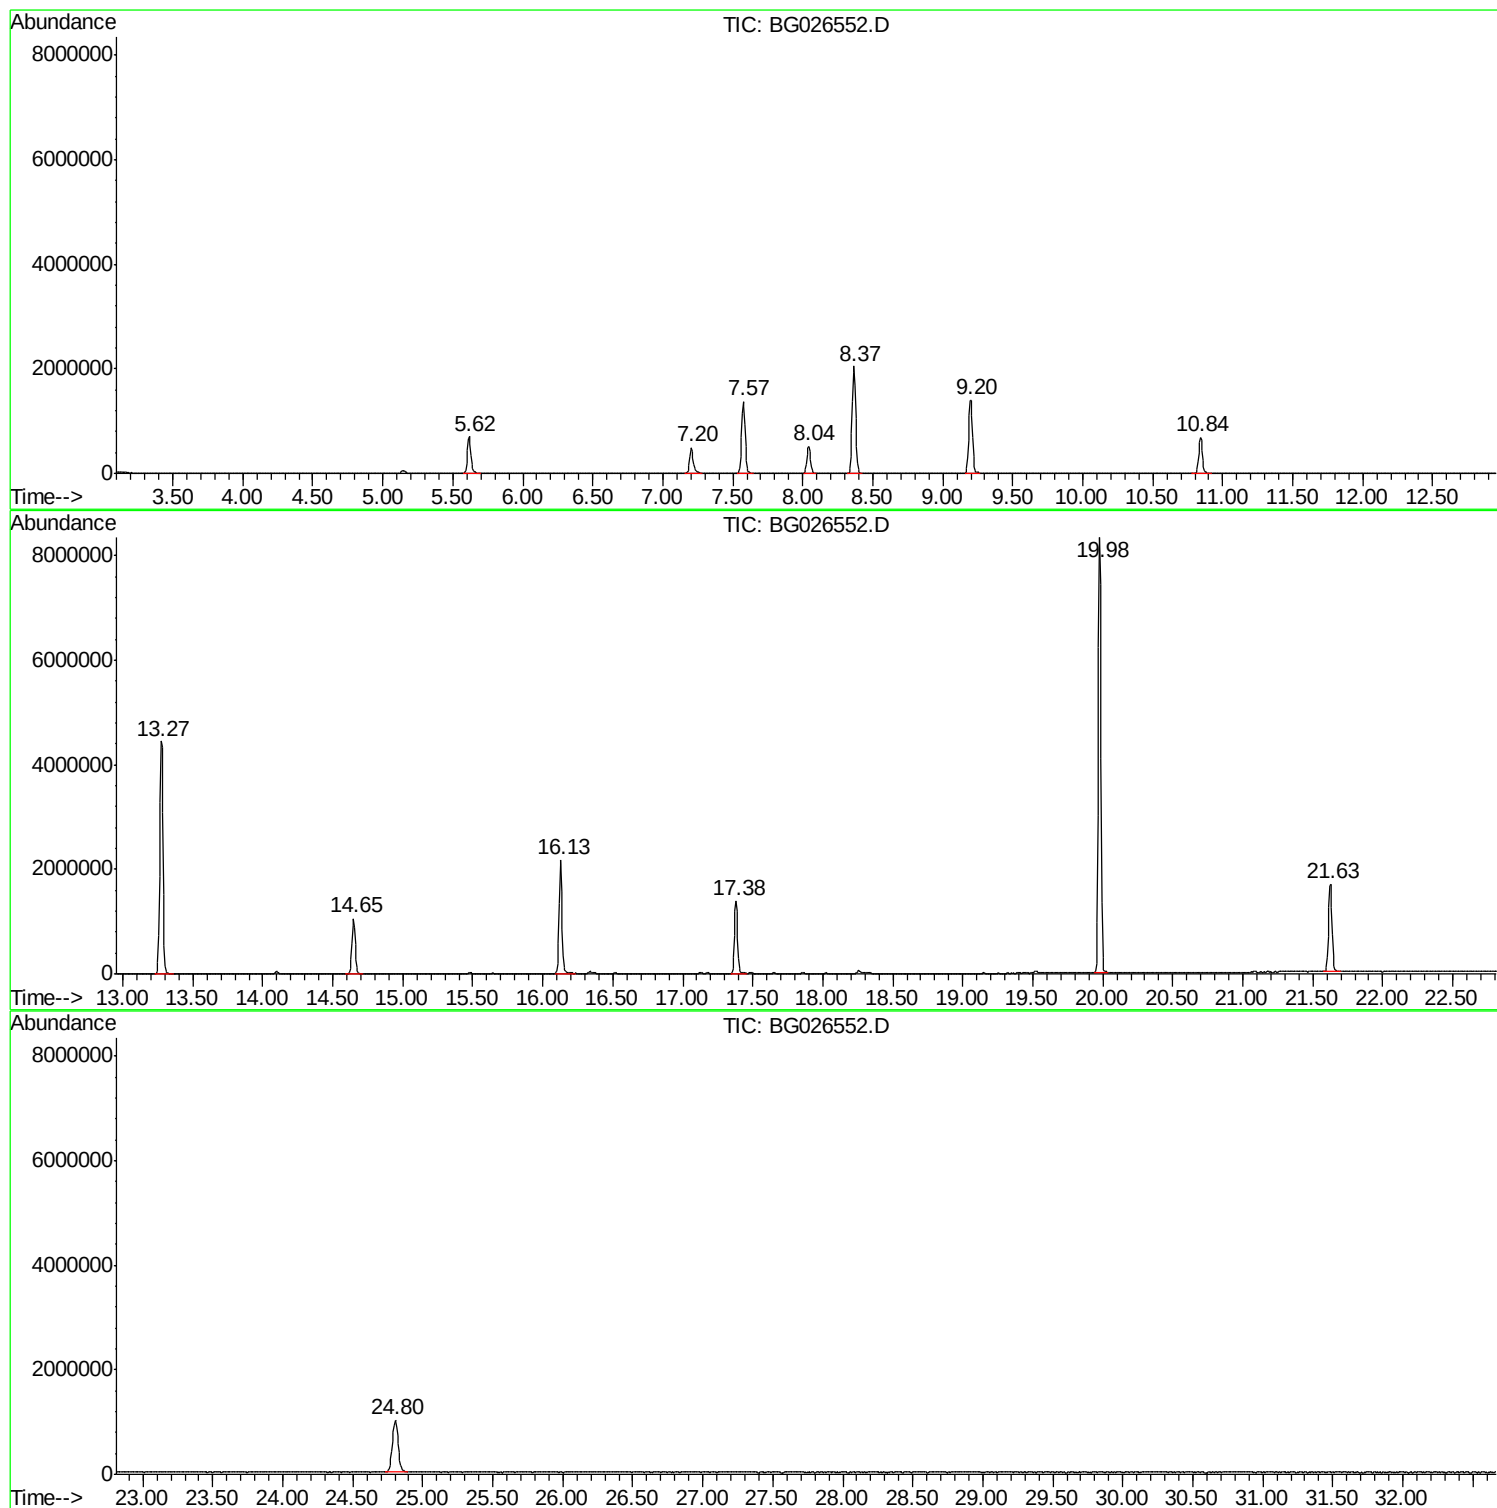

Data Path : Z:\HPCHEM1\BNA G\Data\BG040417\
Data File : BG026552.D
Acq On : 4 Apr 2017 20:35
Operator : SJ/MA
Sample : I2485-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032917-DSDC-F-D-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.57 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.57	54.09 ng	2390940	1,4-Dichlorobenzene-d4	8.04

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

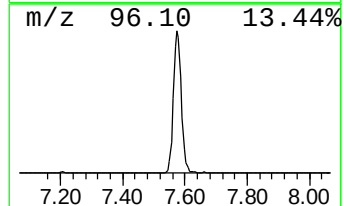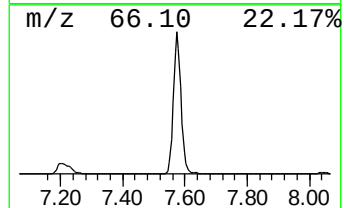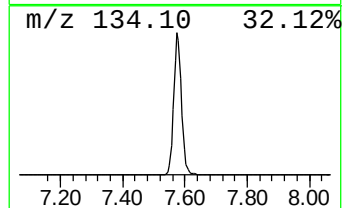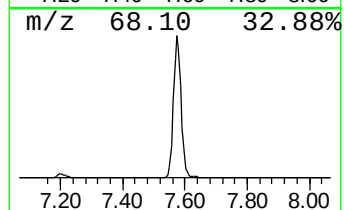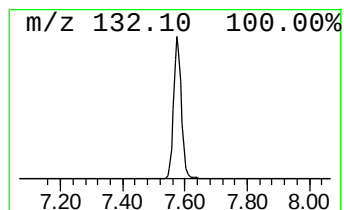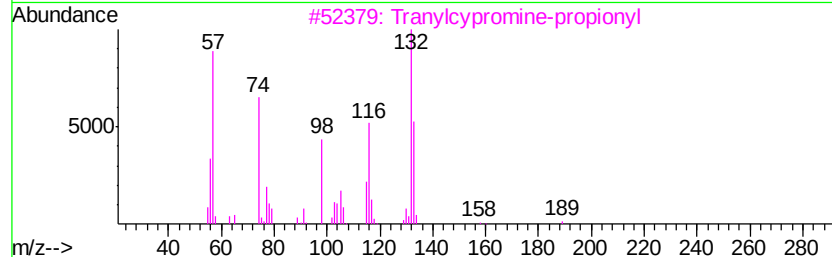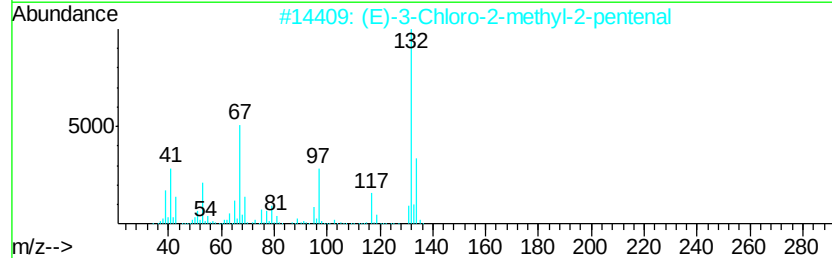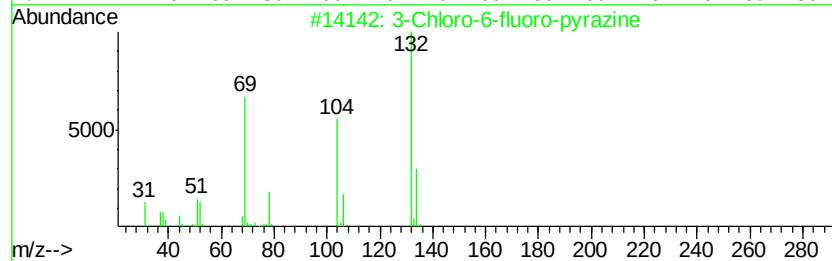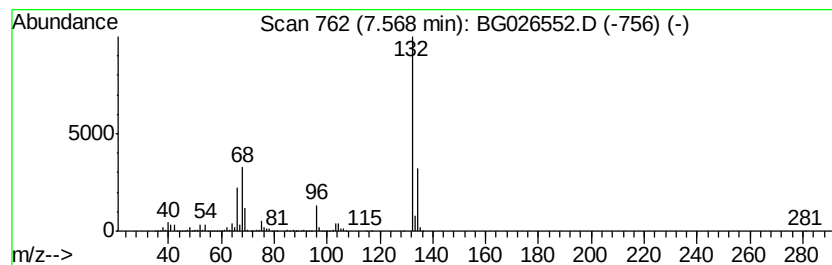

Data Path : Z:\HPCHEM1\BNA_G\Data\BG040417\
Data File : BG026552.D
Acq On : 4 Apr 2017 20:35
Operator : SJ/MA
Sample : I2485-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032917-DSDC-F-D-M

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.57	7.57	54.1	ng	2390940	1	8.04	884110	20.0