
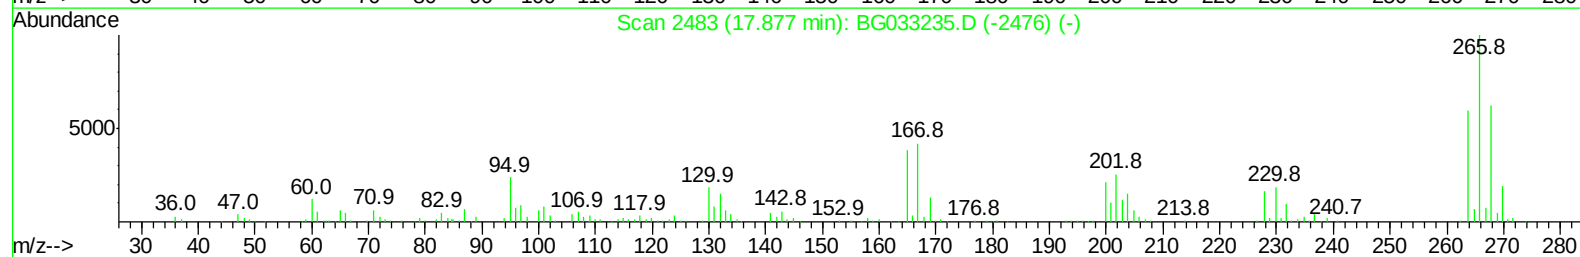
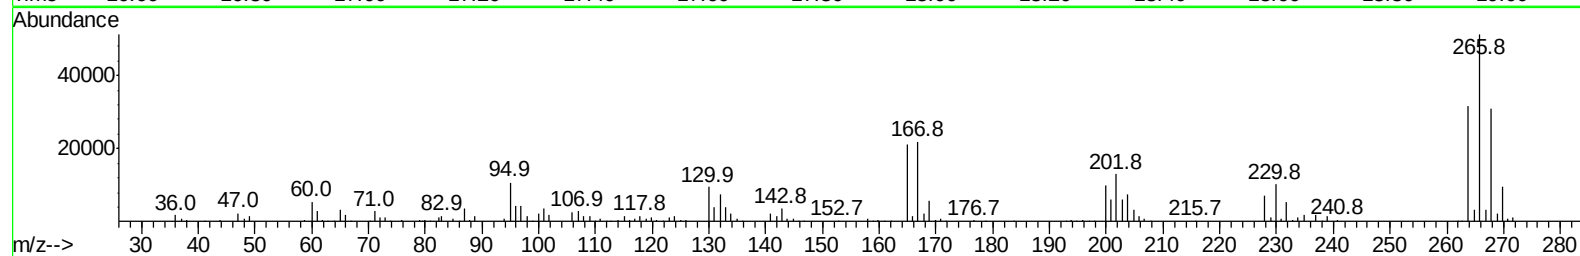


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040418\
Data File : BG033553.D
Acq On : 4 Apr 2018 10:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 04:54:30 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:35:46 2018
Response via : Initial Calibration

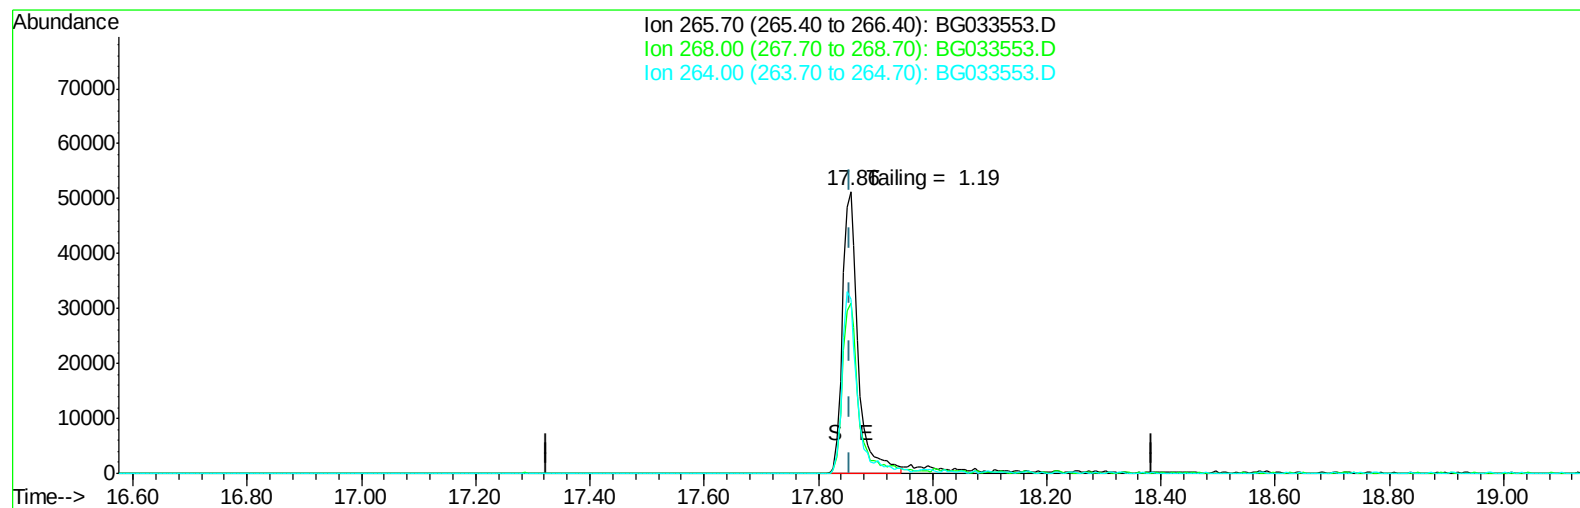

TIC: BG033553.D

(69) Pentachlorophenol (C)




17.856min (+0.001) 17524.09ng

response 97346

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.32
264.00	62.00	61.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040418\
Data File : BG033553.D
Acq On : 4 Apr 2018 10:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 04:54:30 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:35:46 2018
Response via : Initial Calibration

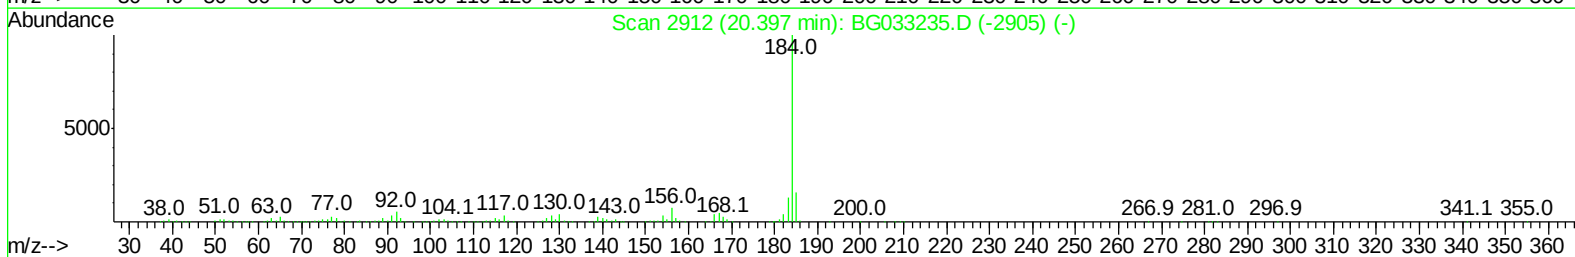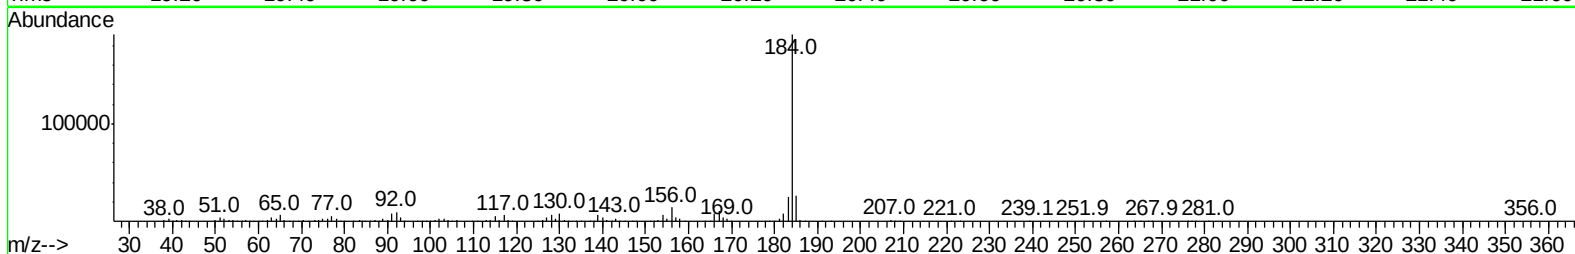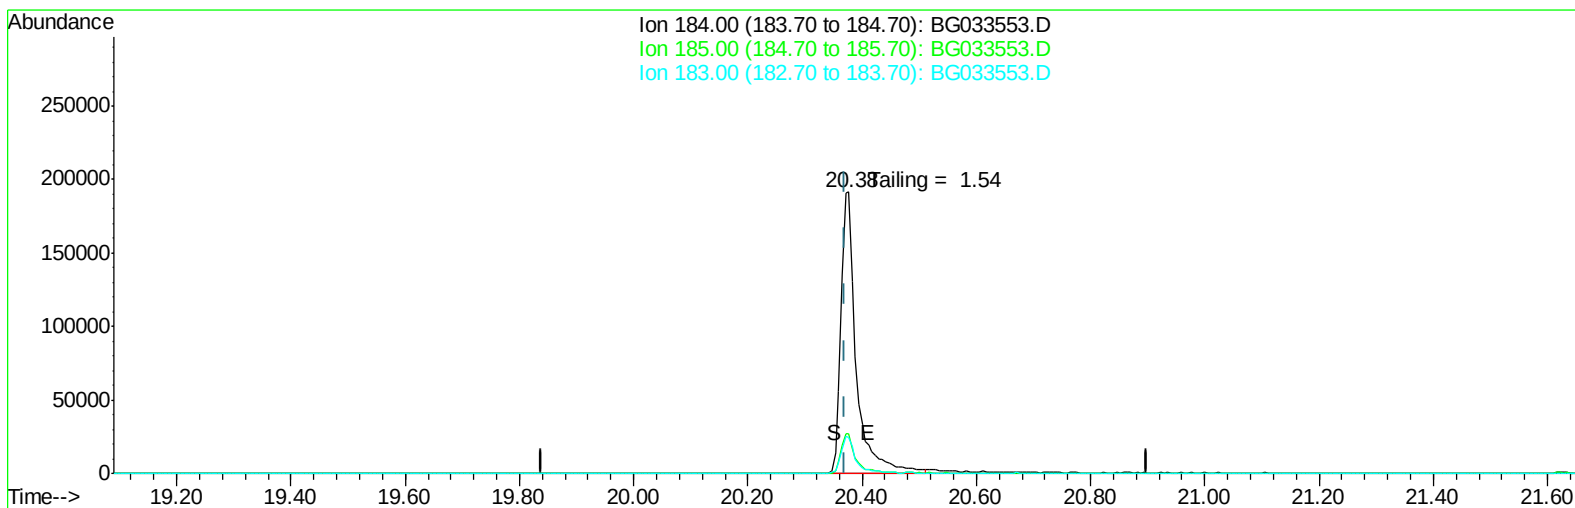

TIC: BG033553.D

(76) Benzidine

20.377min (+0.007) 0.00ng

response 360854

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.09
183.00	13.30	12.81
0.00	0.00	0.00