


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040418\
 Data File : BG033553.D
 Acq On : 4 Apr 2018 10:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 04 18:35:46 2018

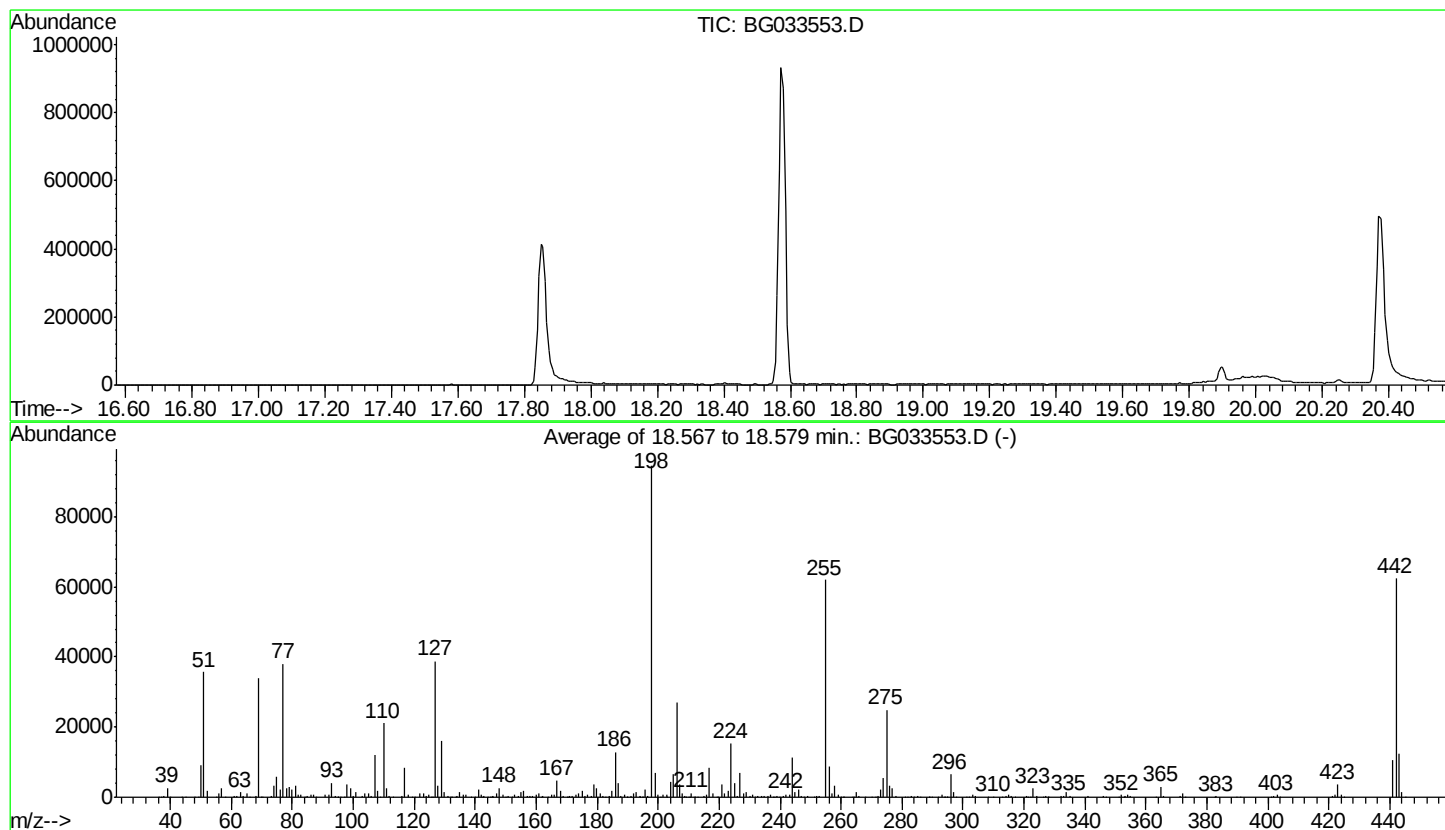

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	35736	PASS
68	69	0.00	2	1.4	479	PASS
69	198	0.00	100	36.0	34061	PASS
70	69	0.00	2	0.2	60	PASS
127	198	10	80	41.0	38714	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94538	PASS
199	198	5	9	7.2	6794	PASS
275	198	10	60	26.3	24898	PASS
365	198	1	100	3.2	3058	PASS
441	443	0.01	100	83.2	10435	PASS
442	198	50	100	65.8	62237	PASS
443	442	15	24	20.1	12535	PASS