

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
 Data File : BG053015.D
 Acq On : 4 Apr 2022 19:42
 Operator : CG/JU
 Sample : N2207-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-098-21-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.688	384	391	402	rBV	344706	581511	17.57%	4.632%
2	7.109	626	633	639	rBV3	16949	33150	1.00%	0.264%
3	7.274	655	661	670	rVB	227199	400398	12.10%	3.190%
4	8.125	800	806	813	rBV	132333	231251	6.99%	1.842%
5	9.289	995	1004	1012	rBV	524795	933263	28.19%	7.435%
6	10.164	1144	1153	1161	rBV3	26802	66103	2.00%	0.527%
7	10.240	1161	1166	1173	rVB3	23449	42914	1.30%	0.342%
8	10.939	1276	1285	1294	rVB	174223	315532	9.53%	2.514%
9	11.462	1366	1374	1384	rBV	68628	146035	4.41%	1.163%
10	13.371	1692	1699	1707	rBV	1251289	1978764	59.78%	15.763%
11	13.653	1739	1747	1753	rBV2	44150	69417	2.10%	0.553%
12	14.746	1927	1933	1939	rBV	273159	427474	12.91%	3.405%
13	15.145	1996	2001	2012	rBV2	34410	53548	1.62%	0.427%
14	16.232	2178	2186	2196	rBV	1083949	1693513	51.16%	13.491%
15	16.761	2266	2276	2282	rBV4	14432	35755	1.08%	0.285%
16	16.872	2287	2295	2303	rVV4	49047	86004	2.60%	0.685%
17	17.237	2350	2357	2366	rBV7	18099	35453	1.07%	0.282%
18	17.489	2394	2400	2408	rVB	350255	535506	16.18%	4.266%
19	18.253	2524	2530	2534	rBV3	29612	47989	1.45%	0.382%
20	18.364	2544	2549	2558	rBV2	56687	89135	2.69%	0.710%
21	20.092	2836	2843	2849	rBV	2376111	3310168	100.00%	26.370%
22	21.396	3061	3065	3076	rBV5	35459	79933	2.41%	0.637%
23	21.772	3121	3129	3137	rBV	376586	638270	19.28%	5.085%
24	23.493	3417	3422	3431	rVB2	35200	67407	2.04%	0.537%
25	25.073	3679	3691	3704	rVB2	222969	654497	19.77%	5.214%




Sum of corrected areas: 12552990

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053015.D
Acq On : 4 Apr 2022 19:42
Operator : CG/JU
Sample : N2207-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-098-21-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

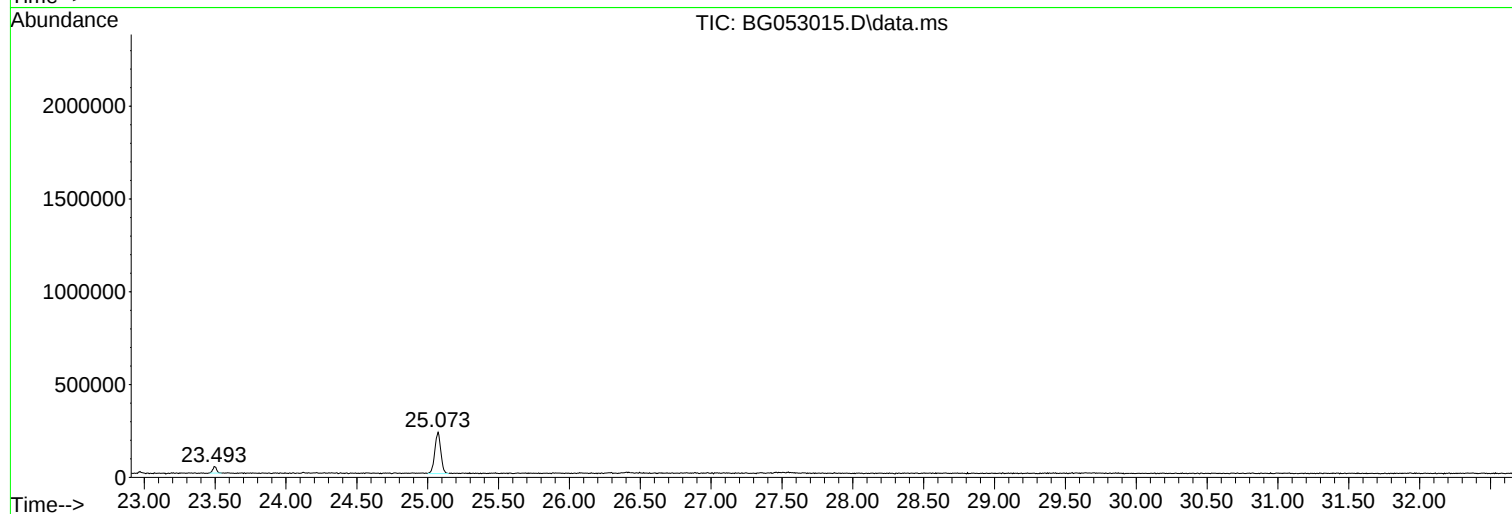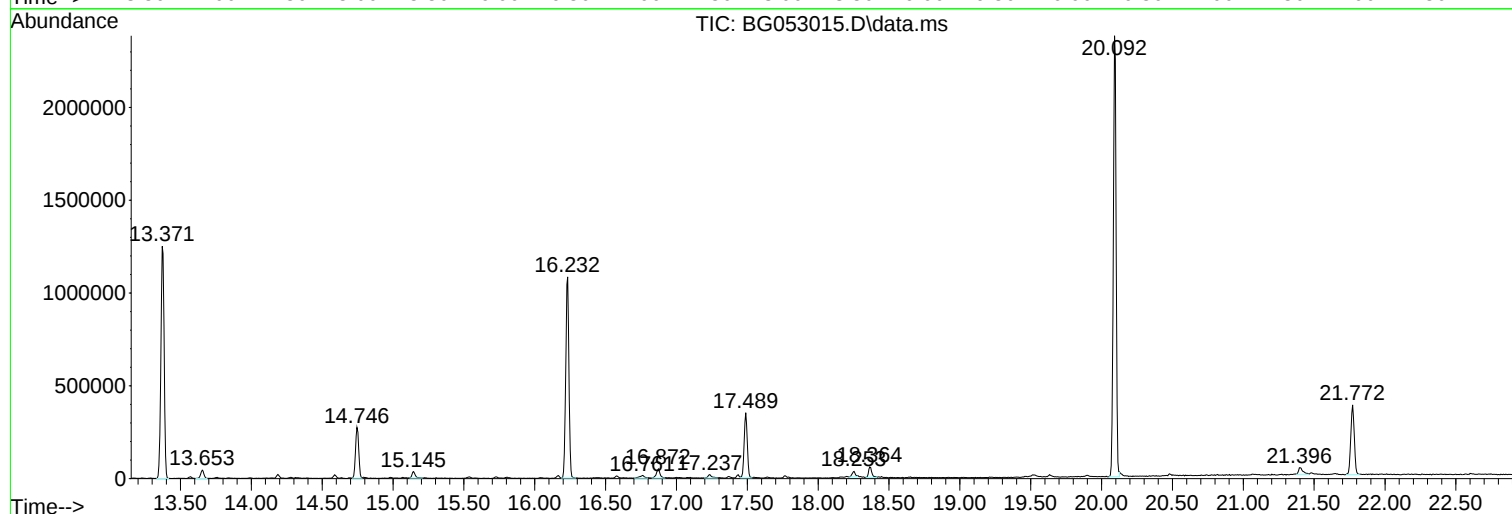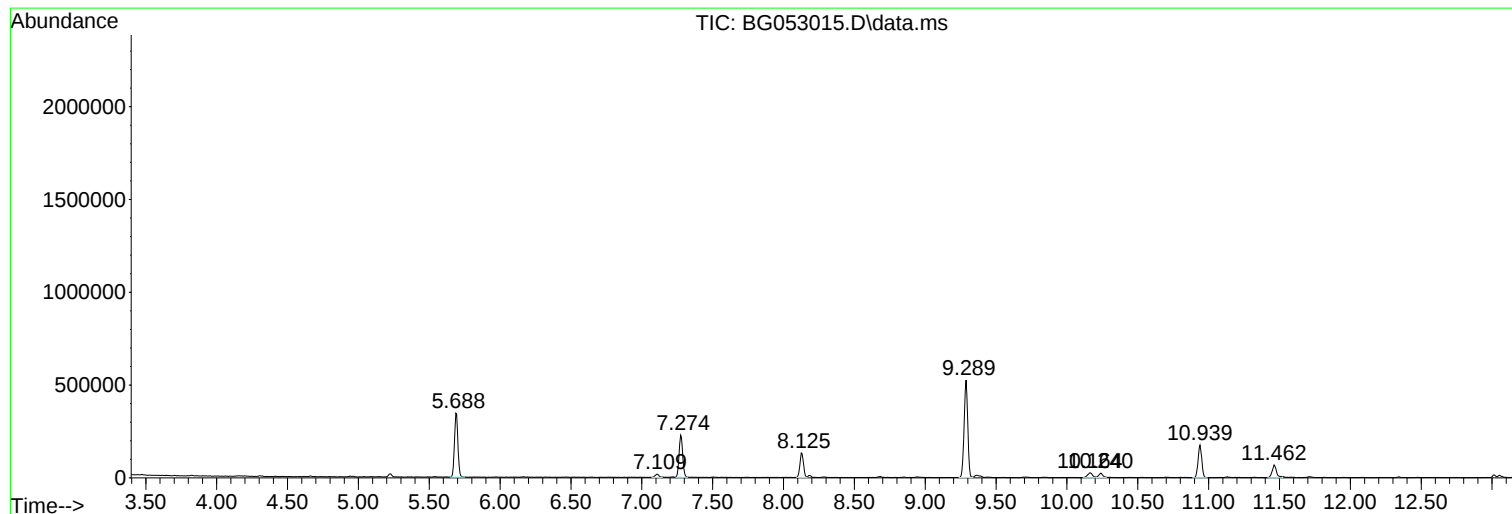

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053015.D
Acq On : 4 Apr 2022 19:42
Operator : CG/JU
Sample : N2207-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-098-21-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053015.D
Acq On : 4 Apr 2022 19:42
Operator : CG/JU
Sample : N2207-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-098-21-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------