

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
 Data File : BG053018.D
 Acq On : 4 Apr 2022 21:39
 Operator : CG/JU
 Sample : N2207-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-096-21-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.692	385	392	401	rVB	295255	497068	15.25%	3.709%
2	7.137	625	638	643	rBV3	41789	105838	3.25%	0.790%
3	7.272	654	661	672	rVB	198334	359785	11.04%	2.685%
4	8.130	798	807	813	rBV	140199	254355	7.80%	1.898%
5	8.688	895	902	908	rBV3	18496	34356	1.05%	0.256%
6	9.287	994	1004	1012	rBV	446390	819117	25.12%	6.112%
7	9.364	1012	1017	1026	rVB4	22715	48696	1.49%	0.363%
8	10.168	1144	1154	1161	rBV7	20959	63386	1.94%	0.473%
9	10.262	1161	1170	1178	rVB3	70334	161165	4.94%	1.203%
10	10.938	1277	1285	1291	rBV	181169	327891	10.06%	2.447%
11	13.023	1633	1640	1644	rBV2	53645	96780	2.97%	0.722%
12	13.370	1690	1699	1708	rVB	1101888	1822884	55.91%	13.602%
13	13.652	1740	1747	1754	rBV	55929	94782	2.91%	0.707%
14	13.758	1759	1765	1775	rVV5	20715	37537	1.15%	0.280%
15	14.592	1900	1907	1912	rVB	34559	55656	1.71%	0.415%
16	14.745	1928	1933	1939	rBV	282066	443418	13.60%	3.309%
17	14.985	1969	1974	1984	rVB3	21962	41105	1.26%	0.307%
18	15.150	1994	2002	2011	rBV	124235	200192	6.14%	1.494%
19	15.732	2094	2101	2106	rBV3	25533	41282	1.27%	0.308%
20	15.802	2109	2113	2122	rVB6	20302	34968	1.07%	0.261%
21	16.231	2178	2186	2196	rBV	1100574	1656639	50.81%	12.361%
22	16.577	2240	2245	2251	rBV4	33997	47746	1.46%	0.356%
23	16.760	2270	2276	2281	rVB3	19028	37481	1.15%	0.280%
24	16.877	2288	2296	2303	rBV2	104349	172881	5.30%	1.290%
25	17.235	2351	2357	2364	rBV3	58020	106209	3.26%	0.792%
26	17.435	2387	2391	2394	rVV2	36010	48169	1.48%	0.359%
27	17.488	2394	2400	2408	rVB	357033	560042	17.18%	4.179%
28	17.770	2441	2448	2460	rBV4	26266	64247	1.97%	0.479%
29	18.252	2525	2530	2537	rVB2	56569	92206	2.83%	0.688%
30	18.369	2544	2550	2555	rBV2	82368	112892	3.46%	0.842%
31	19.521	2739	2746	2758	rBV10	31565	83128	2.55%	0.620%
32	19.632	2761	2765	2771	rVB8	22618	33572	1.03%	0.250%
33	20.096	2837	2844	2856	rBV	2349452	3260323	100.00%	24.327%
34	21.400	3062	3066	3071	rBV4	38429	59895	1.84%	0.447%
35	21.770	3122	3129	3135	rBV	386072	656917	20.15%	4.902%
36	23.497	3417	3423	3431	rVB	89850	179505	5.51%	1.339%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053018.D
Acq On : 4 Apr 2022 21:39
Operator : CG/JU
Sample : N2207-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-03

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	25.072	3681	3691	3704	rVB2	236559	689932	21.16%	5.148%
----	--------	------	------	------	------	--------	--------	--------	--------




Sum of corrected areas: 13402045

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053018.D
Acq On : 4 Apr 2022 21:39
Operator : CG/JU
Sample : N2207-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

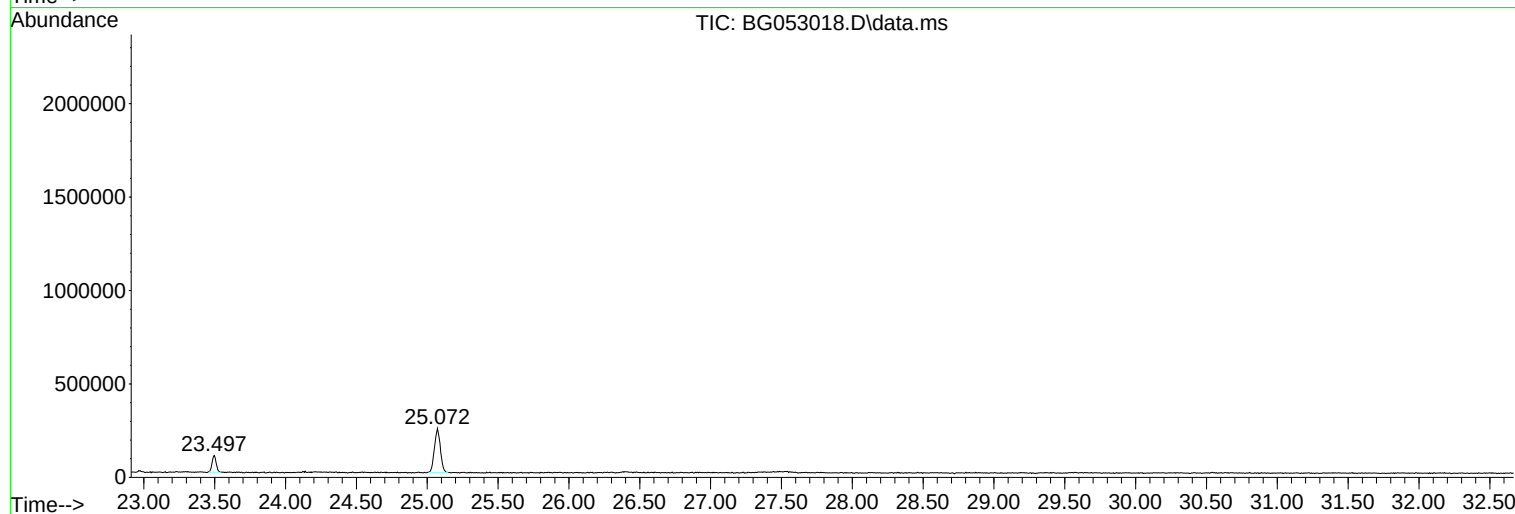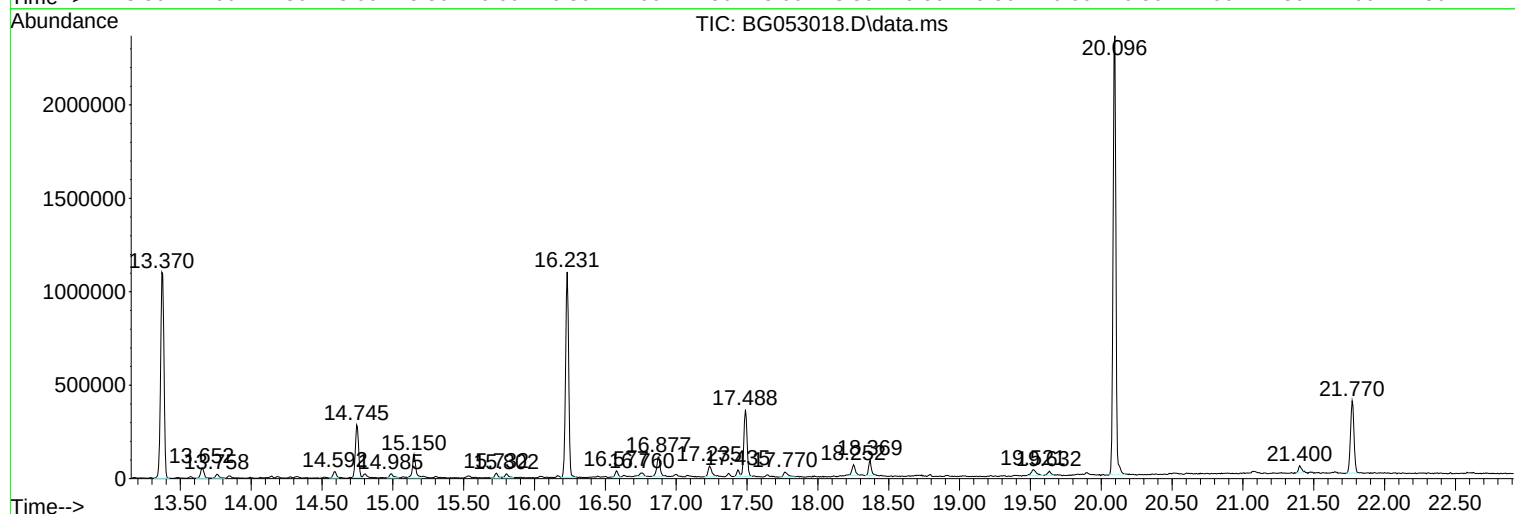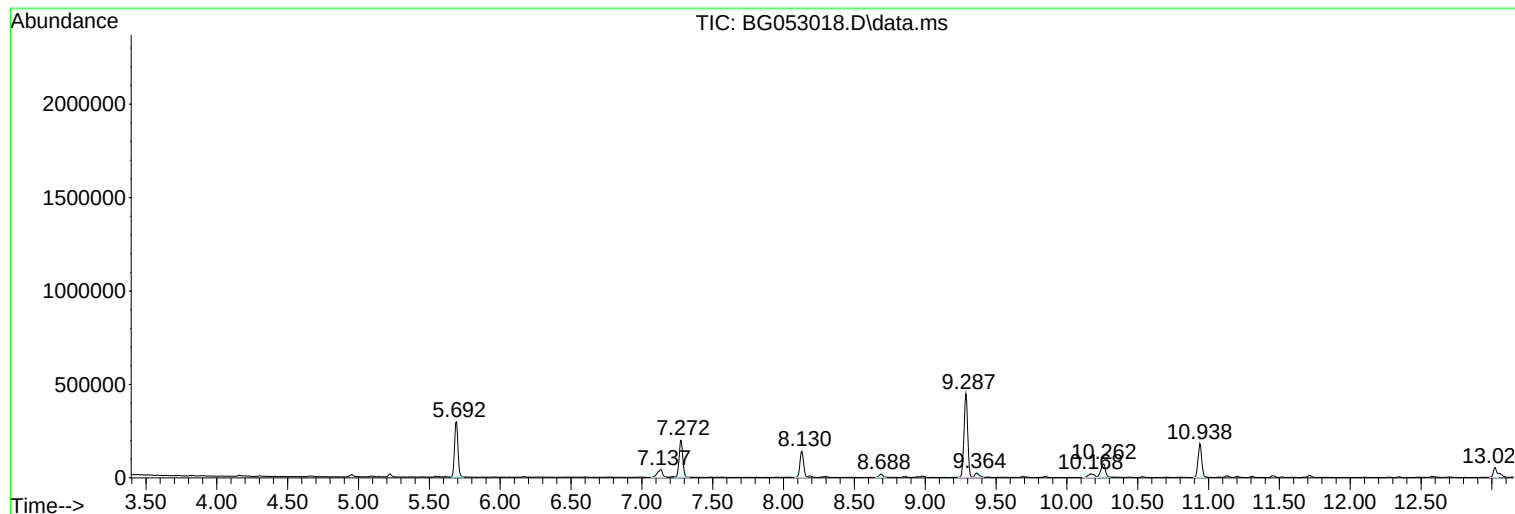

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053018.D
Acq On : 4 Apr 2022 21:39
Operator : CG/JU
Sample : N2207-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053018.D
Acq On : 4 Apr 2022 21:39
Operator : CG/JU
Sample : N2207-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------