

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
 Data File : BG053020.D
 Acq On : 4 Apr 2022 22:56
 Operator : CG/JU
 Sample : N2207-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-096-21-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.691	385	392	403	rVB	296765	487330	15.47%	3.930%
2	7.130	627	637	645	rBV	33396	78906	2.50%	0.636%
3	7.277	655	662	672	rVB2	200249	353615	11.23%	2.852%
4	8.129	799	807	813	rBV	147929	252596	8.02%	2.037%
5	9.286	995	1004	1012	rBV	445208	803285	25.50%	6.478%
6	9.362	1012	1017	1025	rVB3	21288	43558	1.38%	0.351%
7	10.167	1145	1154	1161	rBV6	21742	60680	1.93%	0.489%
8	10.255	1161	1169	1180	rVB2	56933	121745	3.86%	0.982%
9	10.936	1279	1285	1291	rBV	175817	326111	10.35%	2.630%
10	13.022	1634	1640	1643	rBV2	39182	65791	2.09%	0.531%
11	13.051	1643	1645	1653	rVB3	23178	41418	1.31%	0.334%
12	13.374	1693	1700	1708	rVB	1108788	1747629	55.48%	14.094%
13	13.656	1742	1748	1755	rBV	73679	121448	3.86%	0.979%
14	14.590	1902	1907	1912	rBV	40438	62192	1.97%	0.502%
15	14.749	1927	1934	1940	rBV	275979	443797	14.09%	3.579%
16	14.808	1940	1944	1951	rVB5	16501	33468	1.06%	0.270%
17	15.148	1994	2002	2011	rBV2	70009	124498	3.95%	1.004%
18	16.229	2179	2186	2194	rBV	1007855	1565963	49.71%	12.629%
19	16.870	2287	2295	2303	rBV4	65207	126908	4.03%	1.023%
20	17.234	2351	2357	2365	rBV5	44686	85739	2.72%	0.691%
21	17.486	2395	2400	2410	rVB	353945	561657	17.83%	4.530%
22	17.763	2443	2447	2456	rBV3	28672	65785	2.09%	0.531%
23	18.256	2523	2531	2537	rBV6	16834	35732	1.13%	0.288%
24	18.362	2544	2549	2556	rBV2	58635	90593	2.88%	0.731%
25	19.525	2739	2747	2756	rBV2	20683	60249	1.91%	0.486%
26	20.095	2838	2844	2856	rBV	2336231	3150122	100.00%	25.404%
27	21.399	3061	3066	3076	rBV	92685	161897	5.14%	1.306%
28	21.769	3123	3129	3137	rVB	375266	642371	20.39%	5.180%
29	25.070	3681	3691	3706	rVB2	223941	684789	21.74%	5.523%




Sum of corrected areas: 12399872

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053020.D
Acq On : 4 Apr 2022 22:56
Operator : CG/JU
Sample : N2207-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

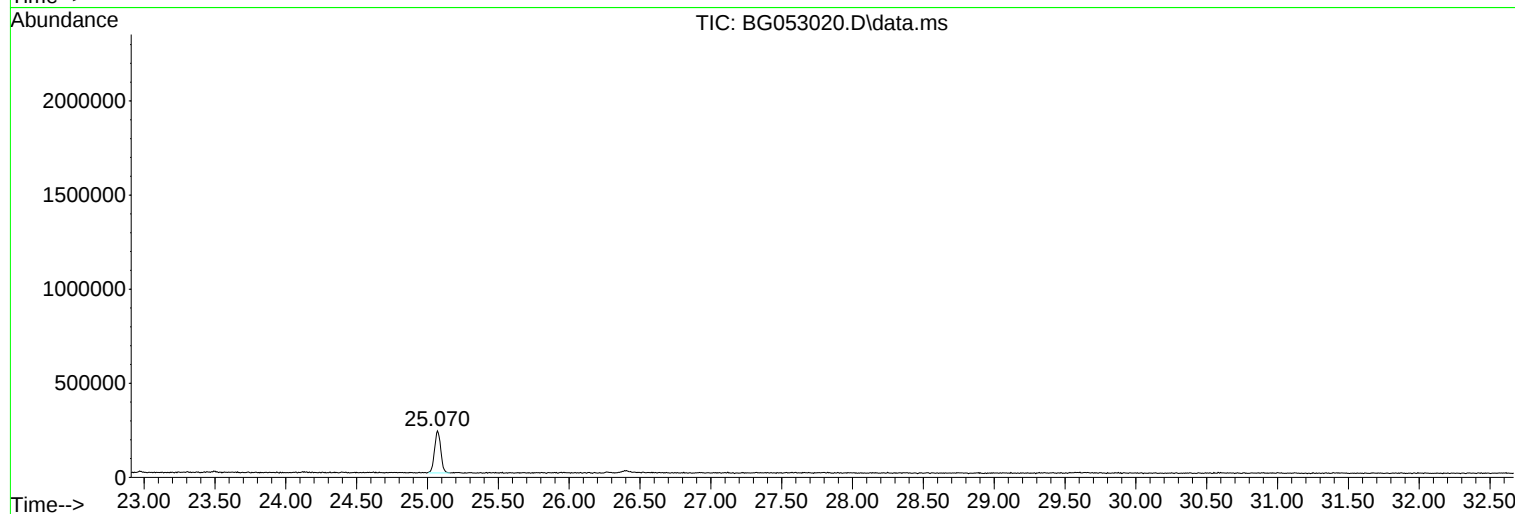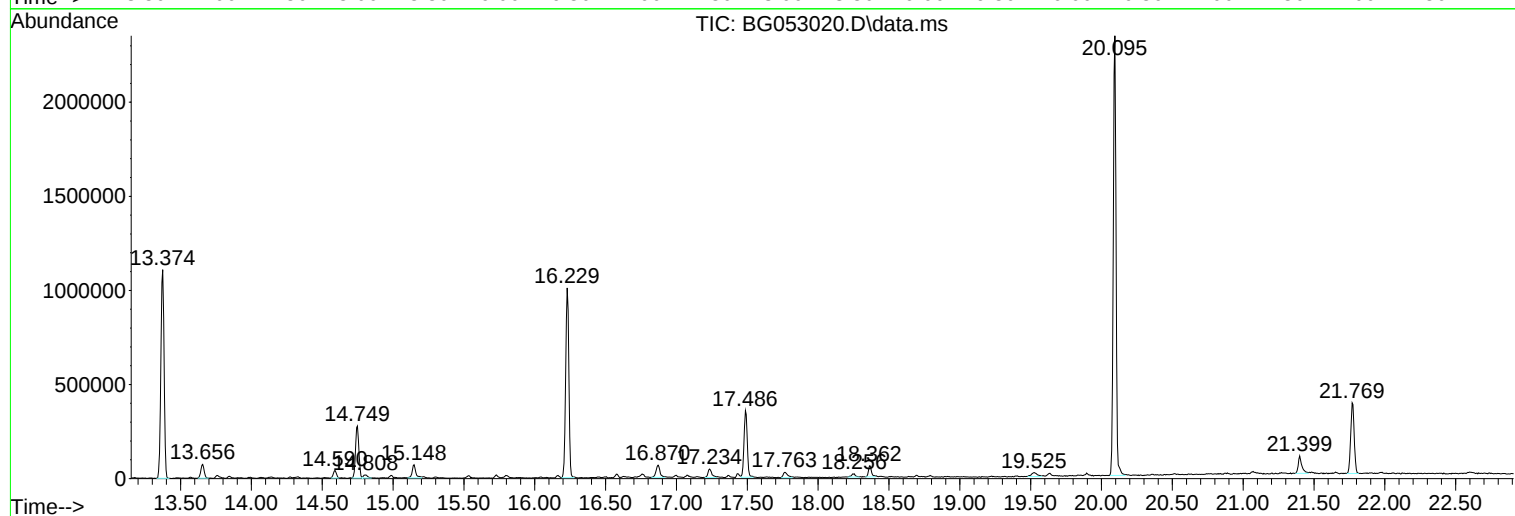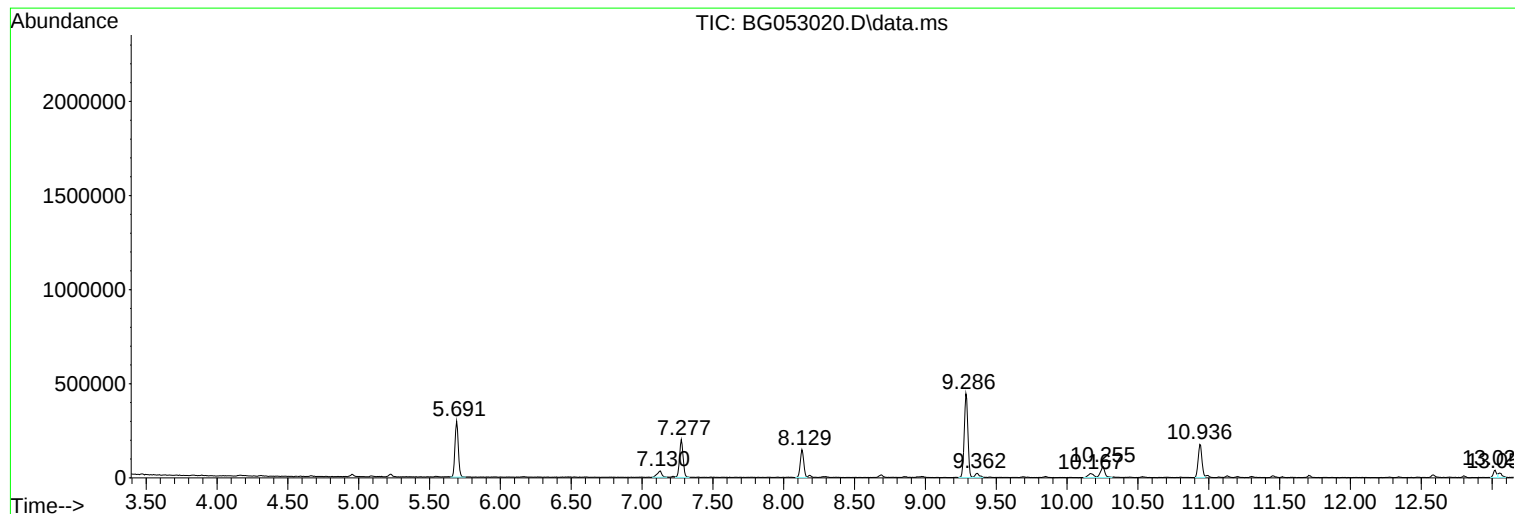

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053020.D
Acq On : 4 Apr 2022 22:56
Operator : CG/JU
Sample : N2207-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053020.D
Acq On : 4 Apr 2022 22:56
Operator : CG/JU
Sample : N2207-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------