


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
 Data File : BG053006.D
 Acq On : 4 Apr 2022 13:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 05 14:24:42 2022

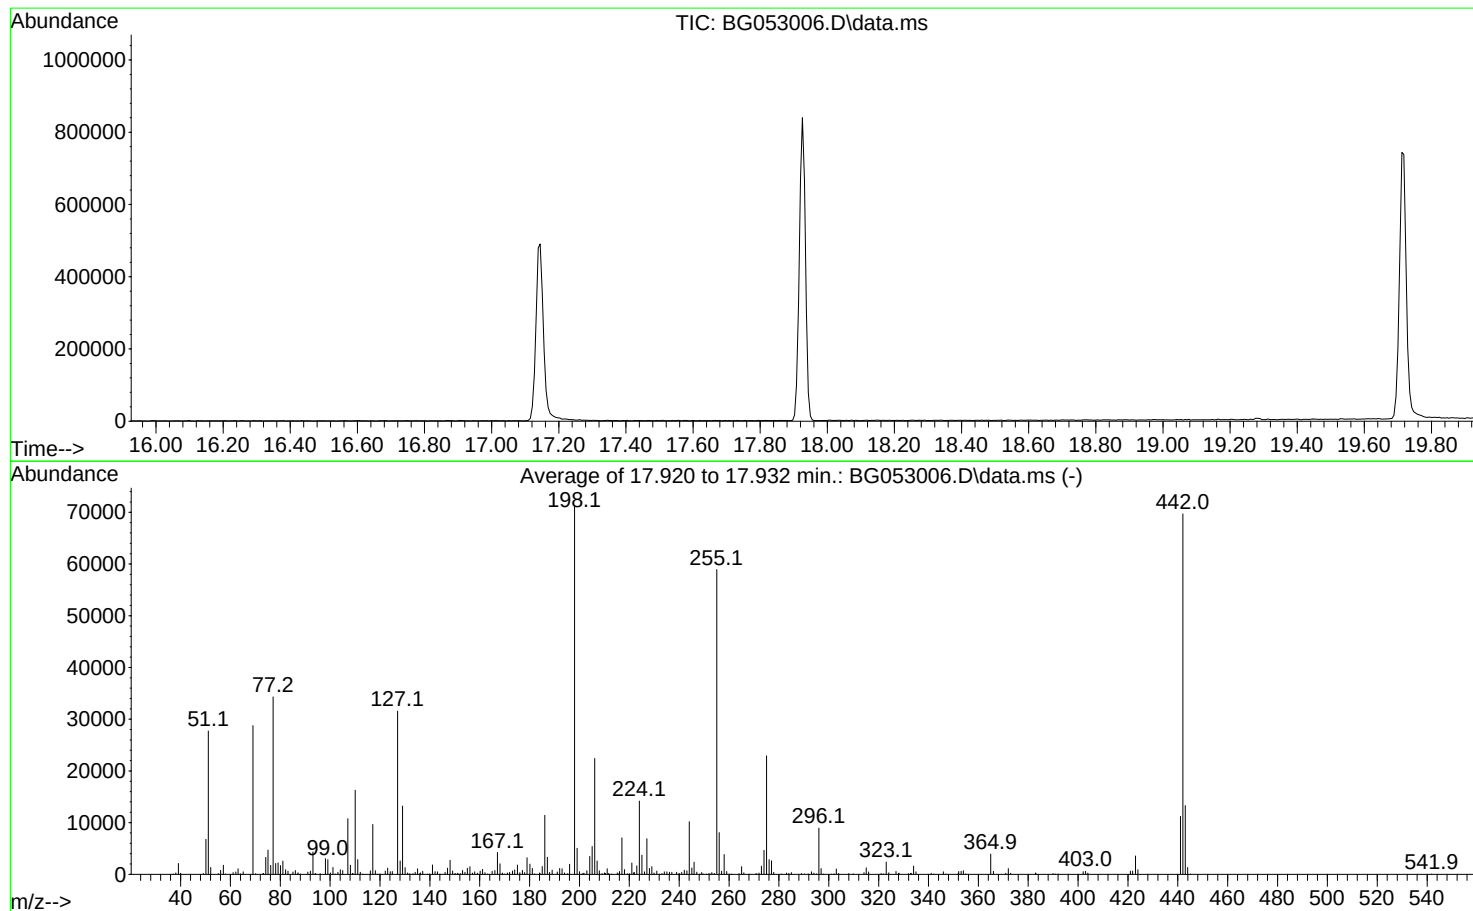




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	27712	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.4	28768	PASS
70	69	0.00	2	0.4	121	PASS
127	198	10	80	44.4	31560	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71123	PASS
199	198	5	9	7.1	5037	PASS
275	198	10	60	32.2	22917	PASS
365	198	1	100	5.5	3942	PASS
441	198	0.01	100	15.8	11206	PASS
442	442	50	100	100.0	69701	PASS
443	442	15	24	19.1	13306	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
Data File : BG053006.D
Acq On : 4 Apr 2022 13:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 02:30:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 16:48:57 2022
Response via : Initial Calibration

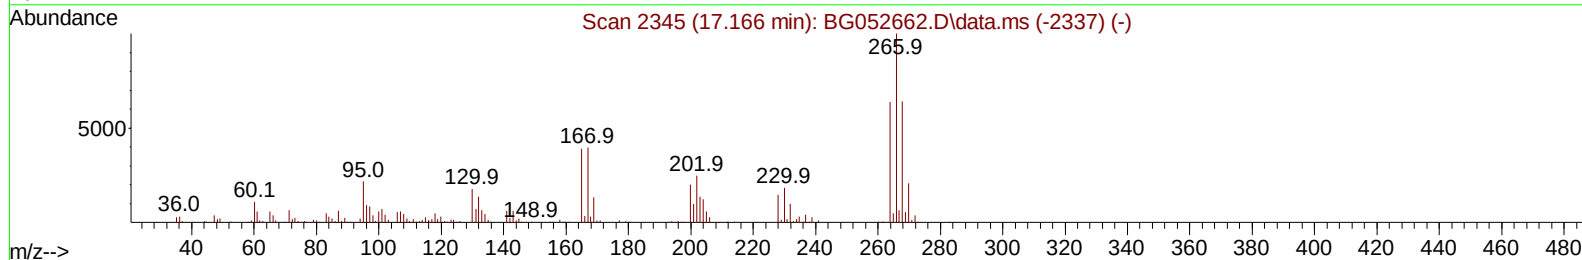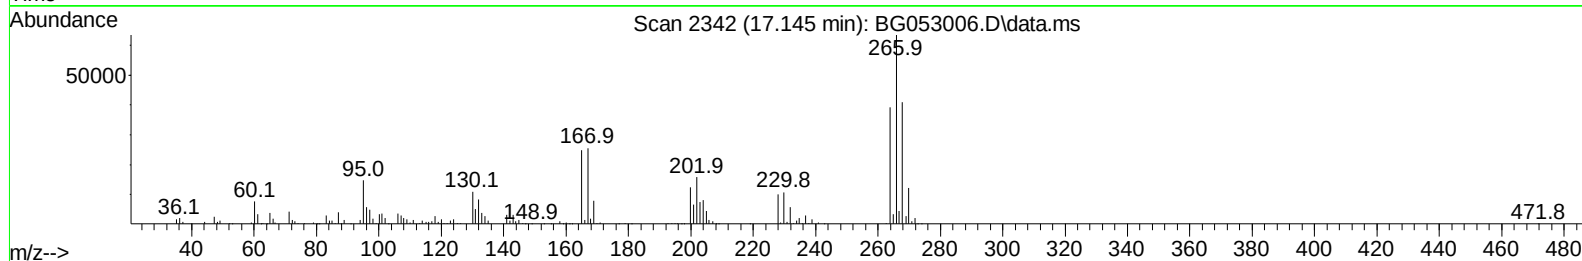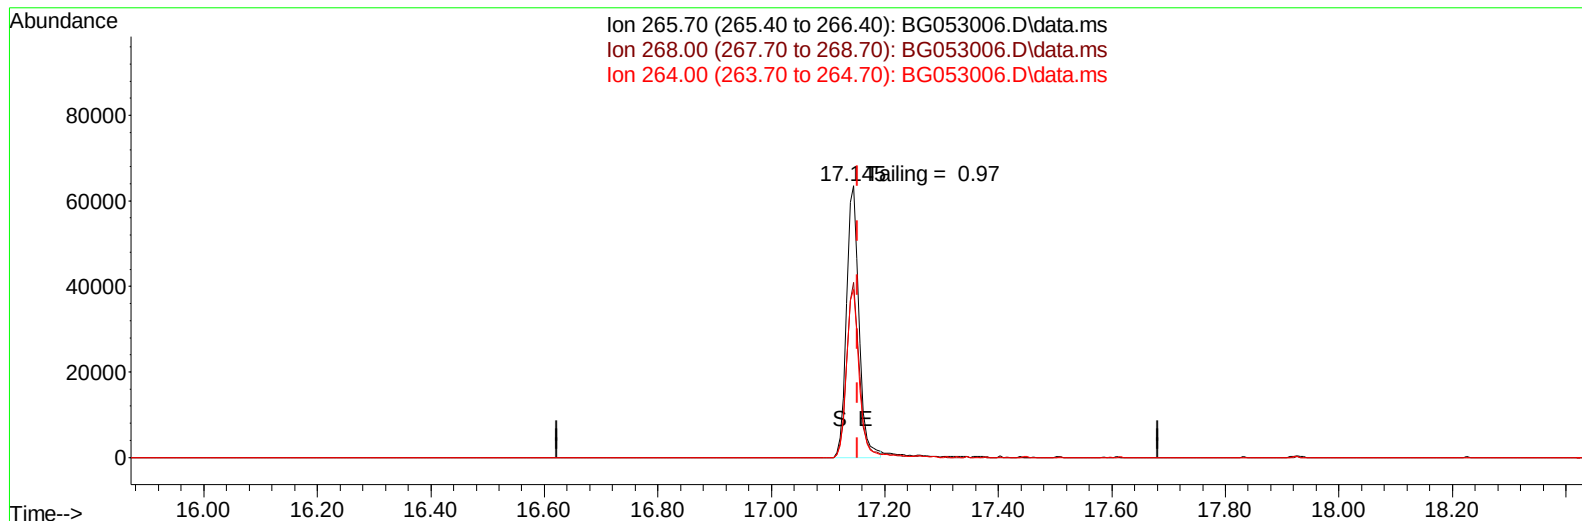

TIC: BG053006.D\data.ms

(70) Pentachlorophenol (C)

17.145min (-0.007) 24558.98 ng




response 99314

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.46
264.00	56.60	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040422\
 Data File : BG053006.D
 Acq On : 4 Apr 2022 13:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 02:30:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 24 16:48:57 2022
 Response via : Initial Calibration

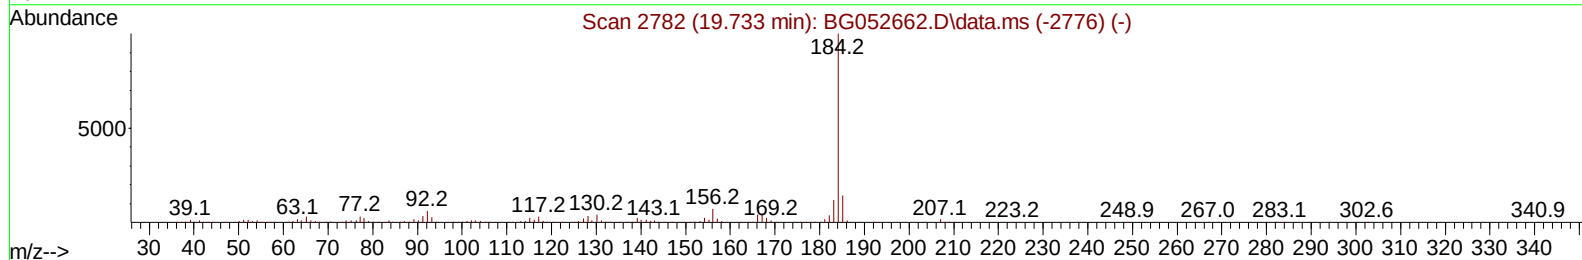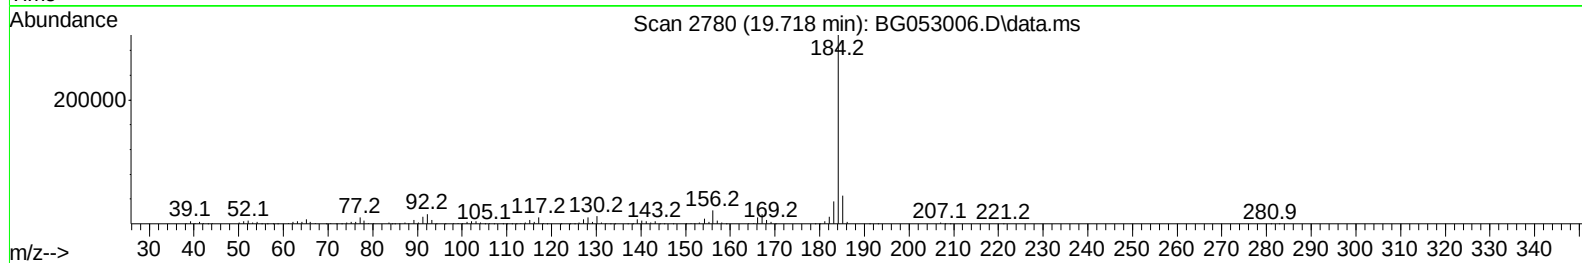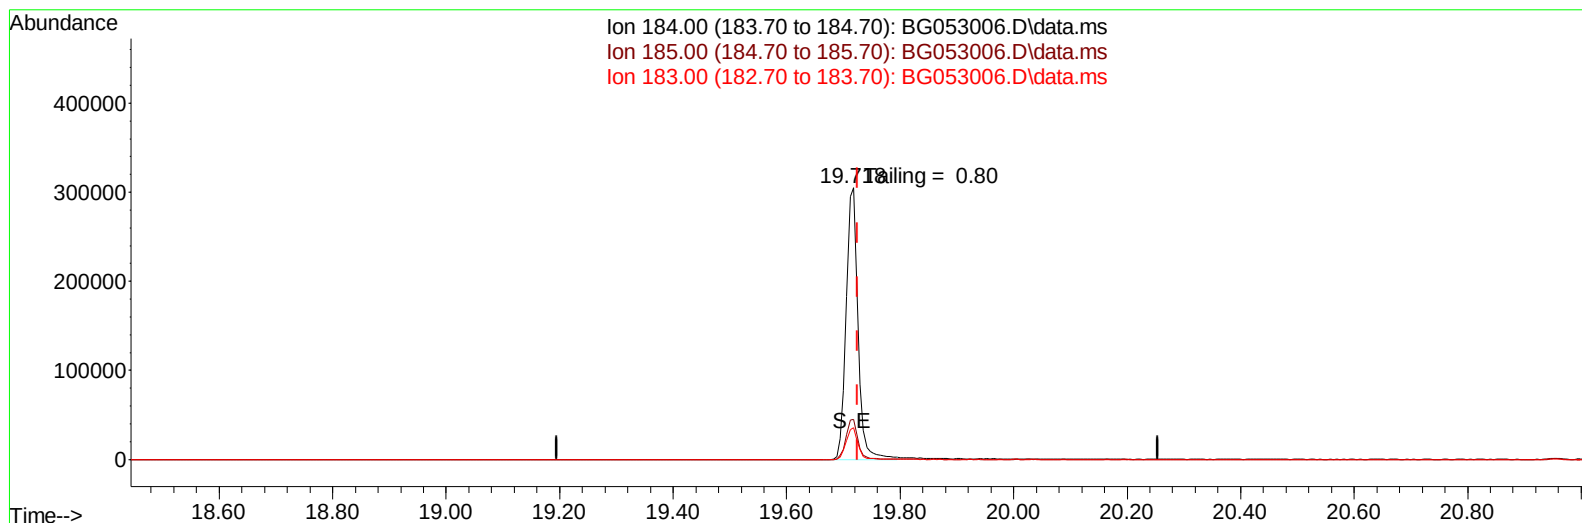

TIC: BG053006.D\data.ms

(77) Benzidine

19.718min (-0.007) 0.00 ng

response 450531

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.82
183.00	11.80	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2022	BNA_G	BG053006.D
Compound Name	Response	Retention Time
DDT	269471	20.957
DDD	7438	20.511
DDE	230	20.006
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7668	277139	2.77

Instrument :
BNA_G
ClientSampleId :
DFTPP