


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040423\
Data File : BG056958.D
Acq On : 4 Apr 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 03:23:11 2023

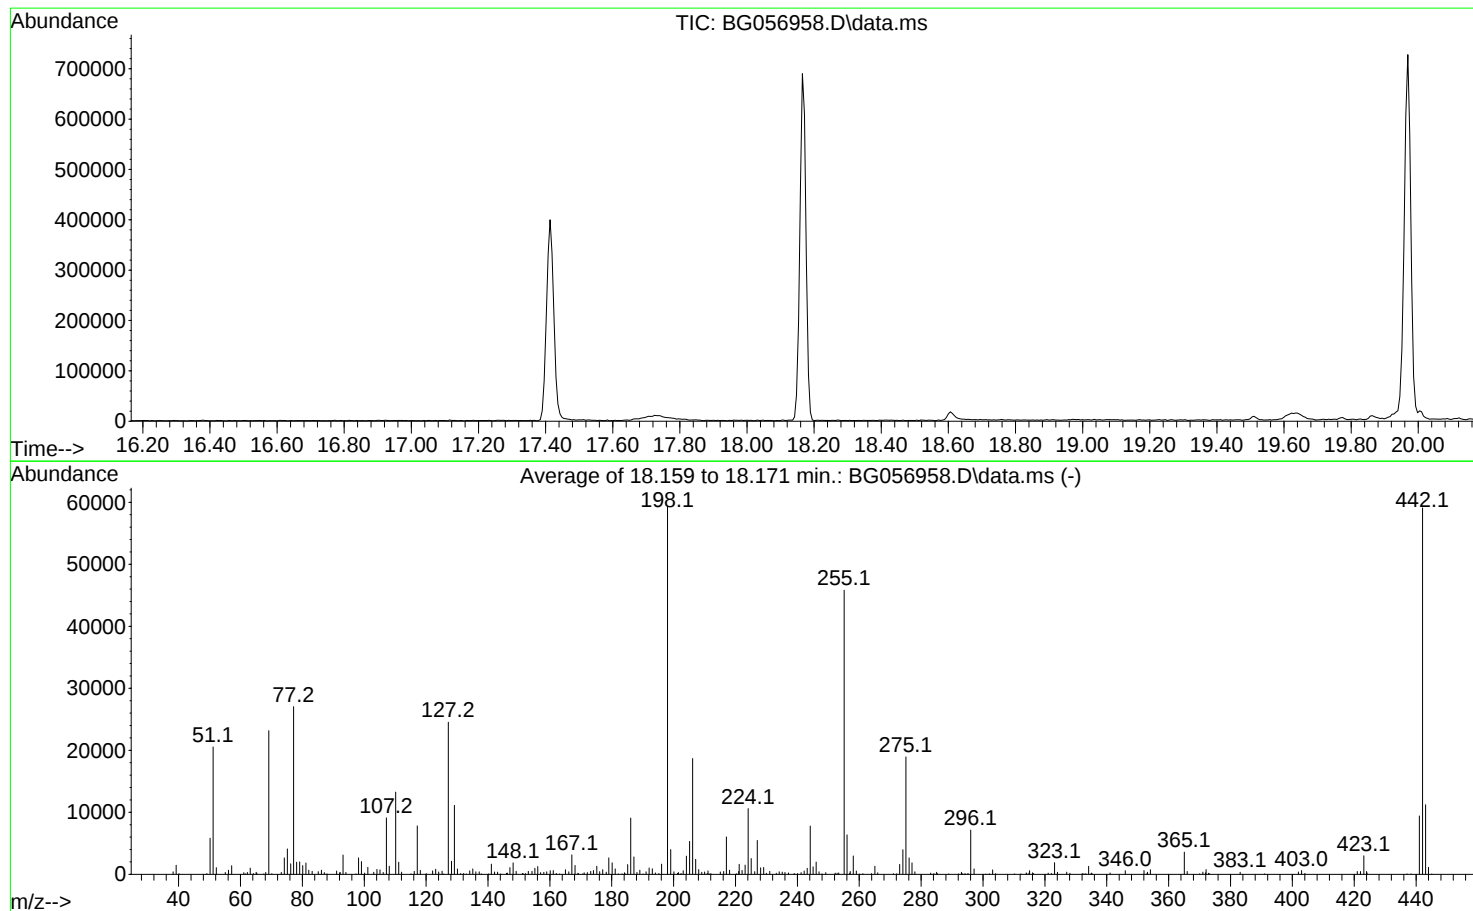




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	20536	PASS
68	69	0.00	2	1.3	302	PASS
69	198	0.00	100	39.0	23164	PASS
70	69	0.00	2	0.4	97	PASS
127	198	10	80	41.3	24533	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59341	PASS
199	198	5	9	6.7	3981	PASS
275	198	10	60	31.9	18942	PASS
365	198	1	100	6.0	3585	PASS
441	198	0.01	100	15.8	9398	PASS
442	442	50	100	100.0	59093	PASS
443	442	15	24	19.0	11216	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040423\
Data File : BG056958.D
Acq On : 4 Apr 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 05:56:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

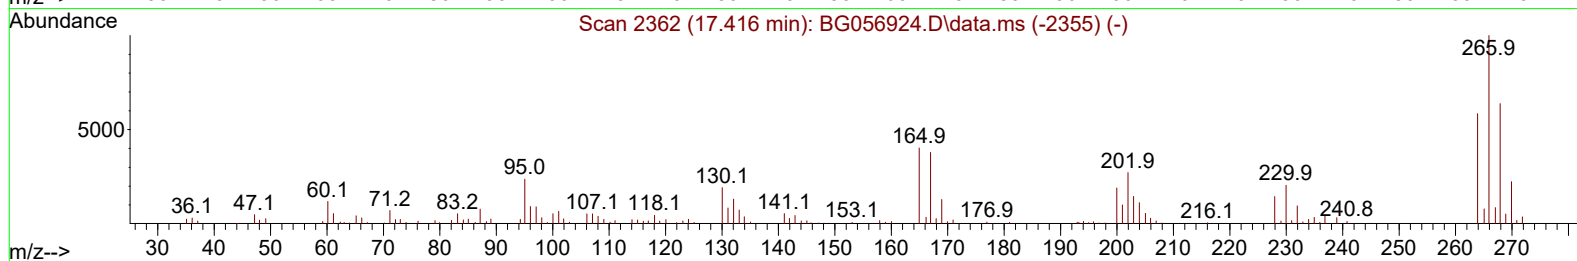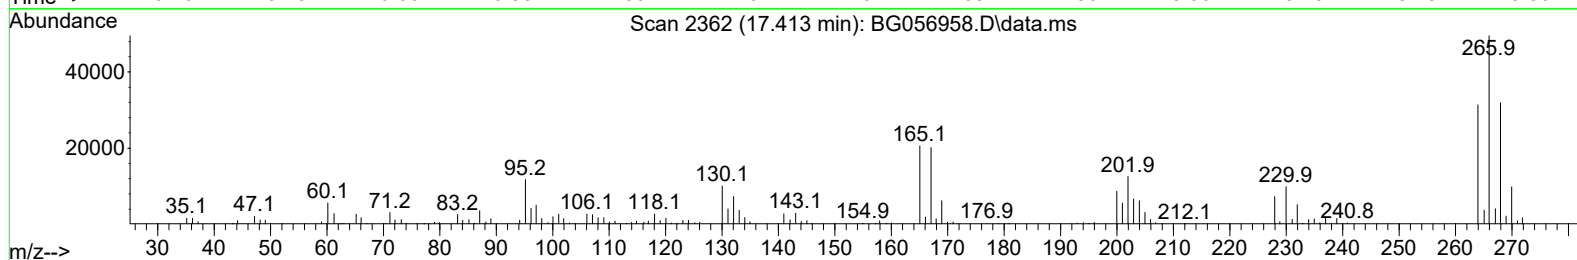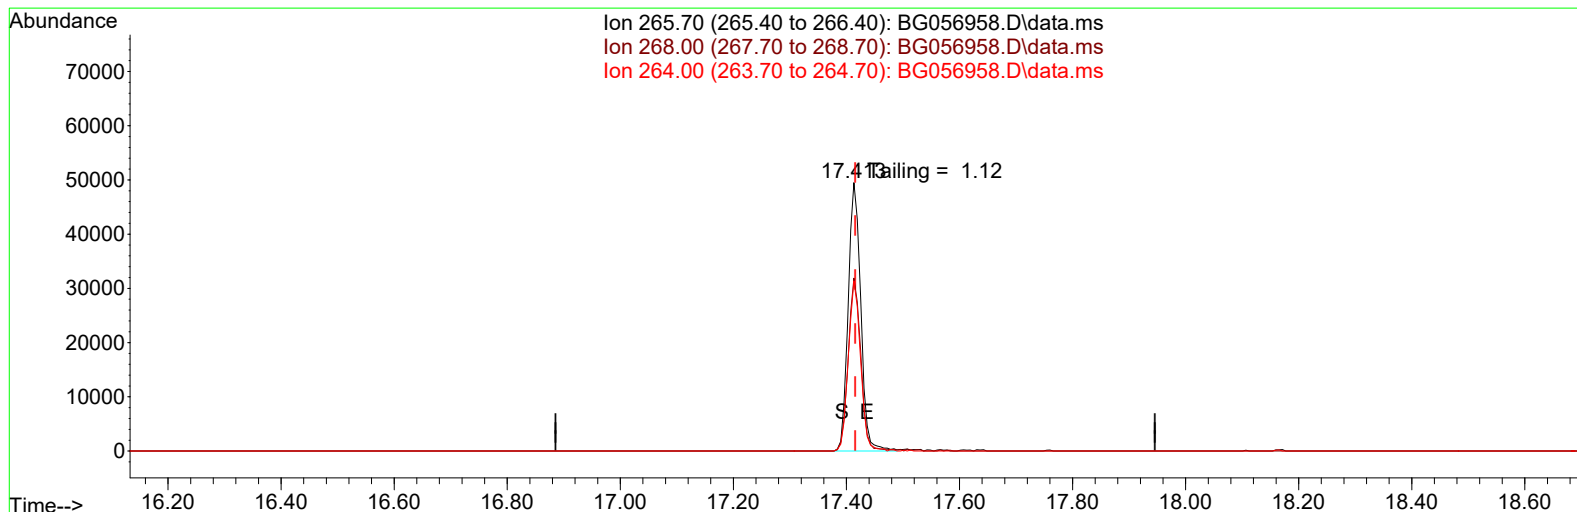

TIC: BG056958.D\data.ms

(70) Pentachlorophenol (C)

17.413min (-0.002) 26873.98 ng




response 76650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.41
264.00	58.50	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040423\
 Data File : BG056958.D
 Acq On : 4 Apr 2023 9:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 05:56:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 03:23:11 2023
 Response via : Initial Calibration

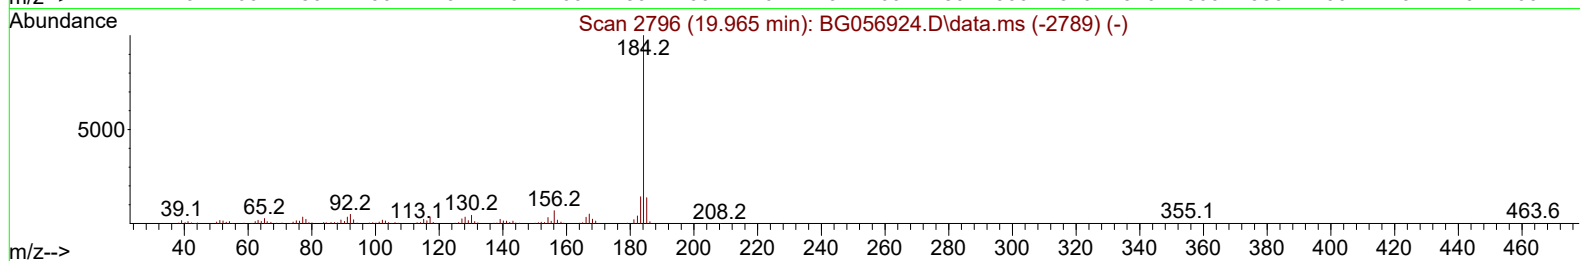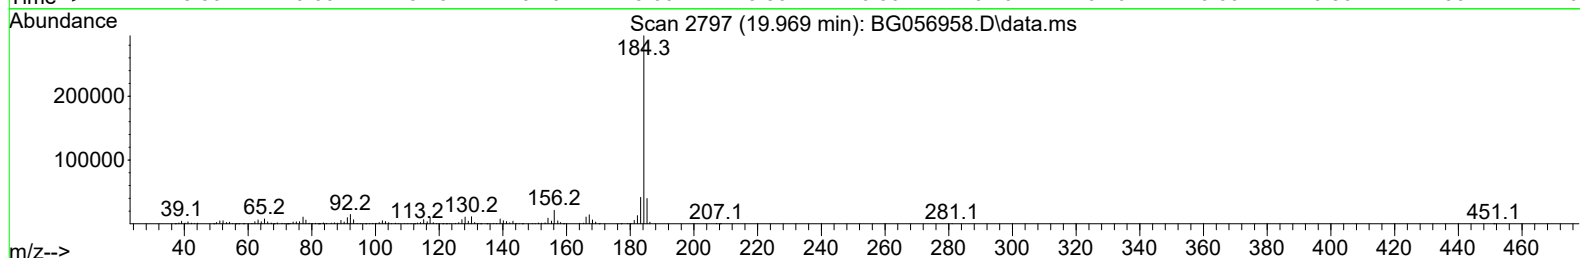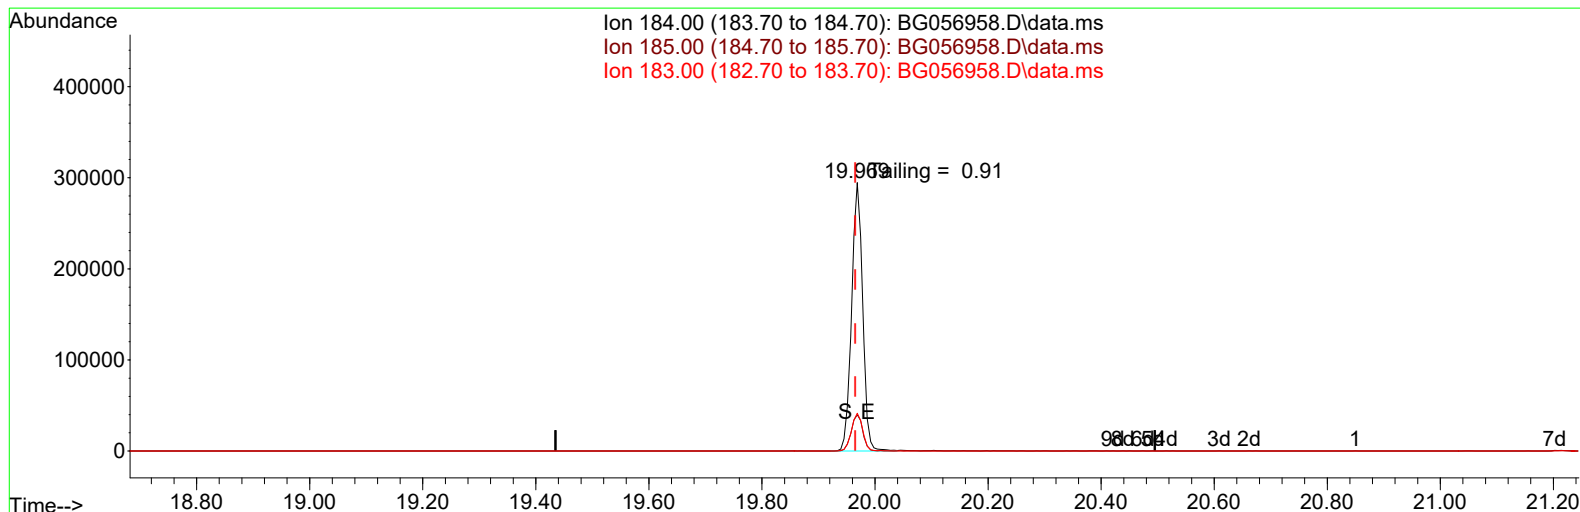

TIC: BG056958.D\data.ms

(77) Benzidine

19.969min (+ 0.004) 272647.73 ng m

response 402427

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.51
183.00	14.20	14.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2023	BNA_G	<u>BG056958.D</u>
Compound Name	Response	Retention Time
DDT	203179	21.214
DDD	3413	20.809
DDE	0	20.232
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3413	206592	1.65

Instrument :
BNA_G
ClientSampleId :
DFTPP