
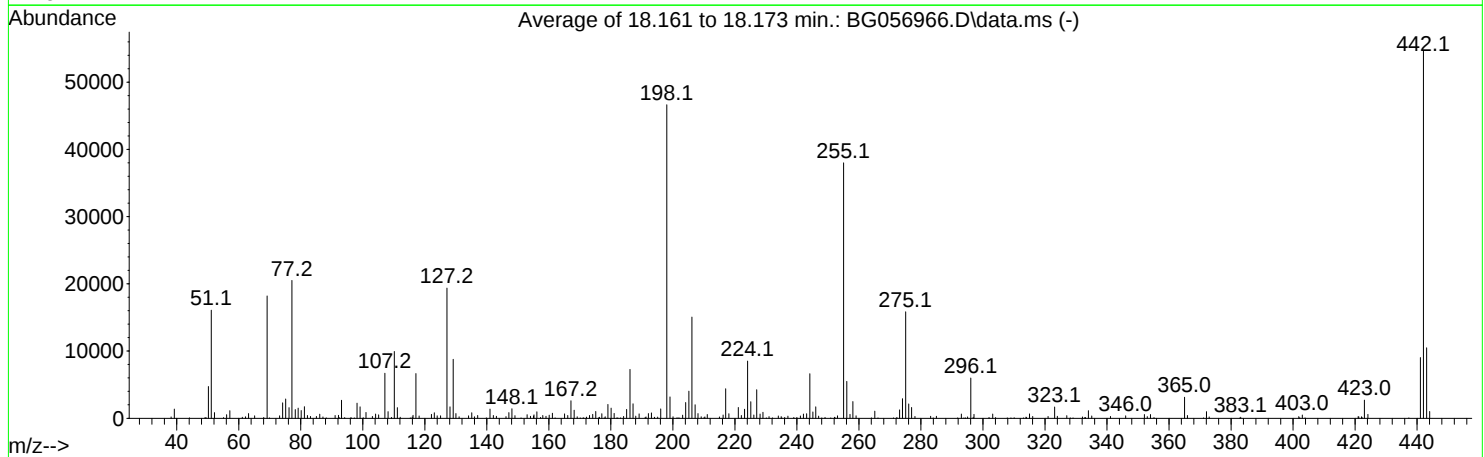


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040423\
Data File : BG056966.D
Acq On : 4 Apr 2023 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 03:23:11 2023

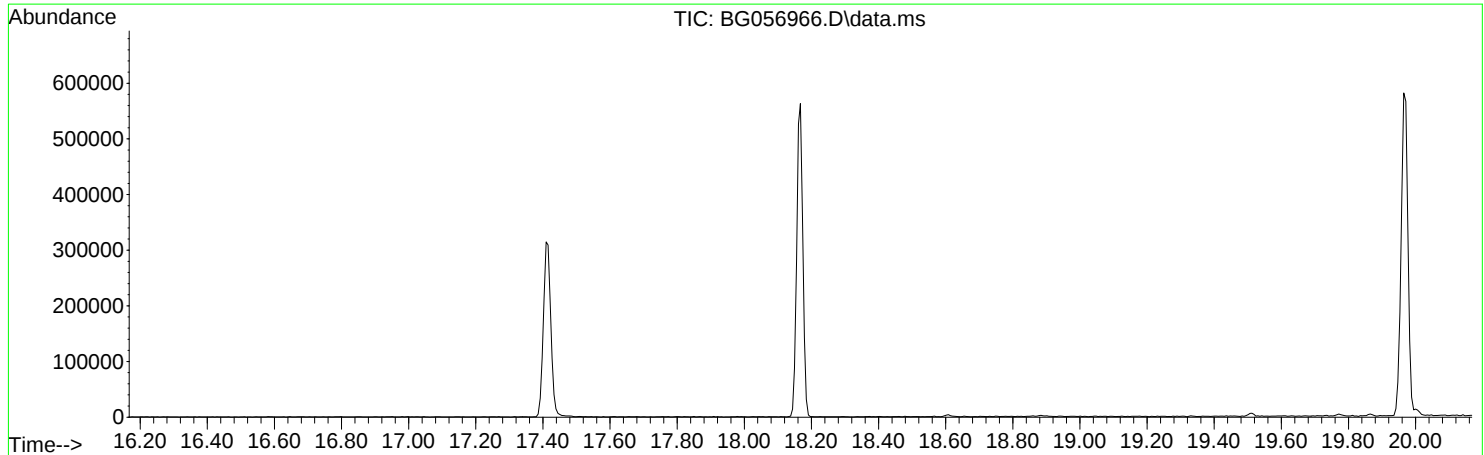




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	16077	PASS
68	69	0.00	2	0.7	122	PASS
69	198	0.00	100	39.0	18190	PASS
70	69	0.00	2	0.3	61	PASS
127	198	10	80	41.5	19366	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46629	PASS
199	198	5	9	6.8	3184	PASS
275	198	10	60	34.0	15845	PASS
365	198	1	100	6.7	3127	PASS
441	198	0.01	100	19.4	9025	PASS
442	442	50	100	100.0	54717	PASS
443	442	15	24	19.2	10483	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040423\
Data File : BG056966.D
Acq On : 4 Apr 2023 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 05:57:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

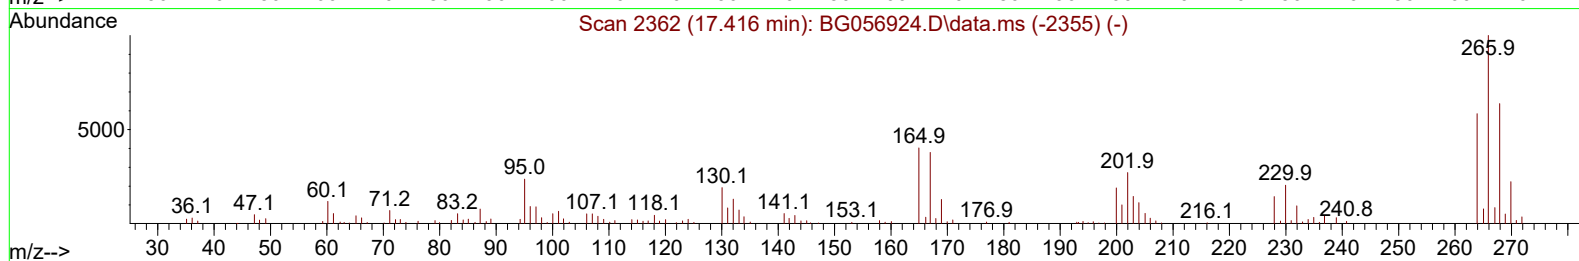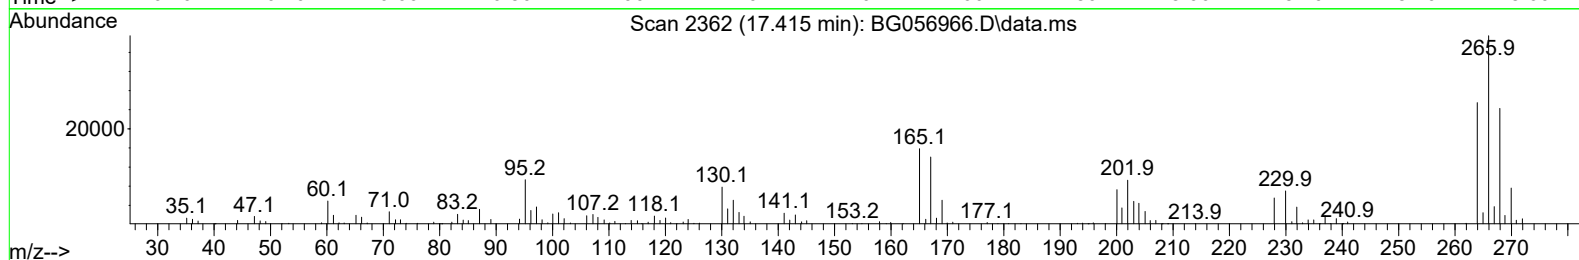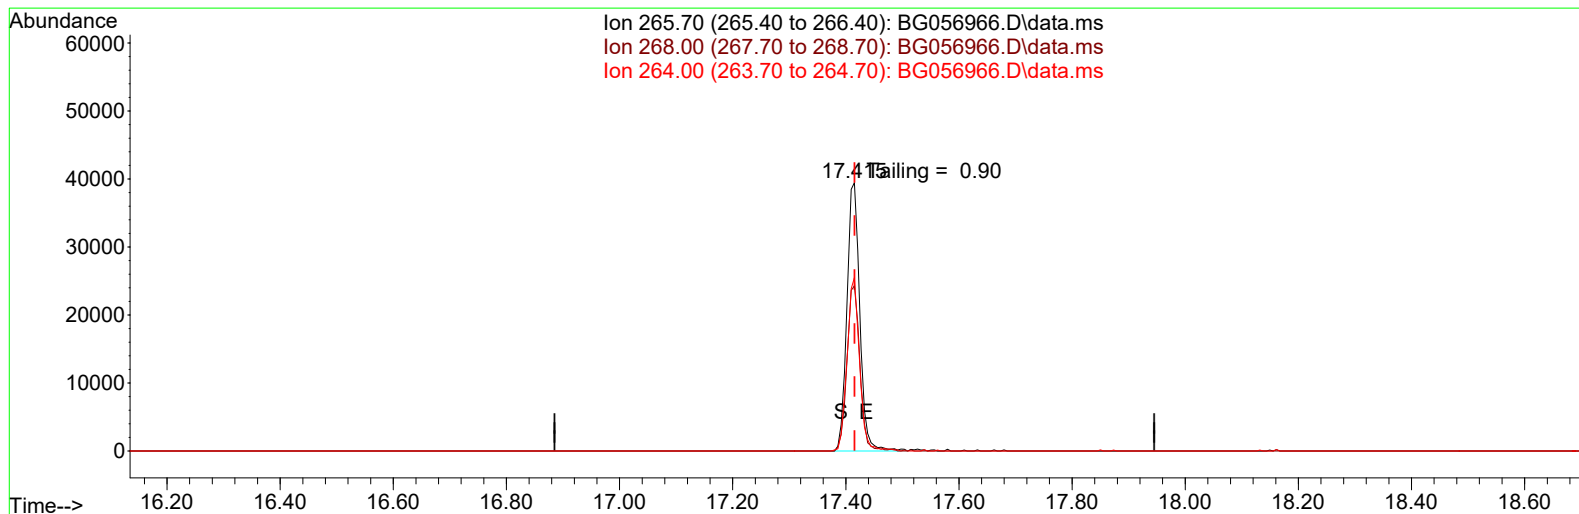

TIC: BG056966.D\data.ms

(70) Pentachlorophenol (C)

17.415min (-0.000) 20223.66 ng




response 62474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	61.53
264.00	58.50	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040423\
 Data File : BG056966.D
 Acq On : 4 Apr 2023 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 05:57:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 03:23:11 2023
 Response via : Initial Calibration

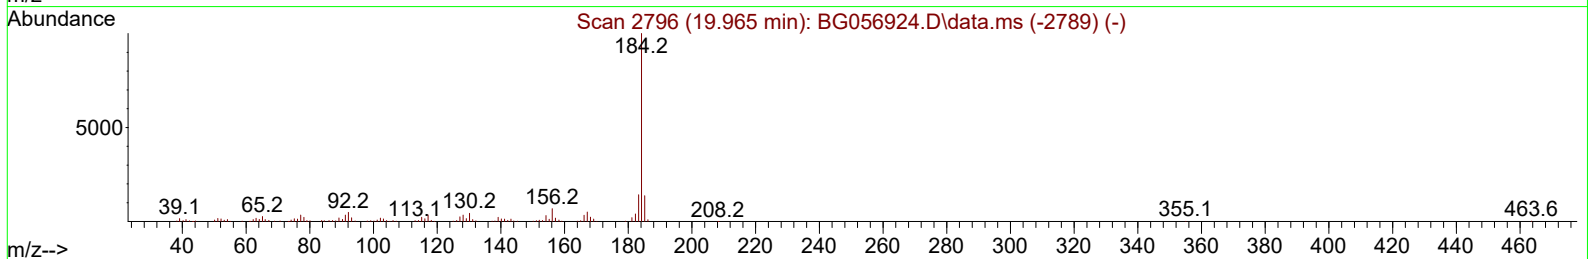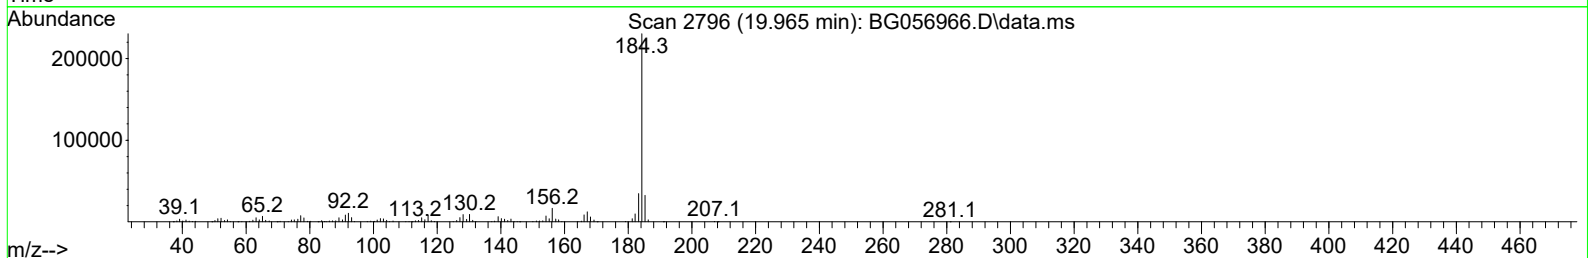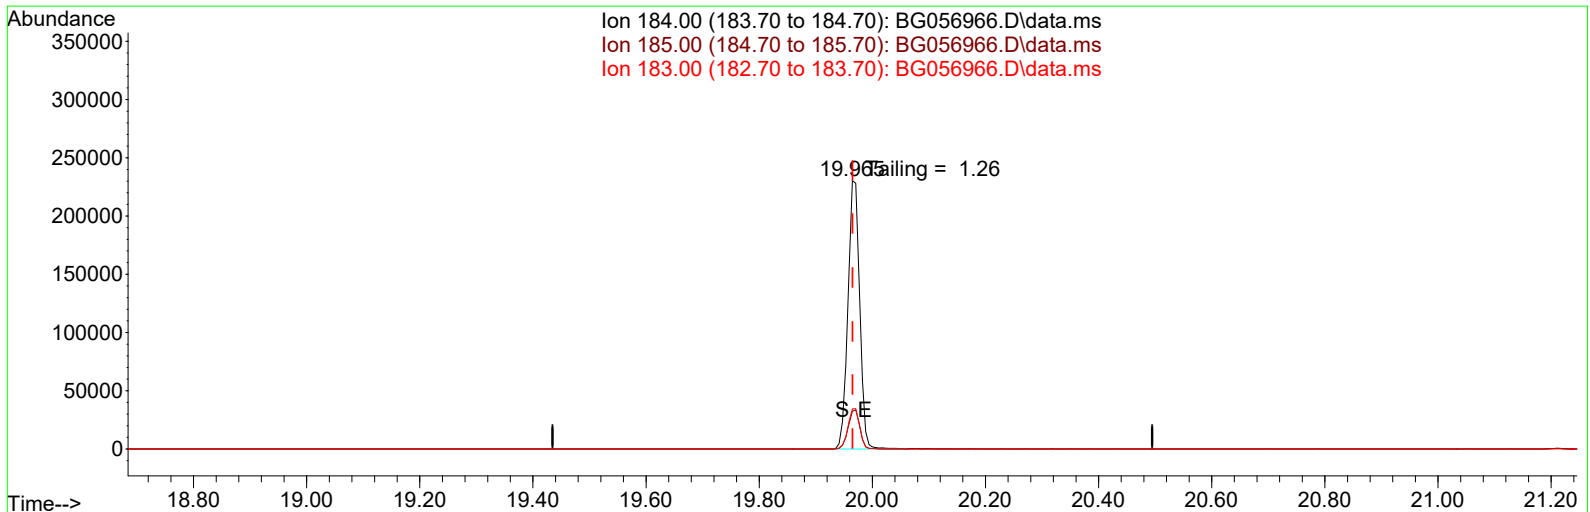

TIC: BG056966.D\data.ms

(77) Benzidine

19.965min (-0.000) 0.00 ng

response 333148

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.11
183.00	14.20	15.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2023	BNA_G	<u>BG056966.D</u>
Compound Name	Response	Retention Time
DDT	179164	21.21
DDD	3355	20.805
DDE		20.235
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3355	182519	1.84

Instrument :
BNA_G
ClientSampleId :
DFTPP