

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040517\
 Data File : BG026560.D
 Acq On : 5 Apr 2017 16:12
 Operator : SJ/MA
 Sample : PB98073TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 06 01:00:52 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 17:43:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	179542	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	712285	20.00	ng	-0.01
38) Acenaphthene-d10	14.65	164	412895	20.00	ng	-0.01
63) Phenanthrene-d10	17.38	188	1010107	20.00	ng	-0.01
75) Chrysene-d12	21.62	240	1196590	20.00	ng	-0.02
86) Perylene-d12	24.80	264	1152705	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	1303174	128.83	ng	0.00
7) Phenol-d6	7.20	99	1665489	122.64	ng	0.00
23) Nitrobenzene-d5	9.20	82	881771	74.44	ng	0.00
41) 2,4,6-Tribromophenol	16.13	330	704720	149.04	ng	-0.01
44) 2-Fluorobiphenyl	13.27	172	2438992	82.84	ng	-0.01
78) Terphenyl-d14	19.98	244	3442699	69.87	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040517\
Data File : BG026560.D
Acq On : 5 Apr 2017 16:12
Operator : SJ/MA
Sample : PB98073TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 06 01:00:52 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

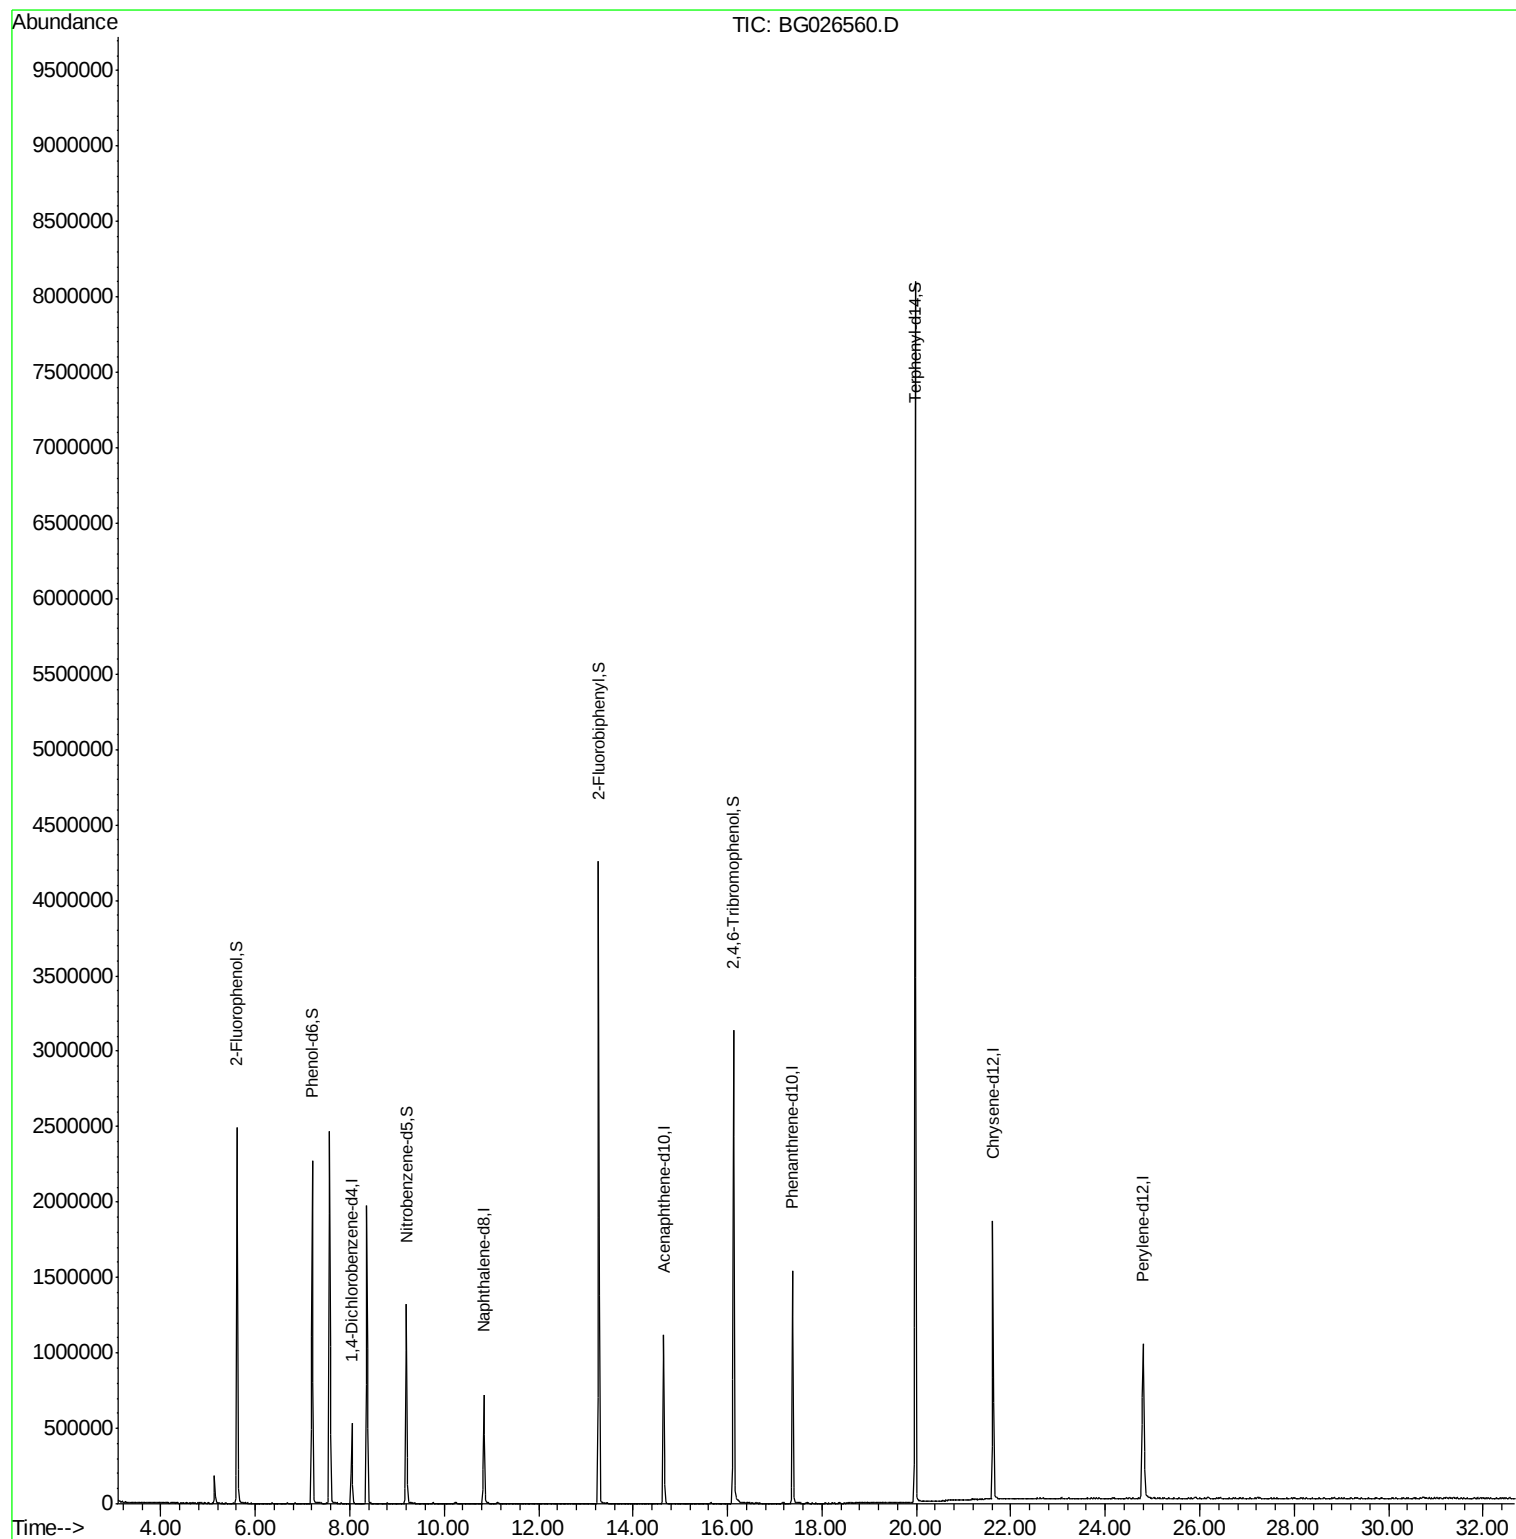

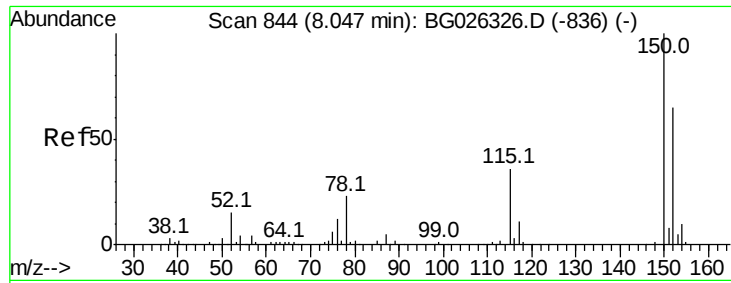


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.00 min
Lab File: BG026560.D
Acq: 5 Apr 2017 16:12

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 179542
Ion Ratio Lower Upper
152 100
150 156.0 114.0 171.0
115 53.2 48.1 72.1

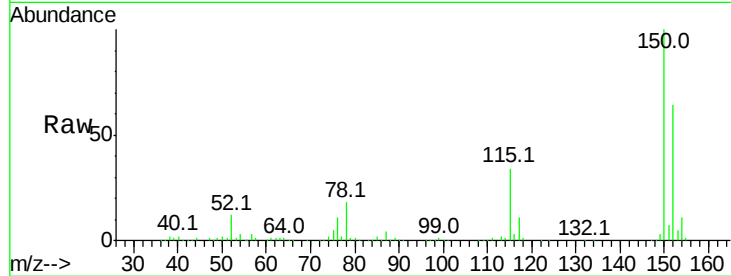


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

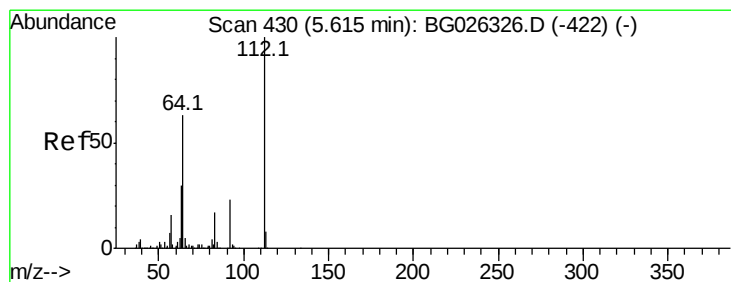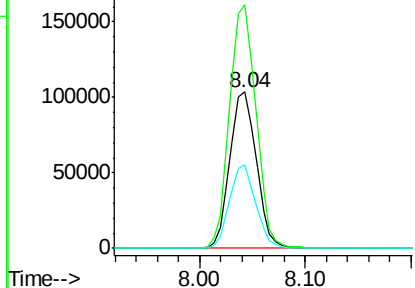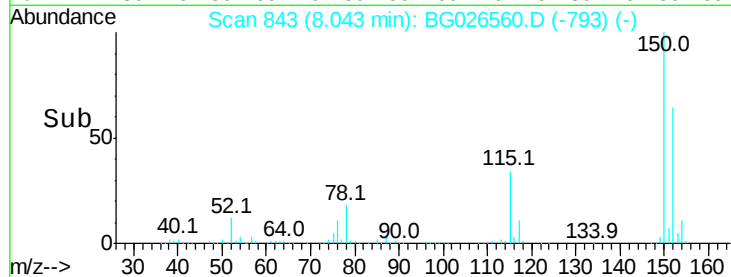



#5


2-Fluorophenol
Concen: 128.83 ng
RT: 5.62 min Scan# 430
Delta R.T. 0.00 min
Lab File: BG026560.D
Acq: 5 Apr 2017 16:12

Tgt Ion:112 Resp: 1303174
Ion Ratio Lower Upper
112 100
64 54.0 61.8 92.6#
63 26.9 37.2 55.8#

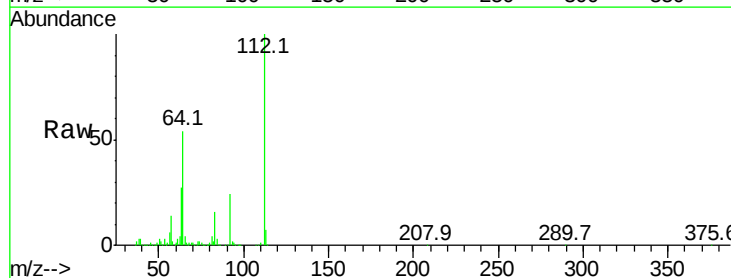

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

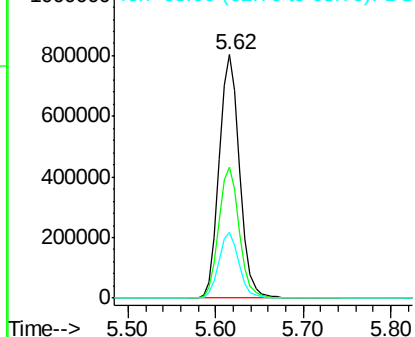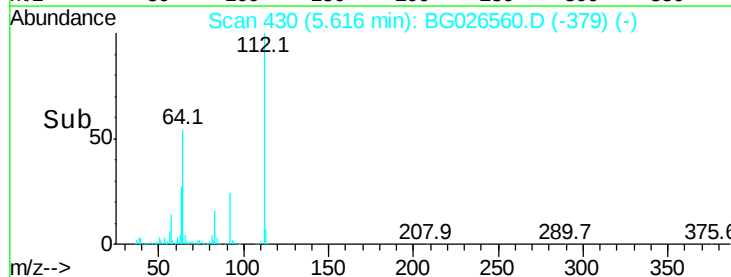

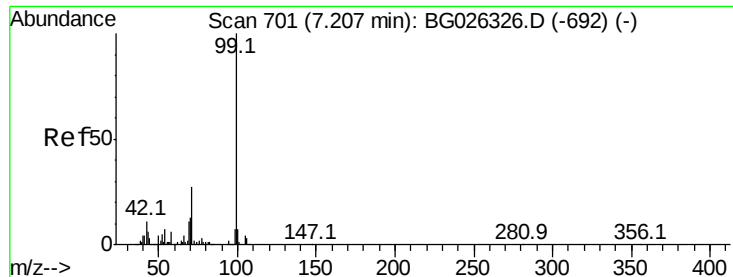

#7

Phenol-d6

Concen: 122.64 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.00 min

Lab File: BG026560.D

Acq: 5 Apr 2017 16:12

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 1665489

Ion Ratio Lower Upper

99 100

42 10.7 20.5 30.7#




71 26.2 37.6 56.4#

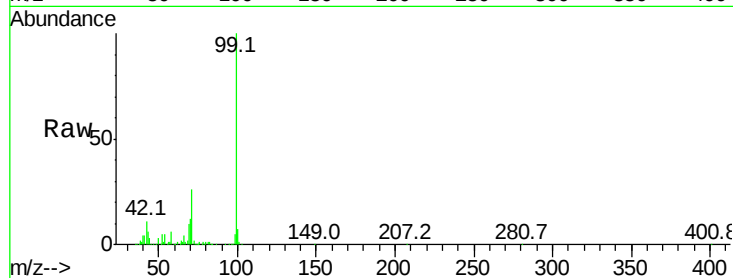

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

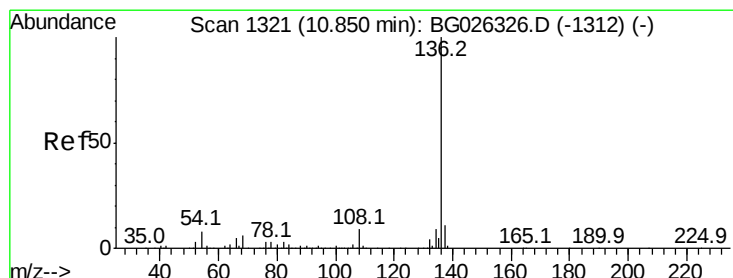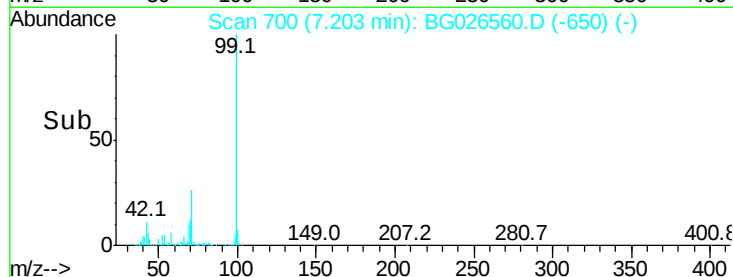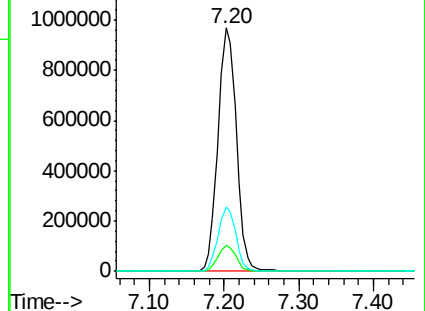

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.84 min Scan# 1319

Delta R.T. -0.01 min

Lab File: BG026560.D

Acq: 5 Apr 2017 16:12

Tgt Ion:136 Resp: 712285


Ion Ratio Lower Upper

136 100

137 10.7 8.9 13.3

54 5.9 9.3 13.9#

68 5.5 5.1 7.7


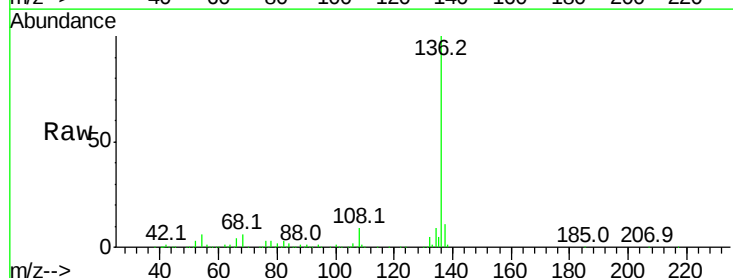



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



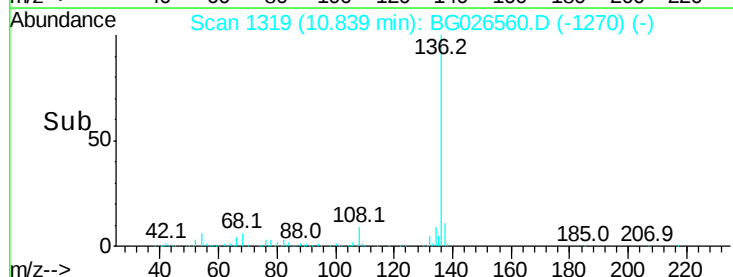
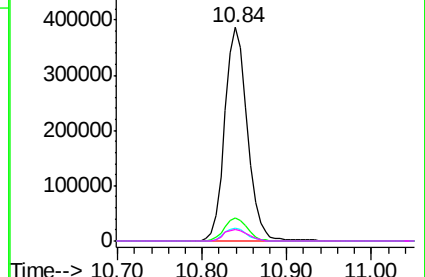


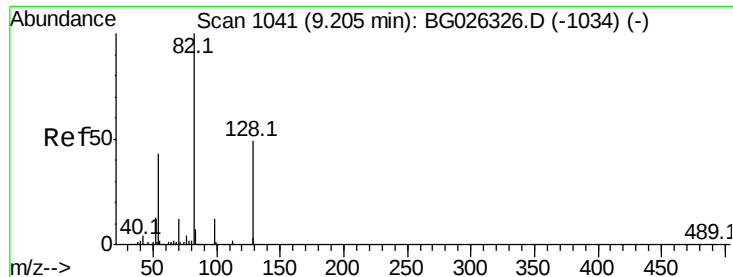

#23
 Nitrobenzene-d5
 Concen: 74.44 ng
 RT: 9.20 min Scan# 1040
 Delta R.T. -0.00 min
 Lab File: BG026560.D
 Acq: 5 Apr 2017 16:12




Instrument :
 BNA_G
 ClientSampleID :


Tot Ion: 82 Resp: 881771
 Ion Ratio Lower Upper
 82 100
 128 55.2 26.4 39.6#
 54 40.9 49.4 74.2#

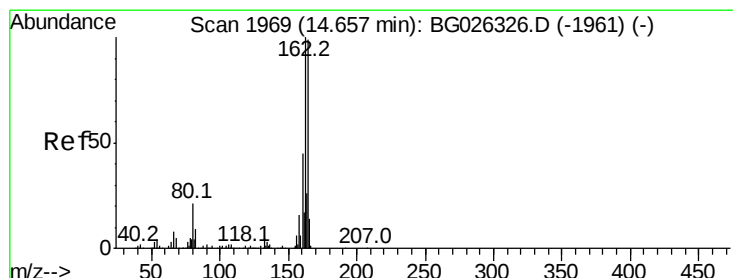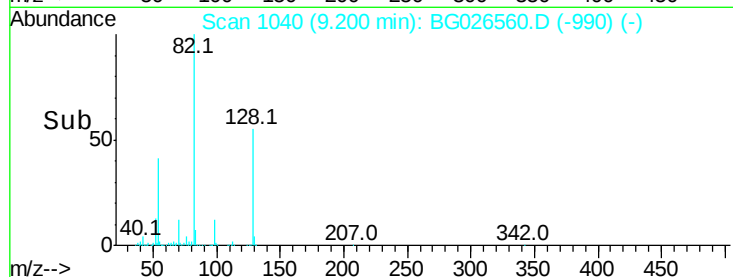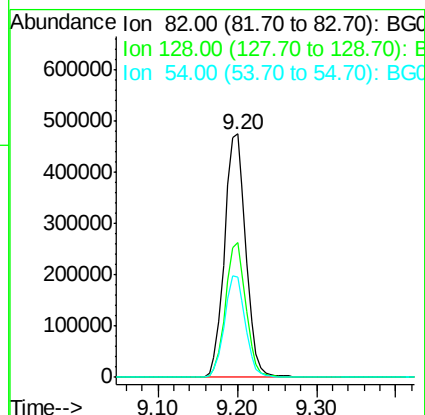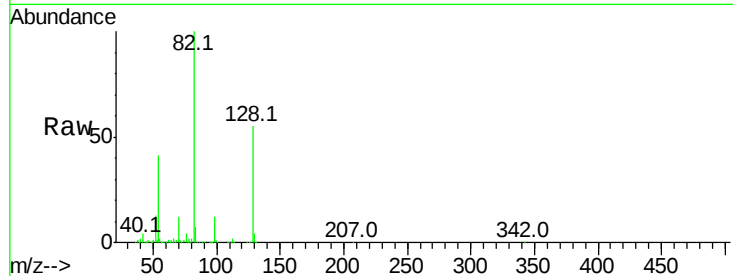

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.65 min Scan# 1967
 Delta R.T. -0.01 min
 Lab File: BG026560.D
 Acq: 5 Apr 2017 16:12

Tgt Ion:164 Resp: 412895
 Ion Ratio Lower Upper
 164 100
 162 102.4 85.1 127.7
 160 46.9 34.7 52.1

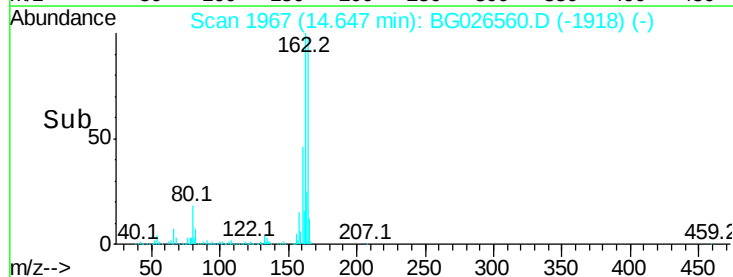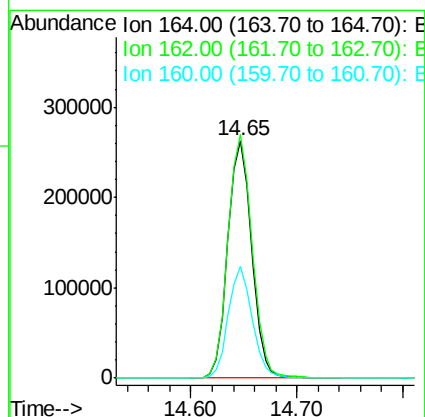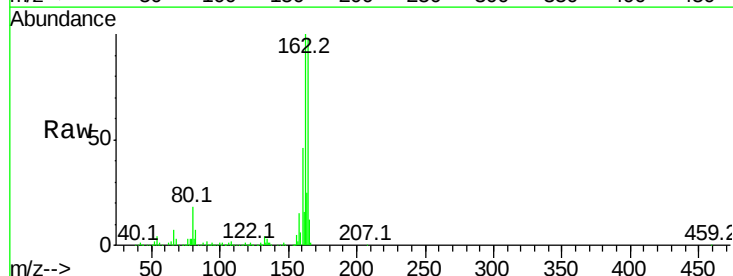


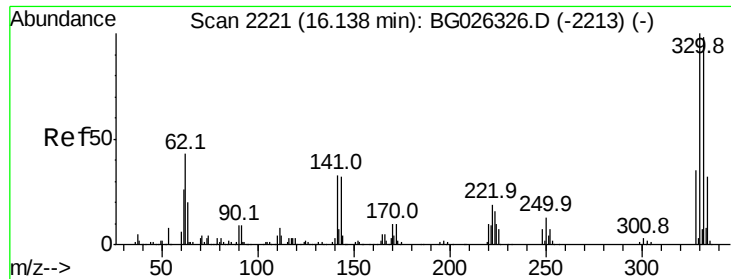




#41
 2,4,6-Tribromophenol
 Concen: 149.04 ng
 RT: 16.13 min Scan# 2219
 Delta R.T. -0.01 min
 Lab File: BG026560.D
 Acq: 5 Apr 2017 16:12

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:330 Resp: 704720
 Ion Ratio Lower Upper
 330 100
 332 98.1 77.3 115.9
 141 29.6 32.1 48.1#

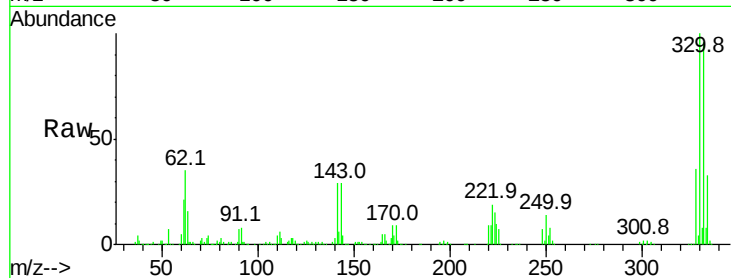


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

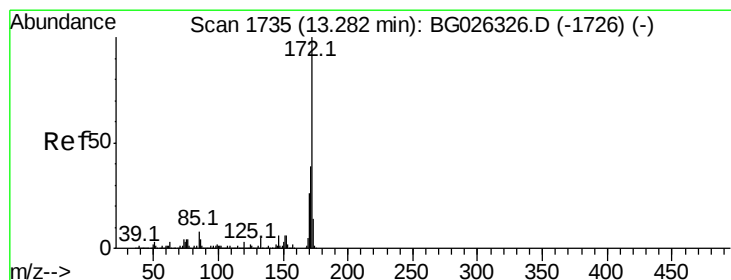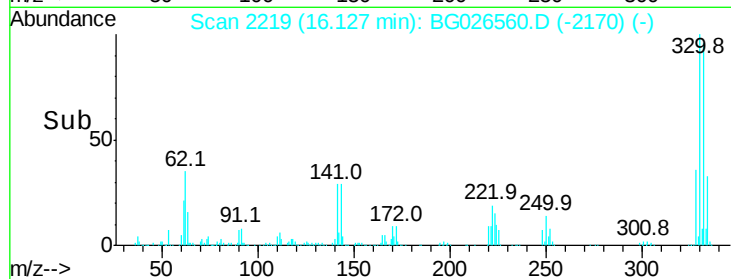
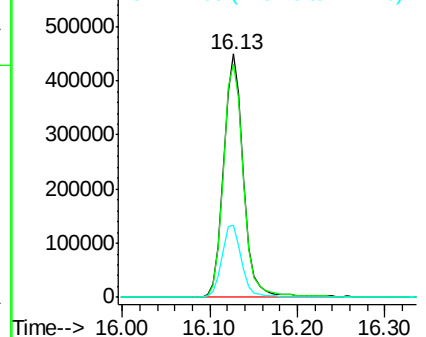



#44
 2-Fluorobiphenyl
 Concen: 82.84 ng
 RT: 13.27 min Scan# 1733
 Delta R.T. -0.01 min
 Lab File: BG026560.D
 Acq: 5 Apr 2017 16:12

Tgt Ion:172 Resp: 2438992
 Ion Ratio Lower Upper
 172 100
 171 39.4 32.2 48.2
 170 25.8 21.8 32.6

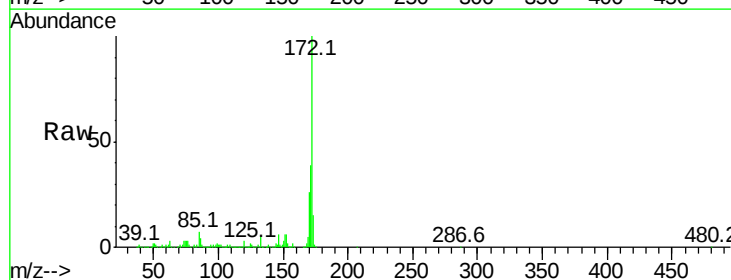

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

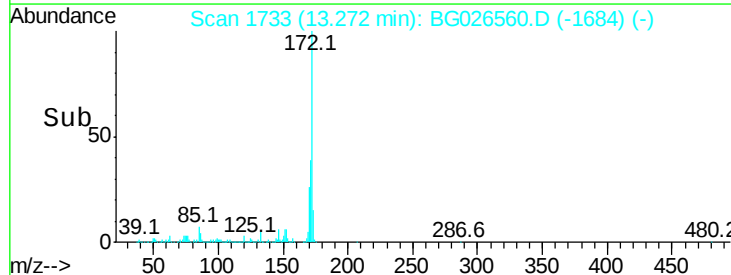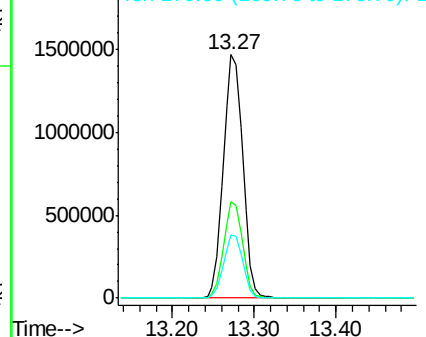


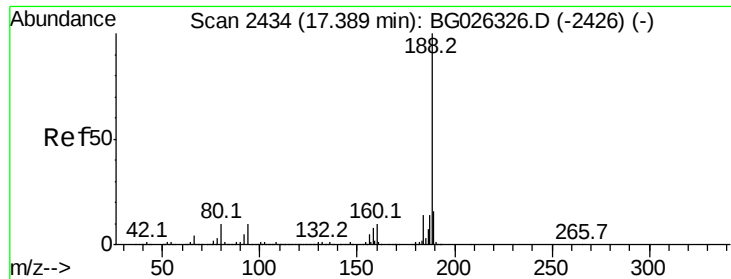




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.38 min Scan# 2432
Delta R.T. -0.01 min
Lab File: BG026560.D
Acq: 5 Apr 2017 16:12

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 1010107
Ion Ratio Lower Upper
188 100
94 9.0 5.8 8.8#
80 9.1 7.5 11.3

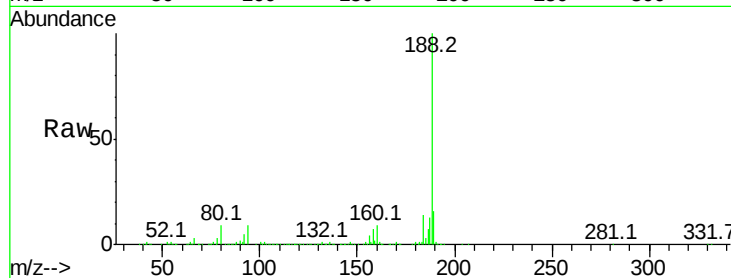


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

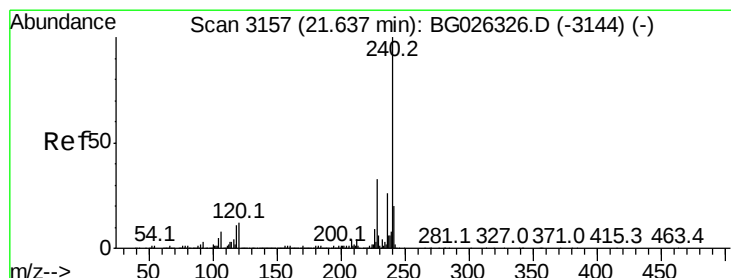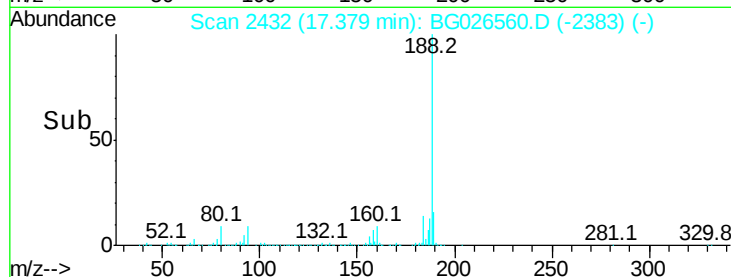
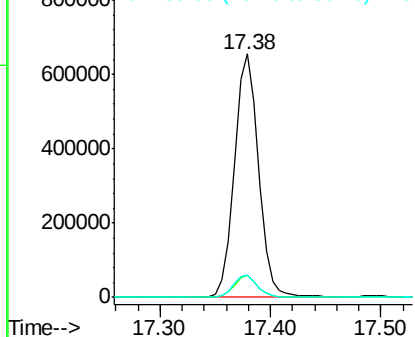



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.62 min Scan# 3154
Delta R.T. -0.02 min
Lab File: BG026560.D
Acq: 5 Apr 2017 16:12

Tgt Ion:240 Resp: 1196590
Ion Ratio Lower Upper
240 100
120 11.3 5.7 8.5#
236 26.5 22.2 33.4

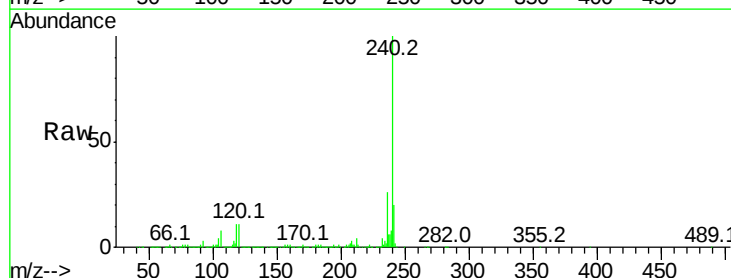

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

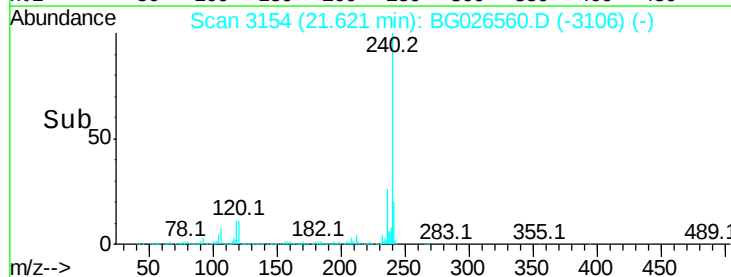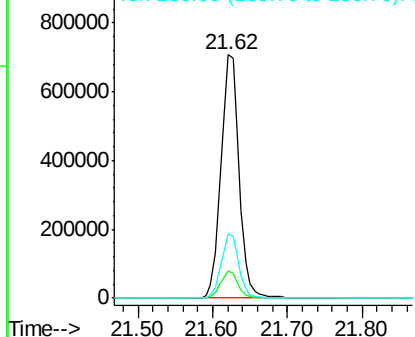

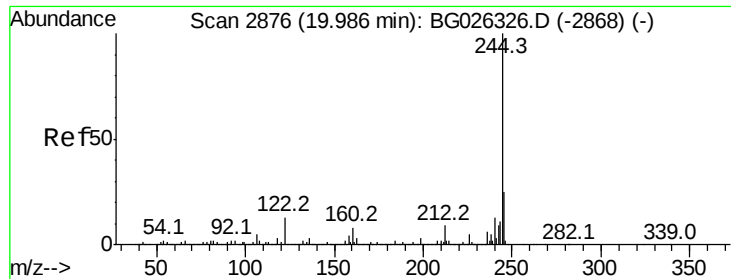

#78

Terphenyl-d14

Concen: 69.87 ng

RT: 19.98 min Scan# 2874

Delta R.T. -0.01 min

Lab File: BG026560.D

Acq: 5 Apr 2017 16:12

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 3442699

Ion Ratio Lower Upper




244 100

212 9.5 10.0 15.0#

122 14.1 8.6 12.8#

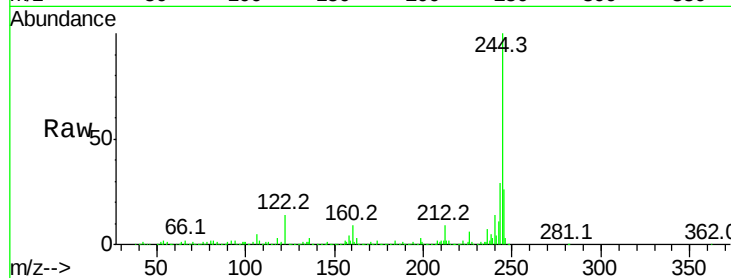

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

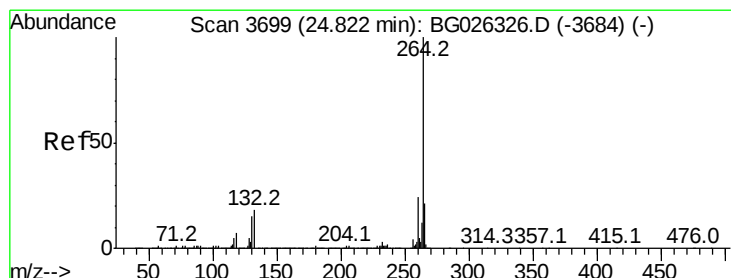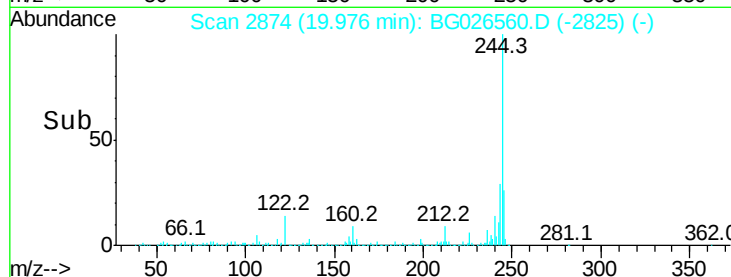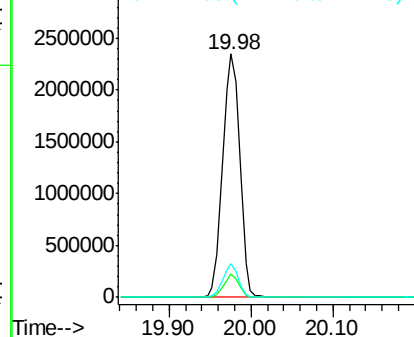

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.80 min Scan# 3695

Delta R.T. -0.02 min

Lab File: BG026560.D

Acq: 5 Apr 2017 16:12


Tgt Ion:264 Resp: 1152705

Ion Ratio Lower Upper

264 100

260 23.5 21.8 32.8

265 22.3 18.2 27.4

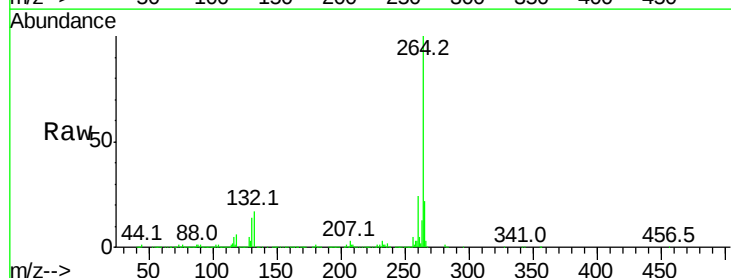

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

