
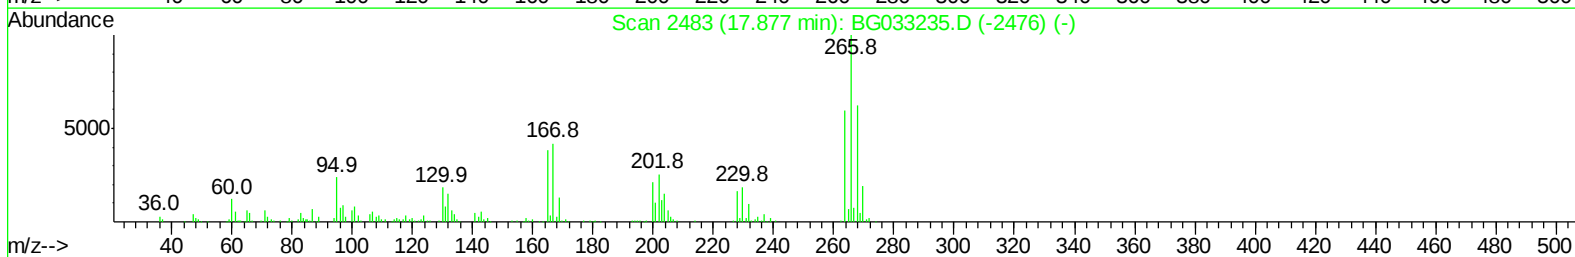
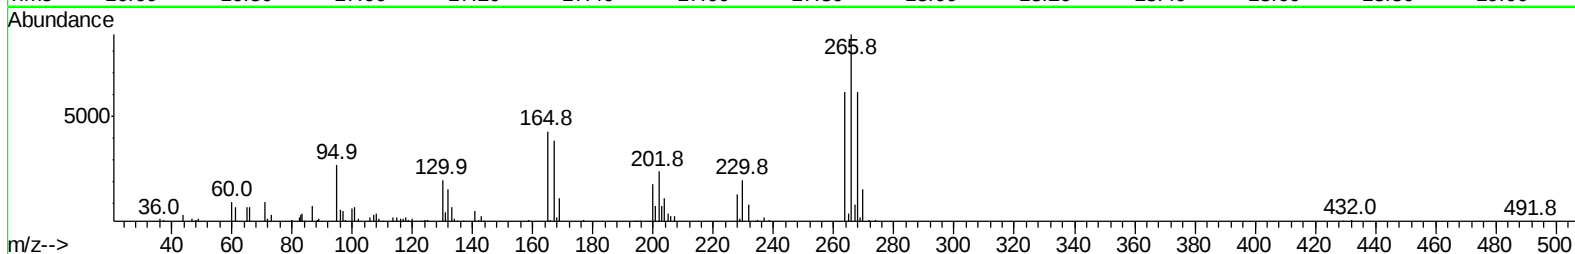


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040518\
Data File : BG033590.D
Acq On : 5 Apr 2018 13:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:20:34 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

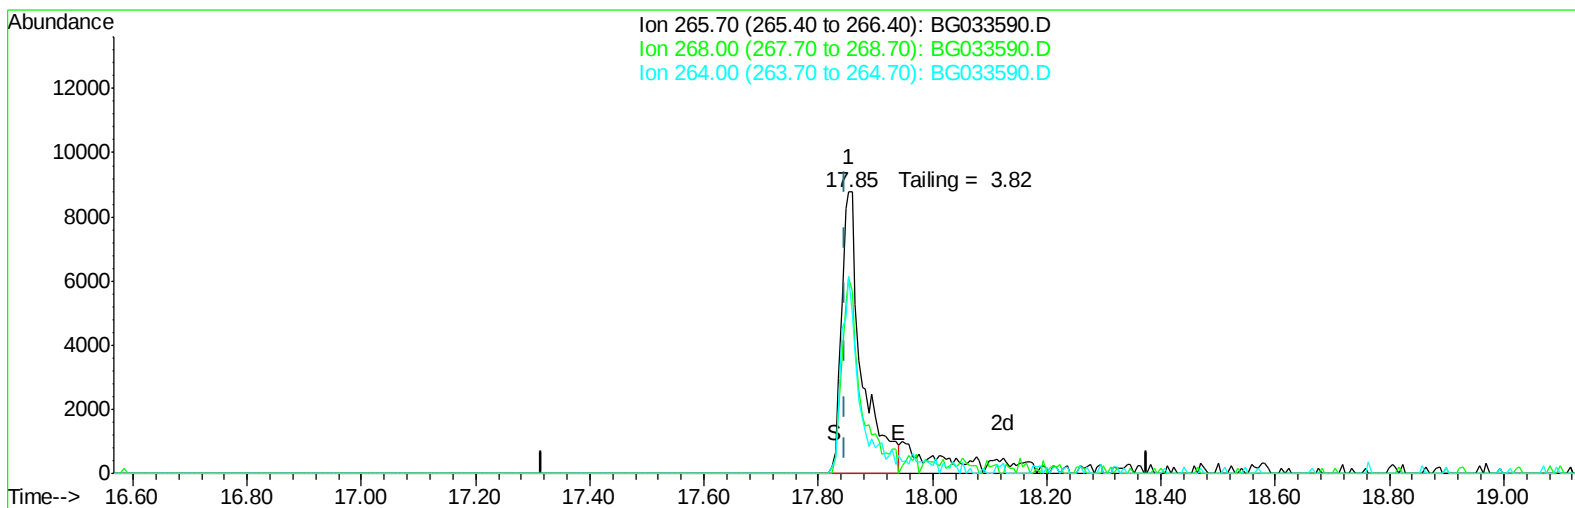

TIC: BG033590.D

(69) Pentachlorophenol (C)




17.853min (+0.006) 28174.18ng

response 22050

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	73.77
264.00	62.00	69.80
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040518\
Data File : BG033590.D
Acq On : 5 Apr 2018 13:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:20:34 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

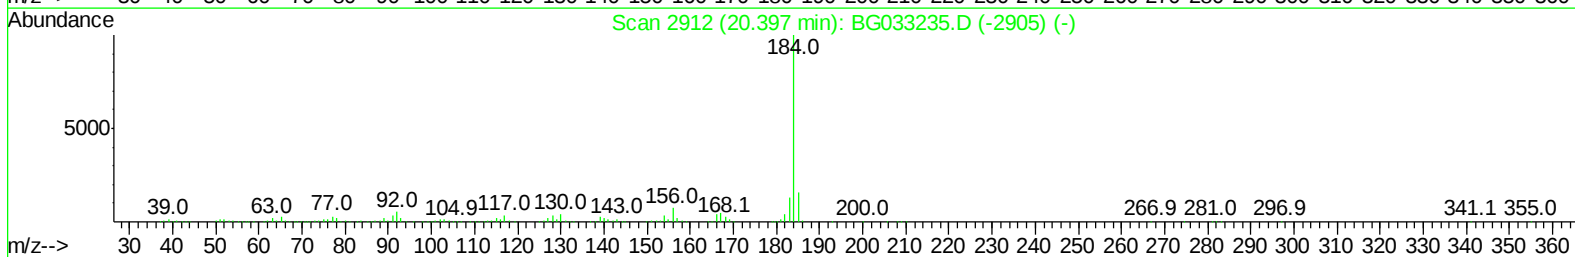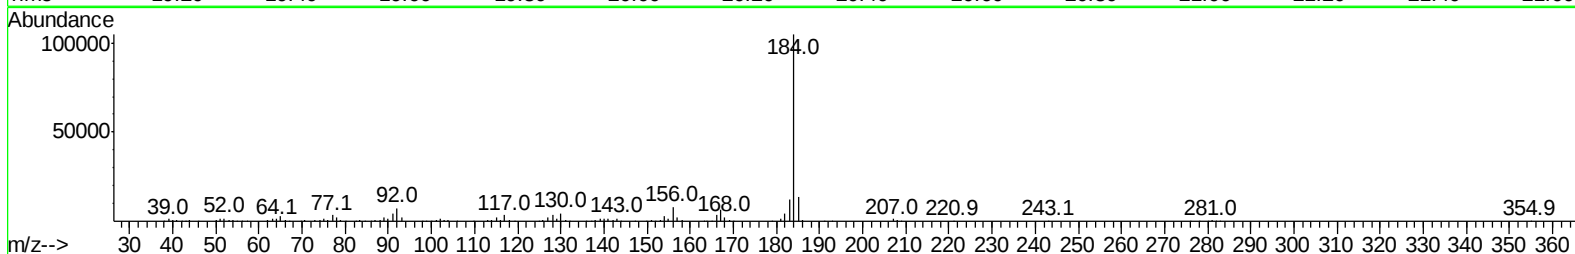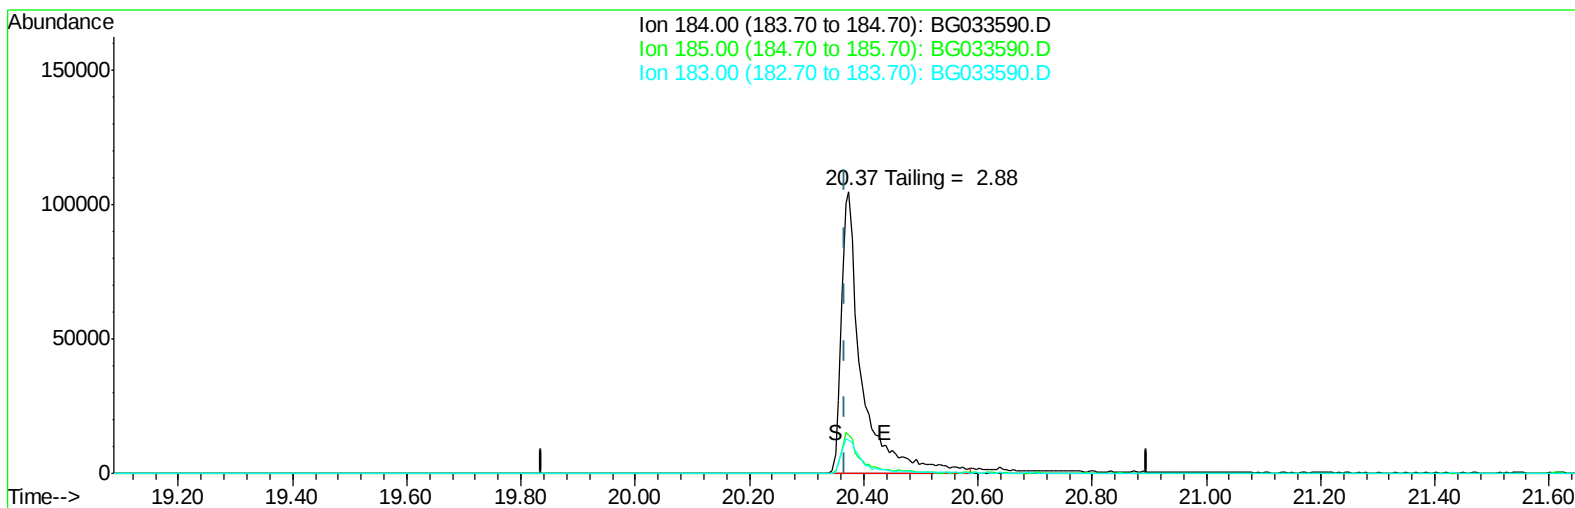

TIC: BG033590.D

(76) Benzidine

20.374min (+0.006) 157837.18ng

response 261099

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.48
183.00	13.30	11.79
0.00	0.00	0.00