
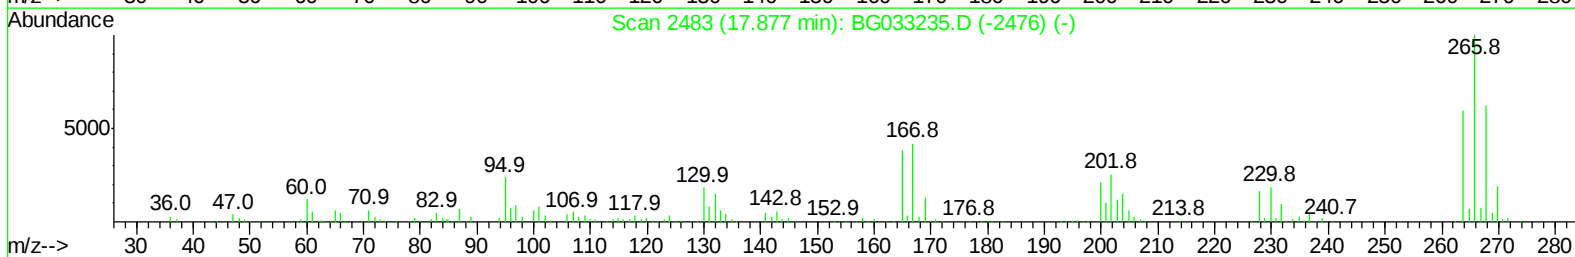
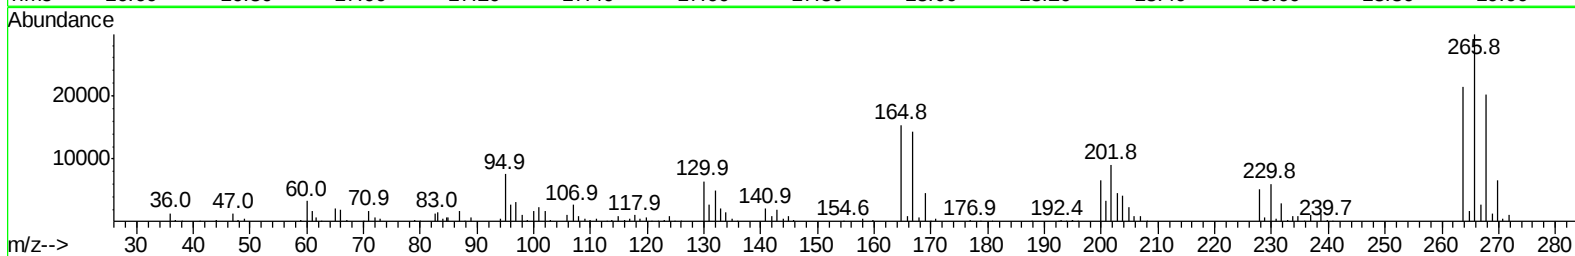


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040518\
Data File : BG033609.D
Acq On : 6 Apr 2018 1:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:21:37 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

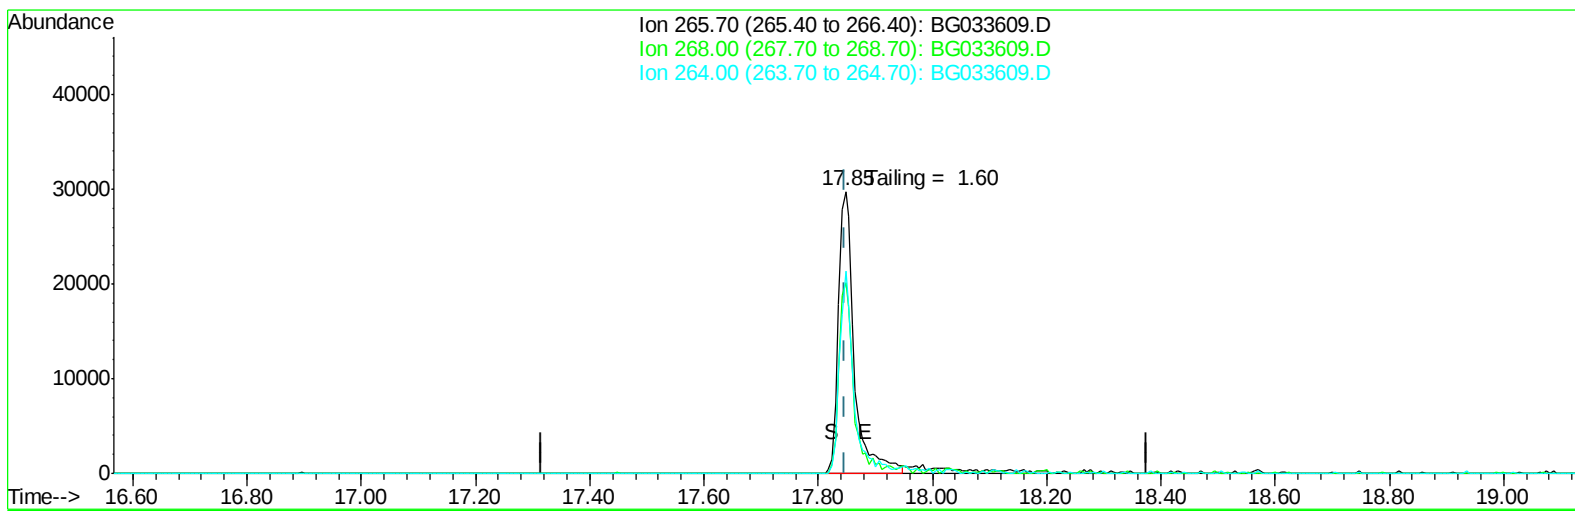

TIC: BG033609.D

(69) Pentachlorophenol (C)




17.848min (+0.000) 12082.61ng

response 57868

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.88
264.00	62.00	71.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040518\
Data File : BG033609.D
Acq On : 6 Apr 2018 1:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:21:37 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 05 17:36:07 2018
Response via : Initial Calibration

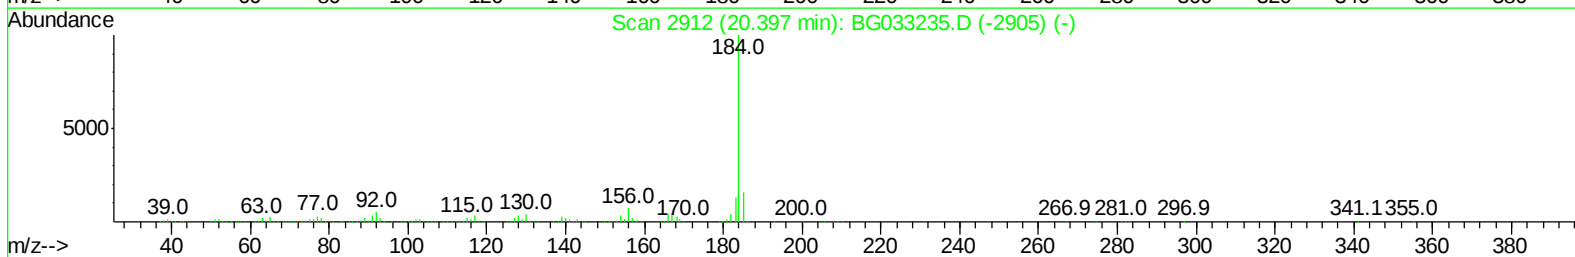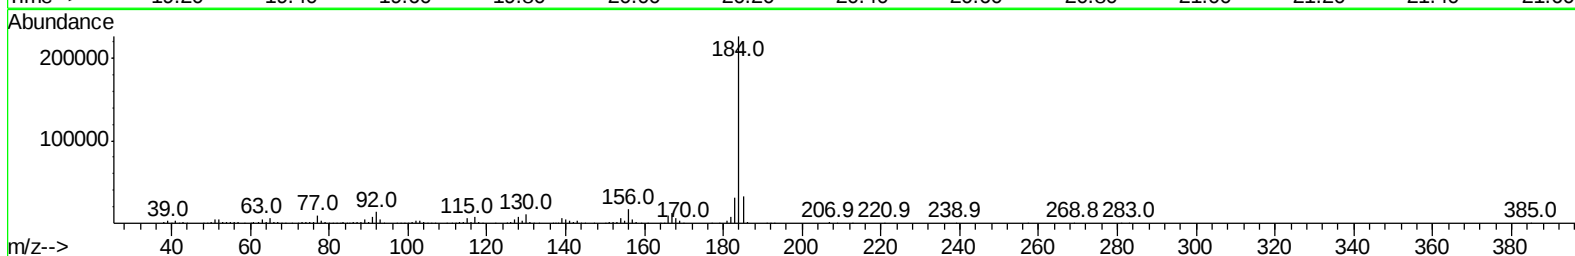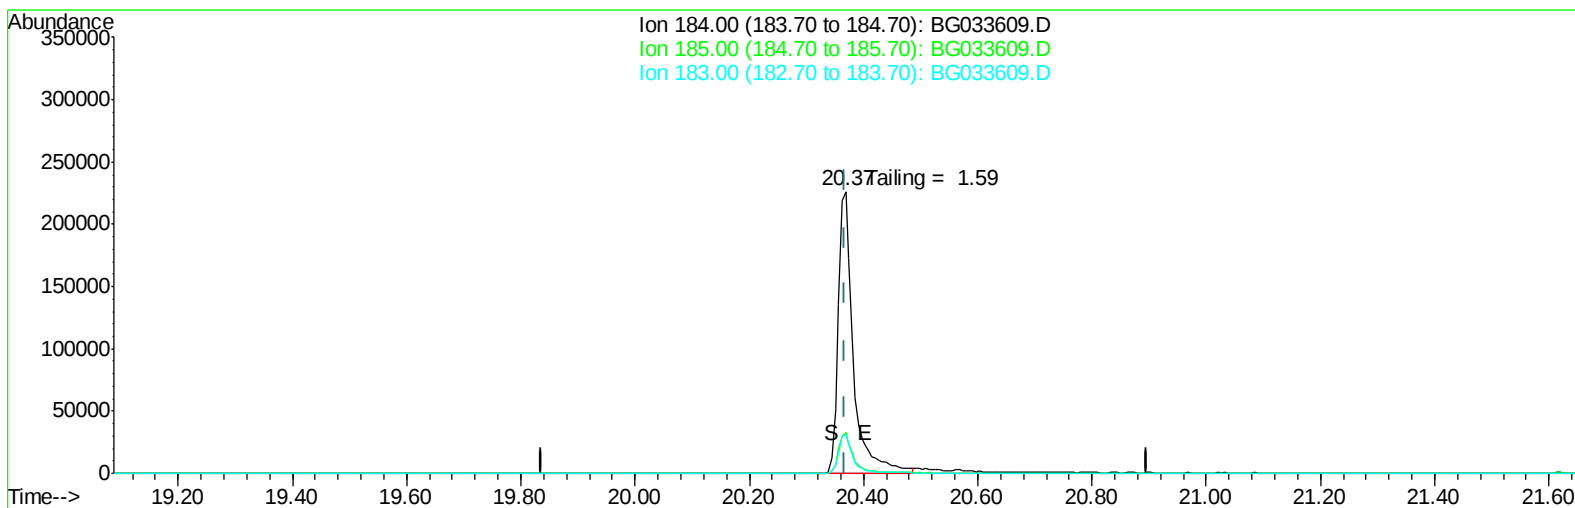

TIC: BG033609.D

(76) Benzidine

20.368min (+0.000) 0.00ng

response 418463

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.59
183.00	13.30	13.67
0.00	0.00	0.00