

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040518\
 Data File : BG033596.D
 Acq On : 5 Apr 2018 17:18
 Operator : SJ/JU
 Sample : J2185-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LOWER-CONCRETE-SLAB-1RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.476	27	32	42	rBV2	78311	152607	5.29%	1.109%
2	3.564	43	47	56	rVB2	40428	64727	2.24%	0.470%
3	5.109	305	310	323	rBV	56700	121629	4.21%	0.884%
4	5.773	416	423	431	rBV	290938	492096	17.05%	3.576%
5	6.296	506	512	521	rBV	80045	185119	6.41%	1.345%
6	7.976	791	798	825	rBV	343474	871707	30.20%	6.334%
7	8.376	859	866	882	rBV	172047	426750	14.79%	3.101%
8	8.864	942	949	964	rBV2	87434	233871	8.10%	1.699%
9	9.193	996	1005	1019	rBV	338532	705472	24.44%	5.126%
10	10.062	1145	1153	1172	rBV2	245416	624504	21.64%	4.538%
11	10.979	1300	1309	1319	rBV4	15573	29049	1.01%	0.211%
12	11.743	1430	1439	1458	rBV2	143028	347956	12.06%	2.528%
13	14.105	1834	1841	1858	rBV	992761	1733509	60.06%	12.596%
14	14.898	1969	1976	1985	rBV	87811	143458	4.97%	1.042%
15	15.303	2040	2045	2051	rBV4	20200	30008	1.04%	0.218%
16	15.479	2067	2075	2088	rBV2	345496	623933	21.62%	4.534%
17	16.243	2200	2205	2209	rVB	32236	39913	1.38%	0.290%
18	16.954	2319	2326	2335	rBV3	81808	159049	5.51%	1.156%
19	17.095	2345	2350	2358	rBV3	29789	54304	1.88%	0.395%
20	18.206	2533	2539	2554	rBV2	462221	818779	28.37%	5.950%
21	19.005	2670	2675	2681	rBV5	20294	36089	1.25%	0.262%
22	20.380	2903	2909	2915	rBV2	49547	65702	2.28%	0.477%
23	20.726	2962	2968	2981	rBV	2121971	2886232	100.00%	20.972%
24	21.431	3081	3088	3092	rVB5	33695	63297	2.19%	0.460%
25	22.066	3191	3196	3208	rBV4	114729	240172	8.32%	1.745%
26	22.354	3239	3245	3249	rVB	34238	54010	1.87%	0.392%
27	22.553	3271	3279	3296	rBV	434944	904928	31.35%	6.576%
28	23.828	3488	3496	3507	rBV	378084	745563	25.83%	5.418%
29	24.416	3590	3596	3603	rVB2	46493	93819	3.25%	0.682%
30	26.314	3909	3919	3941	rVB2	230341	813799	28.20%	5.913%


Sum of corrected areas: 13762051

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040518\
Data File : BG033596.D
Acq On : 5 Apr 2018 17:18
Operator : SJ/JU
Sample : J2185-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LOWER-CONCRETE-SLAB-1RE

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

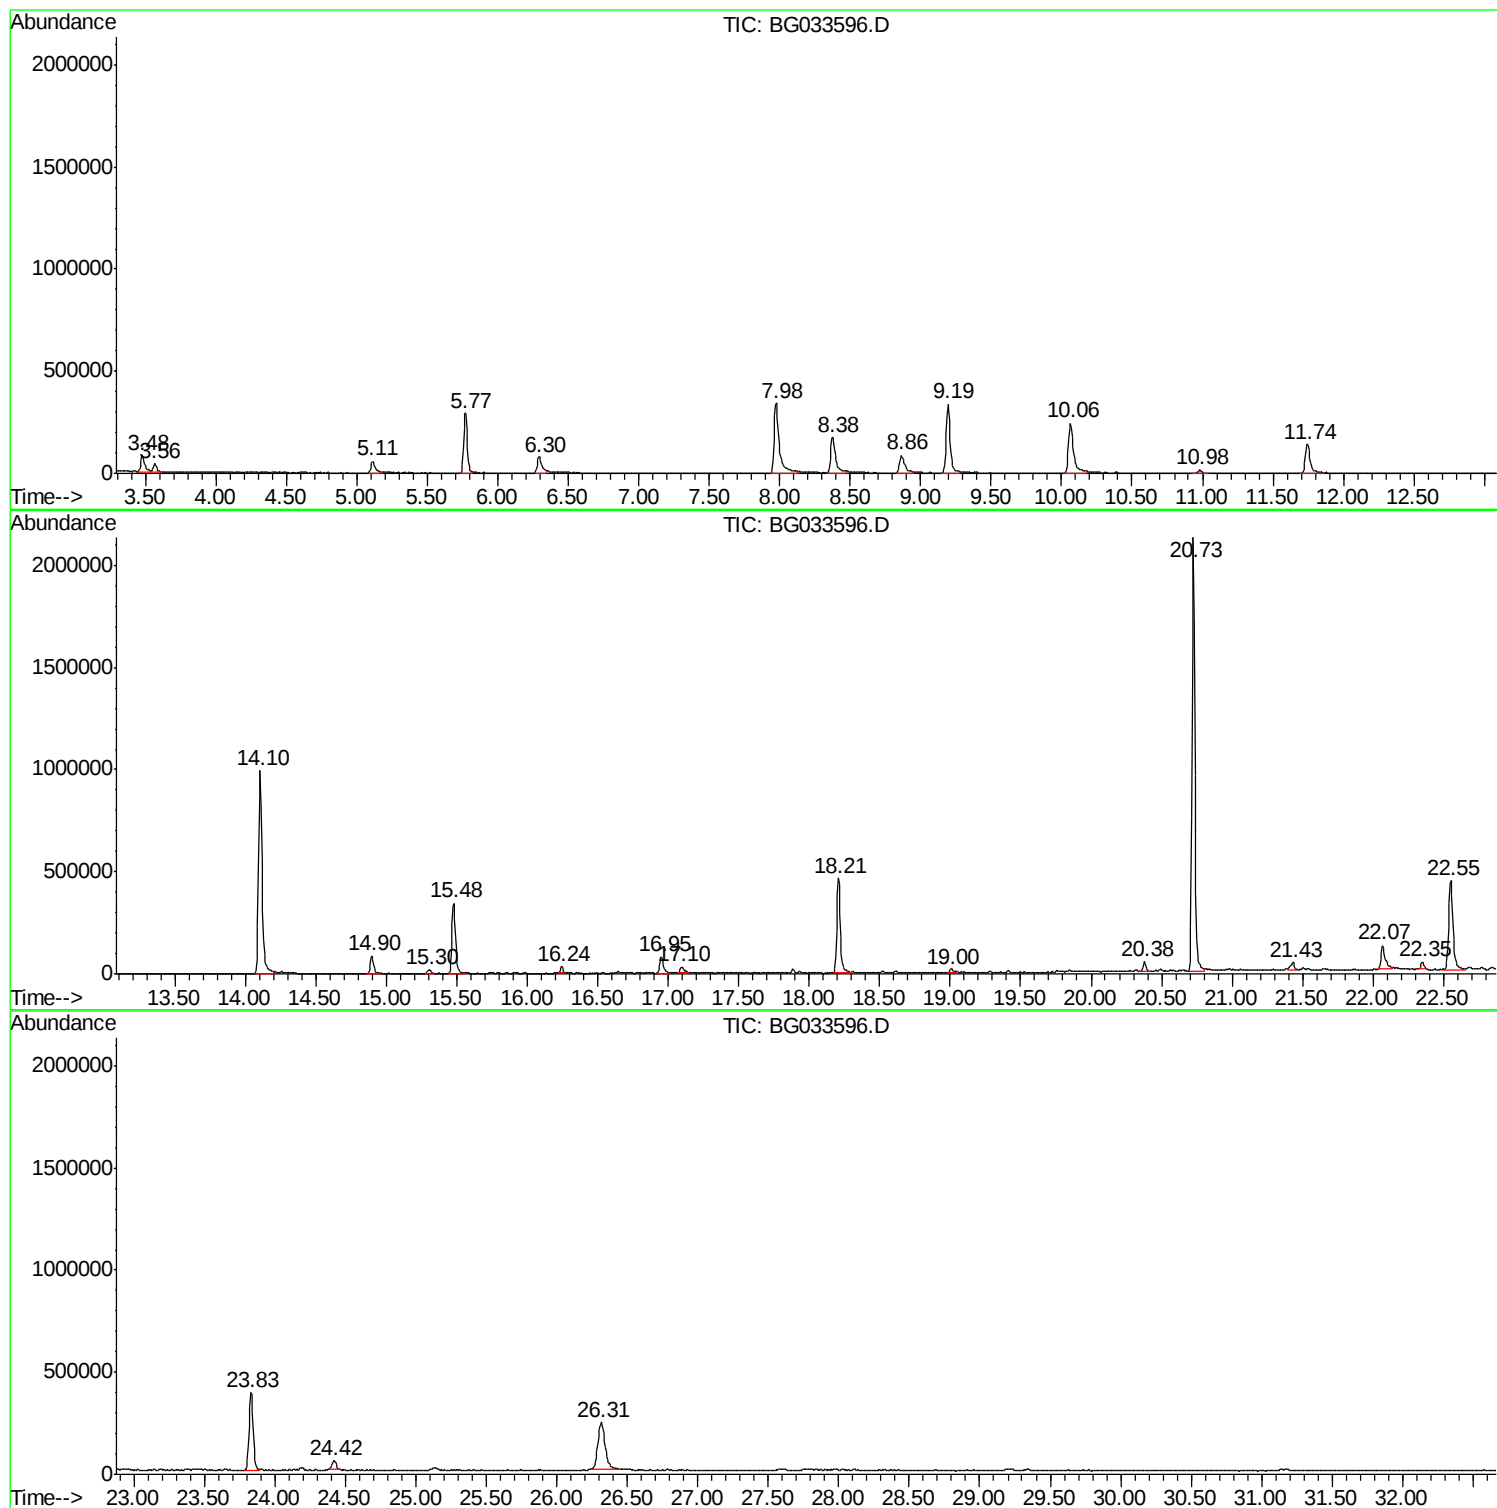

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG040518\
Data_File : BG033596.D
Acq_On : 5 Apr 2018 17:188
Operator : SJ/JUU
Sample : J2185-01REE
Misc :
ALS_Vial : 7 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
LOWER-CONCRETE-SLAB-1RE

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
