


Data Path : Z:\HPCHEM1\BNA G\Data\BG040518\
 Data File : BG033590.D
 Acq On : 5 Apr 2018 13:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 05 17:36:07 2018

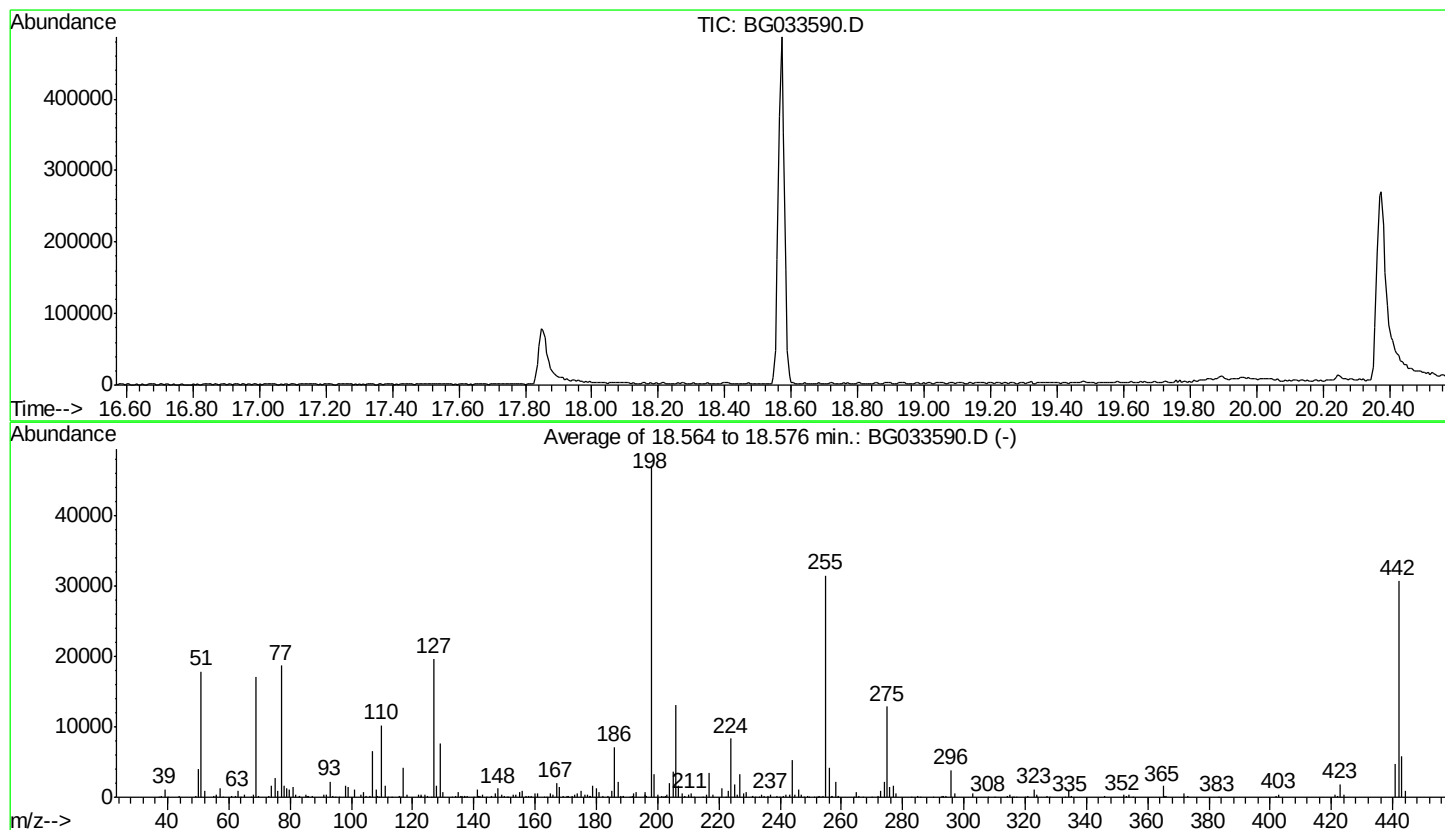

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	17886	PASS
68	69	0.00	2	1.9	323	PASS
69	198	0.00	100	36.1	17035	PASS
70	69	0.00	2	1.0	176	PASS
127	198	10	80	41.8	19711	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47136	PASS
199	198	5	9	7.1	3350	PASS
275	198	10	60	27.3	12888	PASS
365	198	1	100	3.4	1617	PASS
441	443	0.01	100	79.5	4657	PASS
442	198	50	100	65.3	30794	PASS
443	442	15	24	19.0	5858	PASS