

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
 Data File : BG040389.D
 Acq On : 5 Apr 2019 23:05
 Operator : JU/SJ
 Sample : K2242-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 06 00:37:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	75774	20.00	ng	-0.03
21) Naphthalene-d8	10.86	136	294214	20.00	ng	-0.03
39) Acenaphthene-d10	14.68	164	179548	20.00	ng	-0.03
64) Phenanthrene-d10	17.42	188	426085	20.00	ng	-0.03
76) Chrysene-d12	21.69	240	456398	20.00	ng	-0.04
87) Perylene-d12	24.97	264	453161	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	287112	62.99	ng	-0.01
7) Phenol-d6	7.20	99	257349	40.85	ng	-0.03
23) Nitrobenzene-d5	9.22	82	448111	80.96	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	269593	138.93	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	969487	80.01	ng	-0.03
79) Terphenyl-d14	20.02	244	1669357	82.29	ng	-0.03
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.22	70	56610	12.534	ng	# 73
51) 2,6-Dinitrotoluene	14.68	165	23050	7.305	ng	# 25
57) 2,4-Dinitrotoluene	14.68	165	23050	5.258	ng	# 25
67) 4-Bromophenyl-phenylether	16.16	248	20784	4.335	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
Data File : BG040389.D
Acq On : 5 Apr 2019 23:05
Operator : JU/SJ
Sample : K2242-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 06 00:37:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

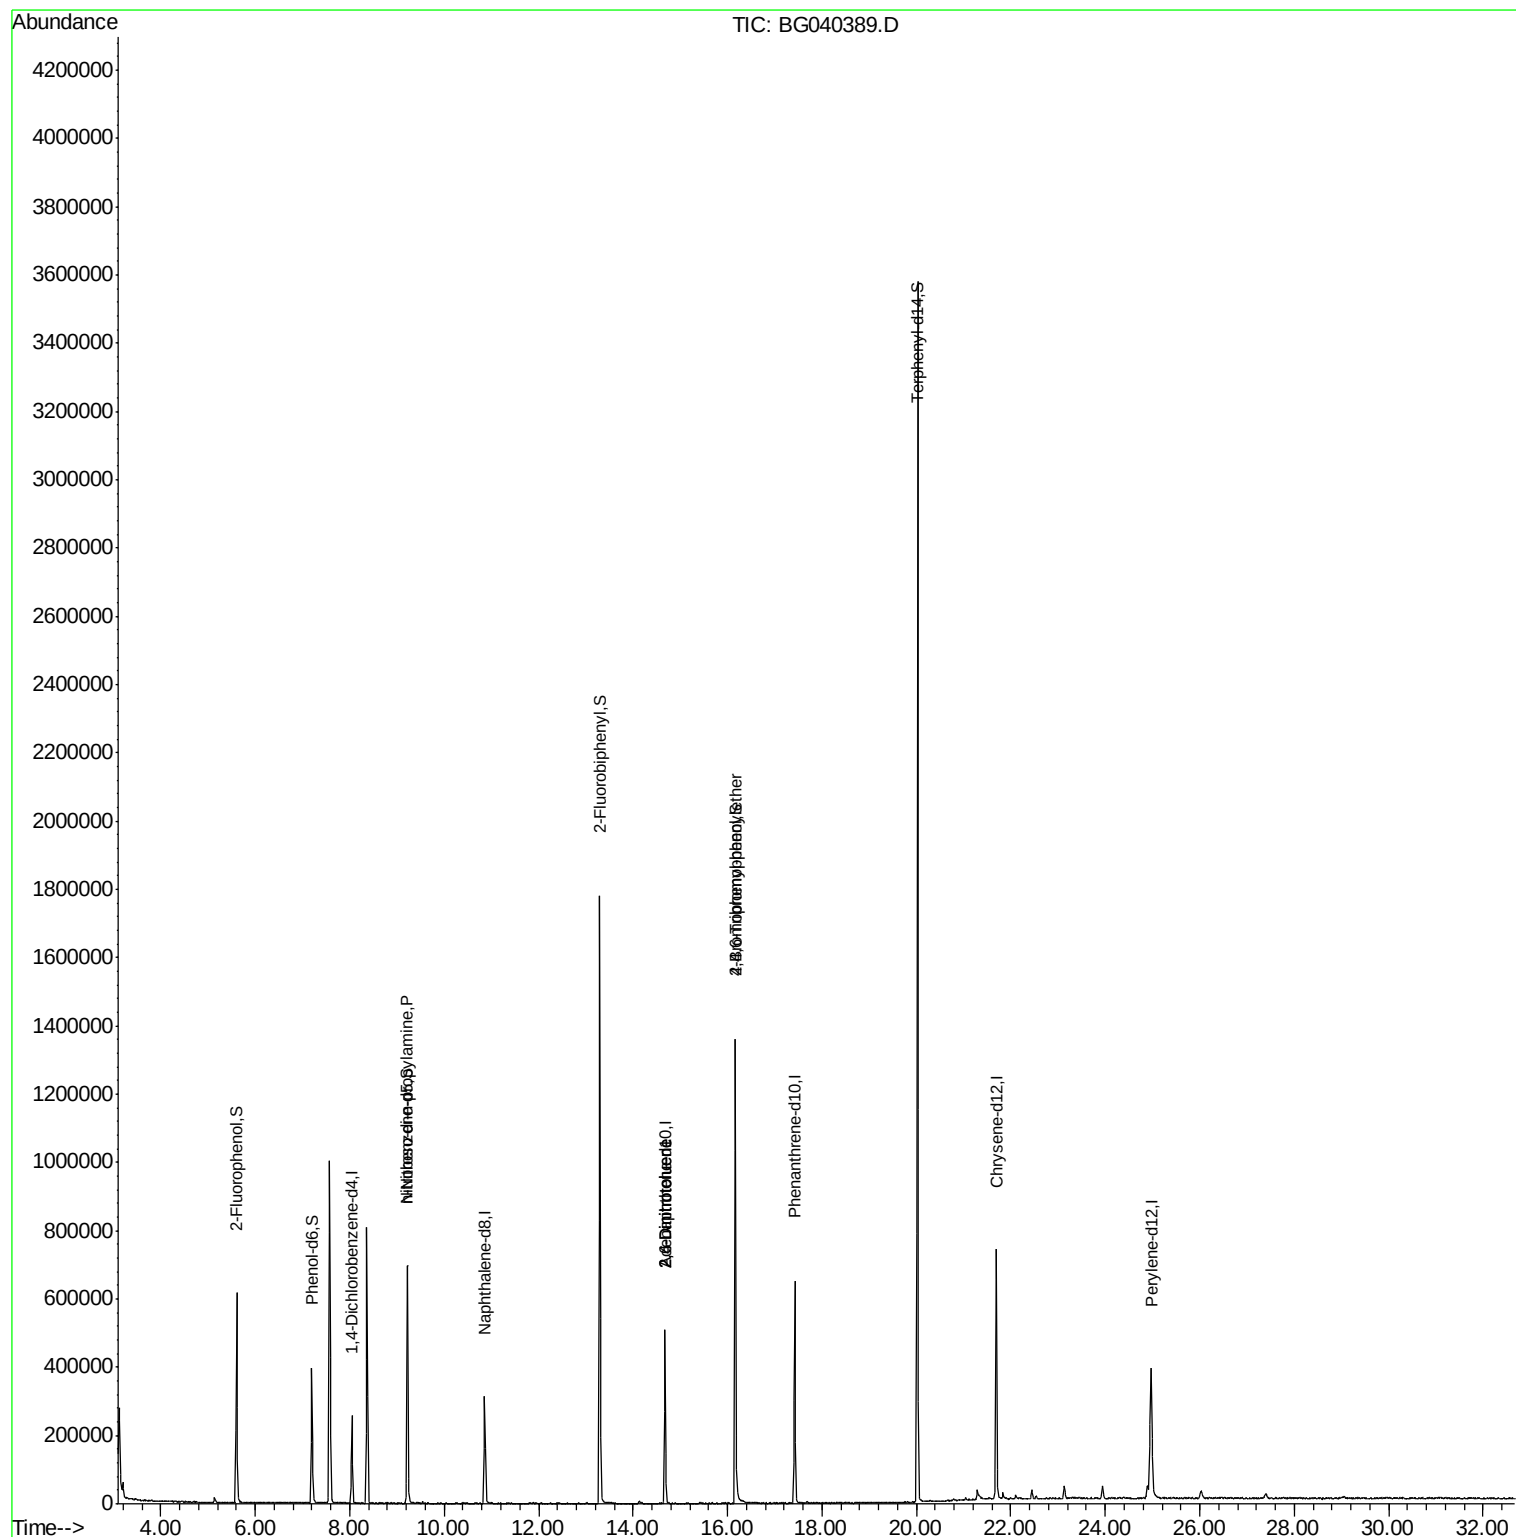

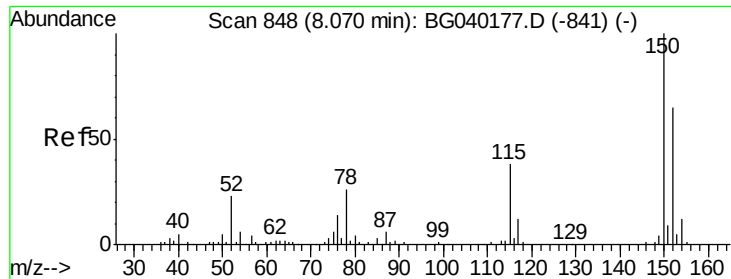


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.03 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 75774
Ion Ratio Lower Upper
152 100
150 149.2 123.7 185.5
115 56.2 46.9 70.3

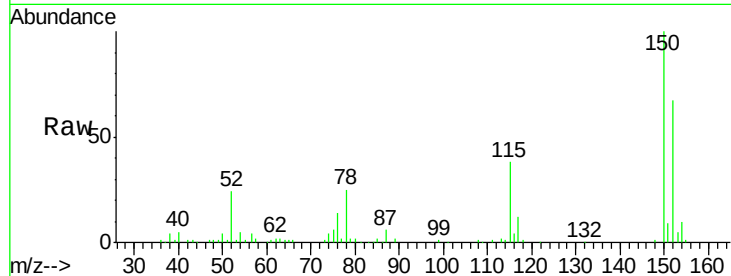


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

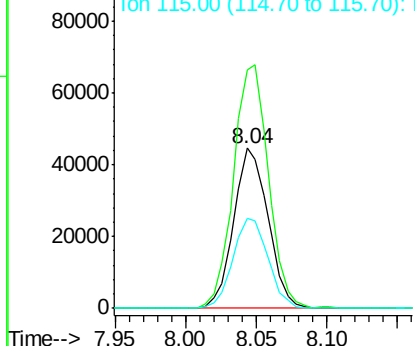



#5


2-Fluorophenol
Concen: 62.990 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.01 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Tgt Ion:112 Resp: 287112
Ion Ratio Lower Upper
112 100
64 67.5 54.2 81.2
63 31.2 26.4 39.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

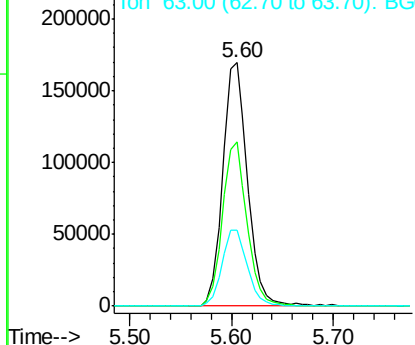

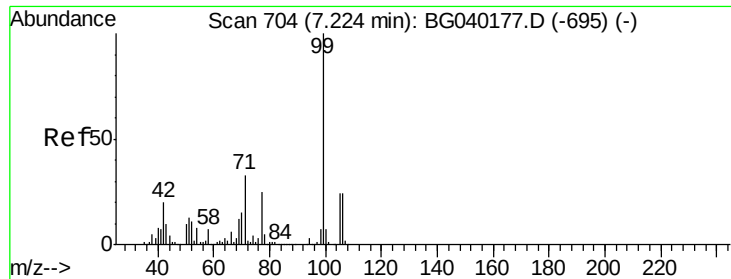

#7

Phenol-d6

Concen: 40.853 ng

RT: 7.20 min Scan# 699

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 257349

Ion Ratio Lower Upper




99 100

42 18.5 16.2 24.2

71 30.4 26.8 40.2

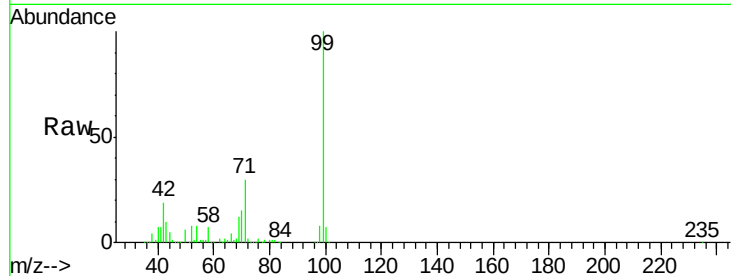

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

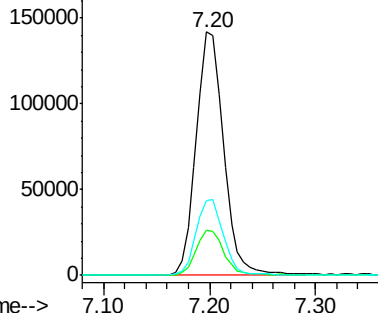

#19

n-Nitroso-di-n-propylamine

Concen: 12.534 ng

RT: 9.22 min Scan# 1043

Delta R.T. 0.34 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Tgt Ion: 70 Resp: 56610


Ion Ratio Lower Upper

70 100



42 49.8 54.0 81.0#


101 0.0 8.6 13.0#

130 2.1 18.2 27.2#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

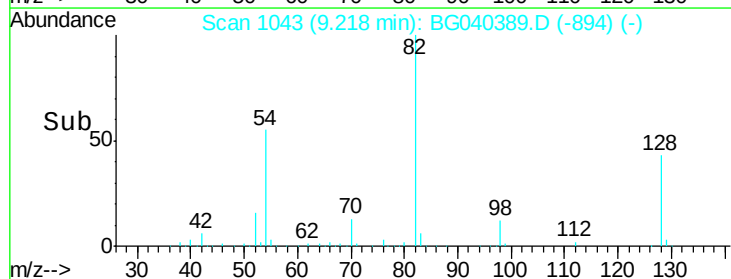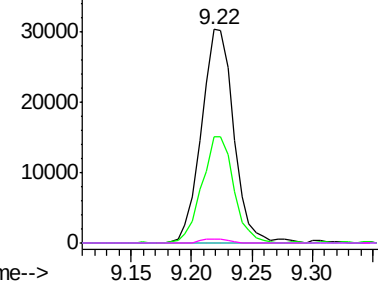


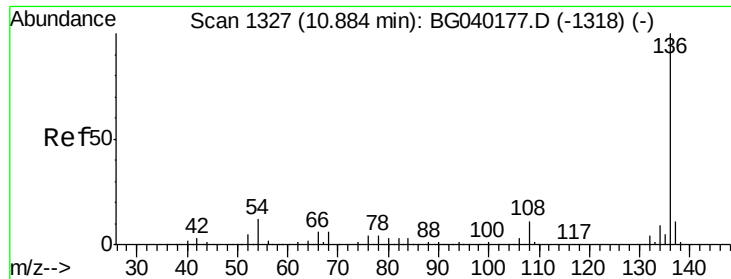




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1322
Delta R.T. -0.03 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	294214
Ion	Ratio	Lower Upper
136	100	
137	11.6	8.9 13.3
54	10.3	9.6 14.4
68	7.1	5.1 7.7

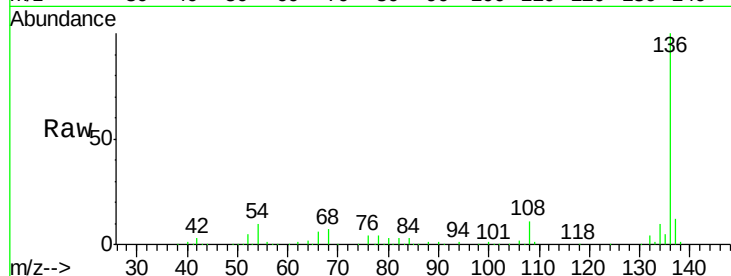


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

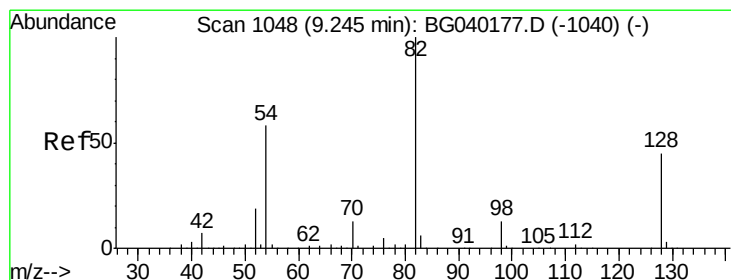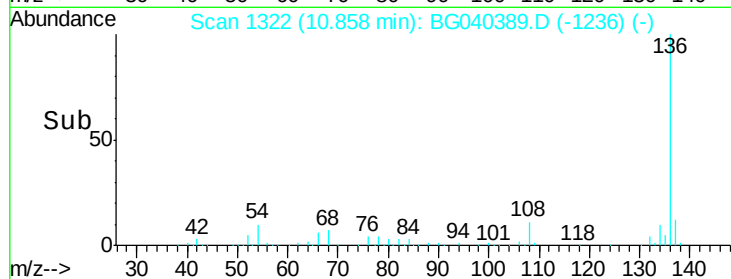
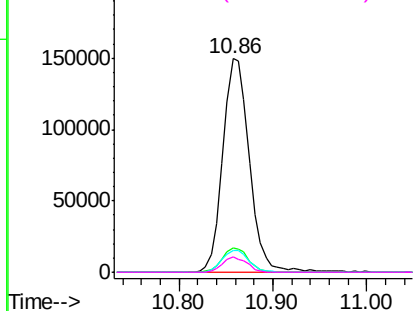



#23
Nitrobenzene-d5
Concen: 80.957 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Tgt Ion: 82	Resp:	448111
Ion	Ratio	Lower Upper
82	100	
128	44.6	35.8 53.8
54	54.9	46.2 69.2



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

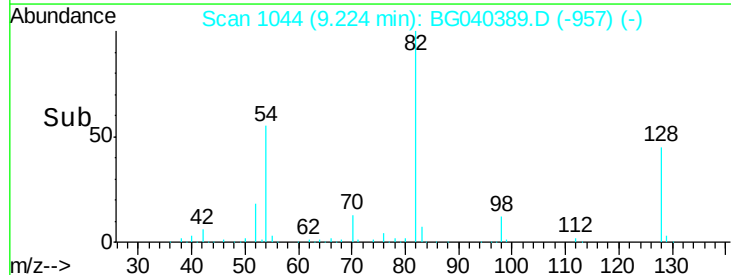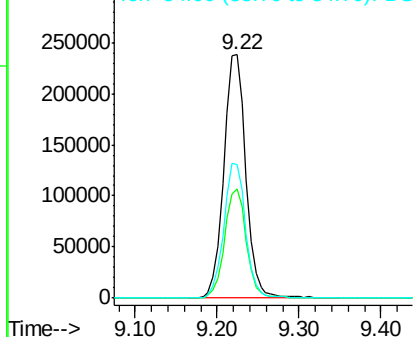



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1972

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 179548

Ion Ratio Lower Upper

164 100

162 100.7 77.4 116.2




160 43.1 35.3 52.9

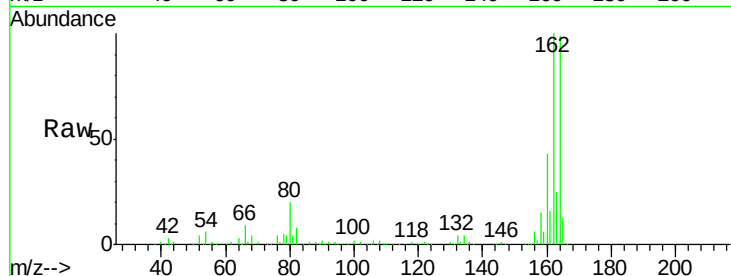

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

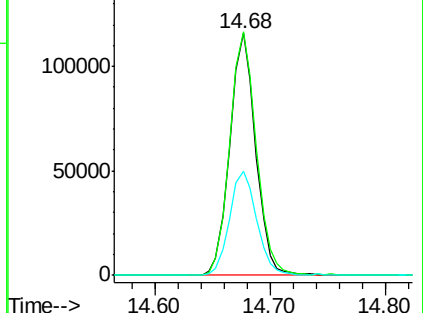

#42

2,4,6-Tribromophenol

Concen: 138.934 ng

RT: 16.17 min Scan# 2226

Delta R.T. -0.02 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05


Tgt Ion:330 Resp: 269593

Ion Ratio Lower Upper

330 100

332 96.9 76.6 115.0



141 38.0 32.6 48.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



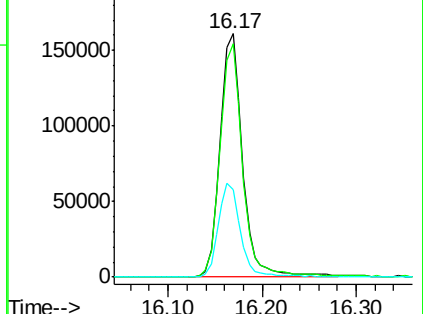





#45
2-Fluorobiphenyl
Concen: 80.009 ng
RT: 13.30 min Scan# 1737
Delta R.T. -0.03 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.7	30.5	45.7
170	25.2	20.1	30.1

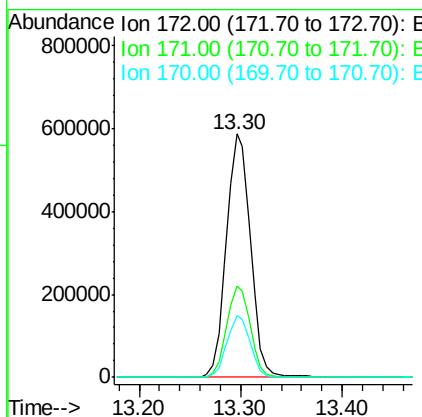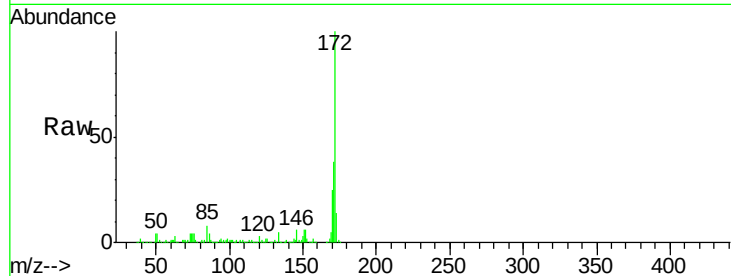

#51
2,6-Dinitrotoluene
Concen: 7.305 ng
RT: 14.68 min Scan# 1972
Delta R.T. 0.39 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.1	66.1#
89	2.0	44.9	67.3#



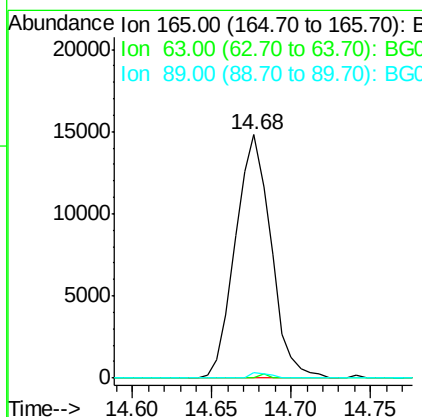
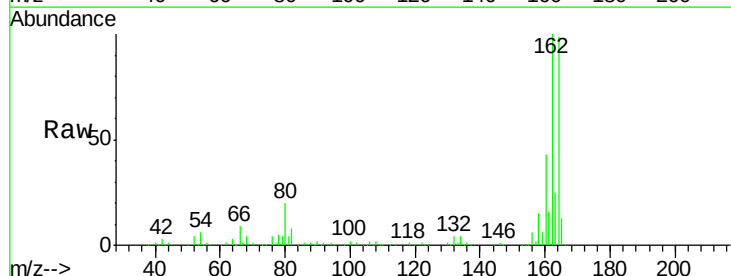




#57
 2,4-Dinitrotoluene
 Concen: 5.258 ng
 RT: 14.68 min Scan# 1972
 Delta R.T. -0.39 min
 Lab File: BG040389.D
 Acq: 5 Apr 2019 23:05




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:165	Resp:	23050
Ion Ratio	Lower	Upper
165	100	
63	0.0	33.8 50.6#
89	2.0	55.4 83.2#
182	0.0	2.2 3.4#

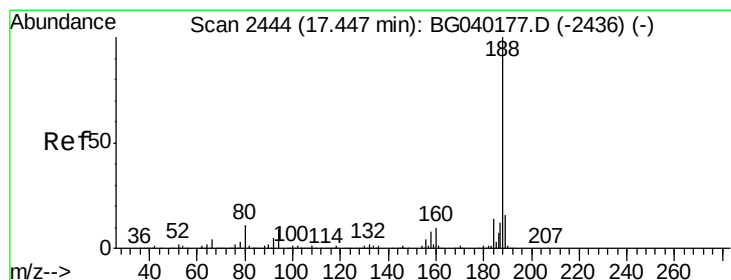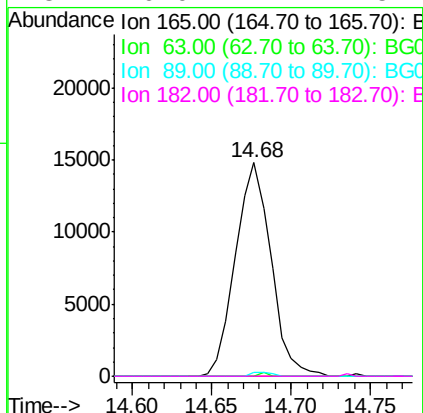

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.42 min Scan# 2439
 Delta R.T. -0.03 min
 Lab File: BG040389.D
 Acq: 5 Apr 2019 23:05

Tgt Ion:188	Resp:	426085
Ion Ratio	Lower	Upper
188	100	
94	8.6	7.0 10.4
80	10.9	8.6 13.0

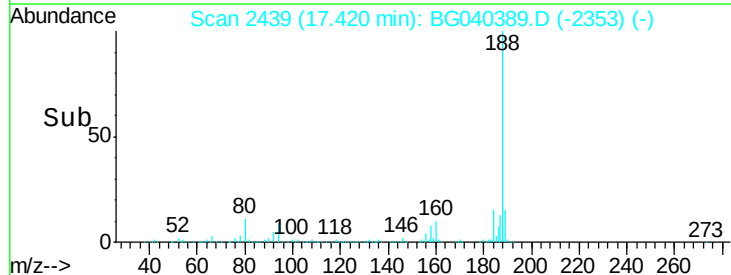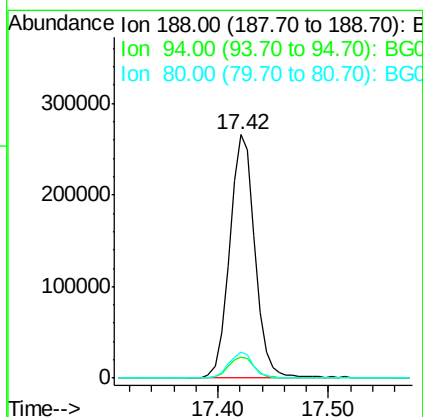


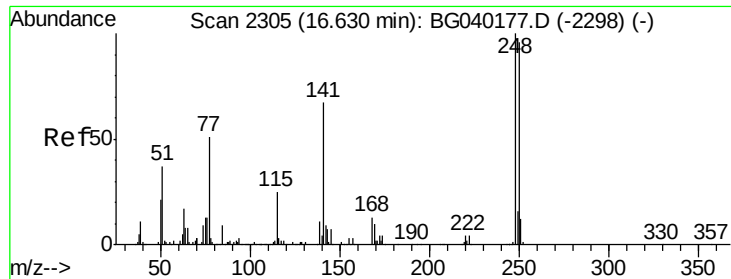




#67
 4-Bromophenyl-phenylether
 Concen: 4.335 ng
 RT: 16.16 min Scan# 2225
 Delta R.T. -0.47 min
 Lab File: BG040389.D
 Acq: 5 Apr 2019 23:05

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:248 Resp: 20784
 Ion Ratio Lower Upper
 248 100
 250 174.8 76.4 114.6#
 141 447.7 53.8 80.8#




Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

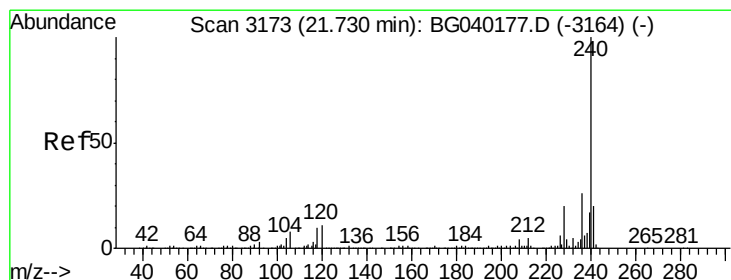
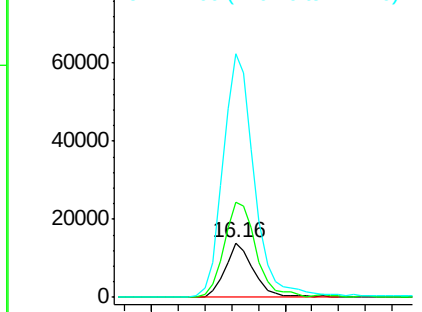



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.69 min Scan# 3166
 Delta R.T. -0.04 min
 Lab File: BG040389.D
 Acq: 5 Apr 2019 23:05

Tgt Ion:240 Resp: 456398
 Ion Ratio Lower Upper
 240 100
 120 10.6 8.4 12.6
 236 25.6 20.8 31.2

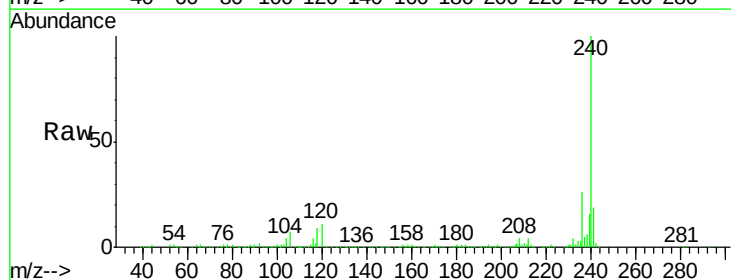

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

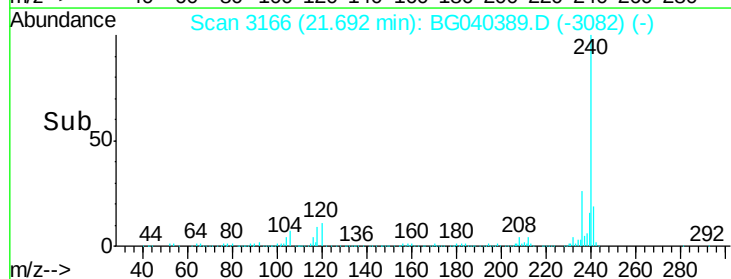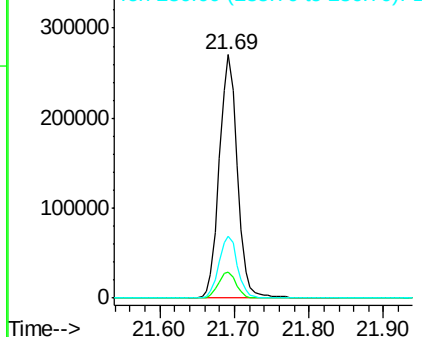



#79

Terphenyl-d14

Concen: 82.285 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 1669357

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.6




122 11.9 8.5 12.7



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

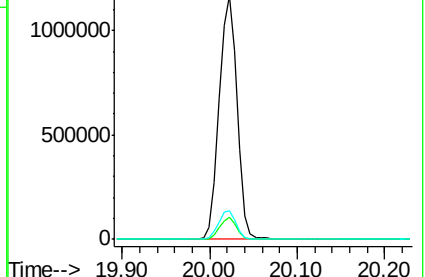

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.97 min Scan# 3724

Delta R.T. -0.06 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05


Tgt Ion:264 Resp: 453161

Ion Ratio Lower Upper

264 100

260 23.7 17.9 26.9

265 21.3 16.8 25.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

