
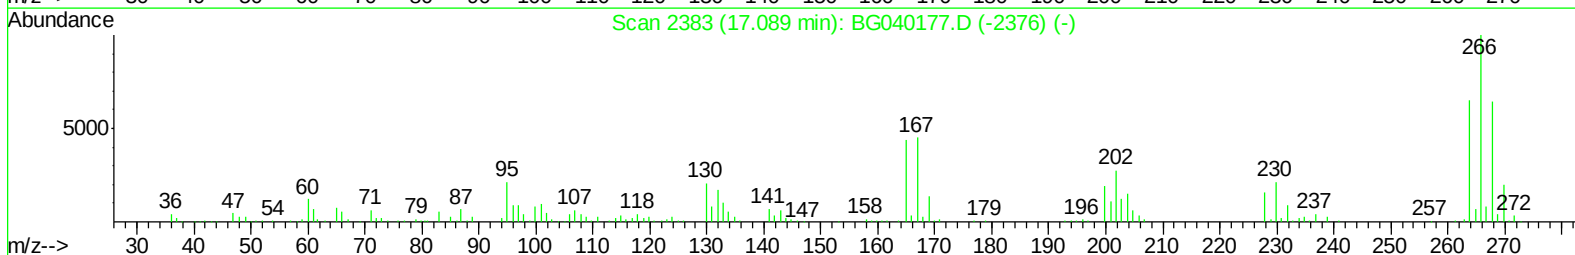
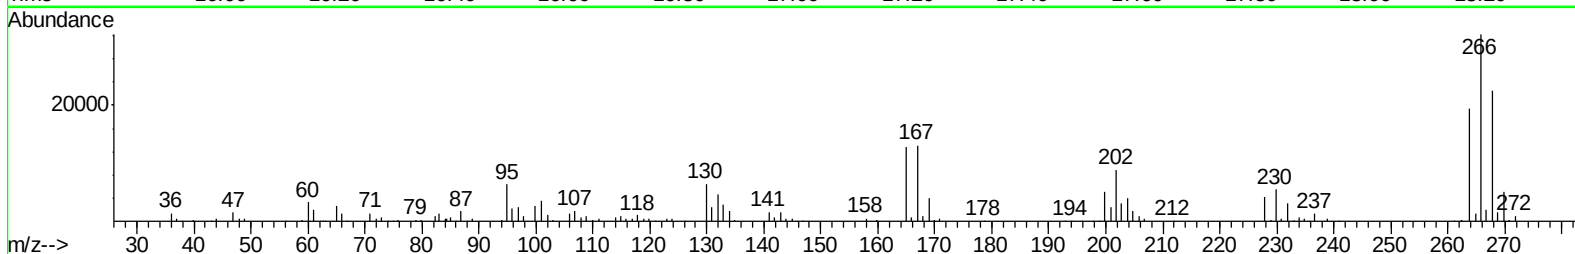


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG040519\
Data File : BG040377.D
Acq On : 5 Apr 2019 14:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 04:21:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

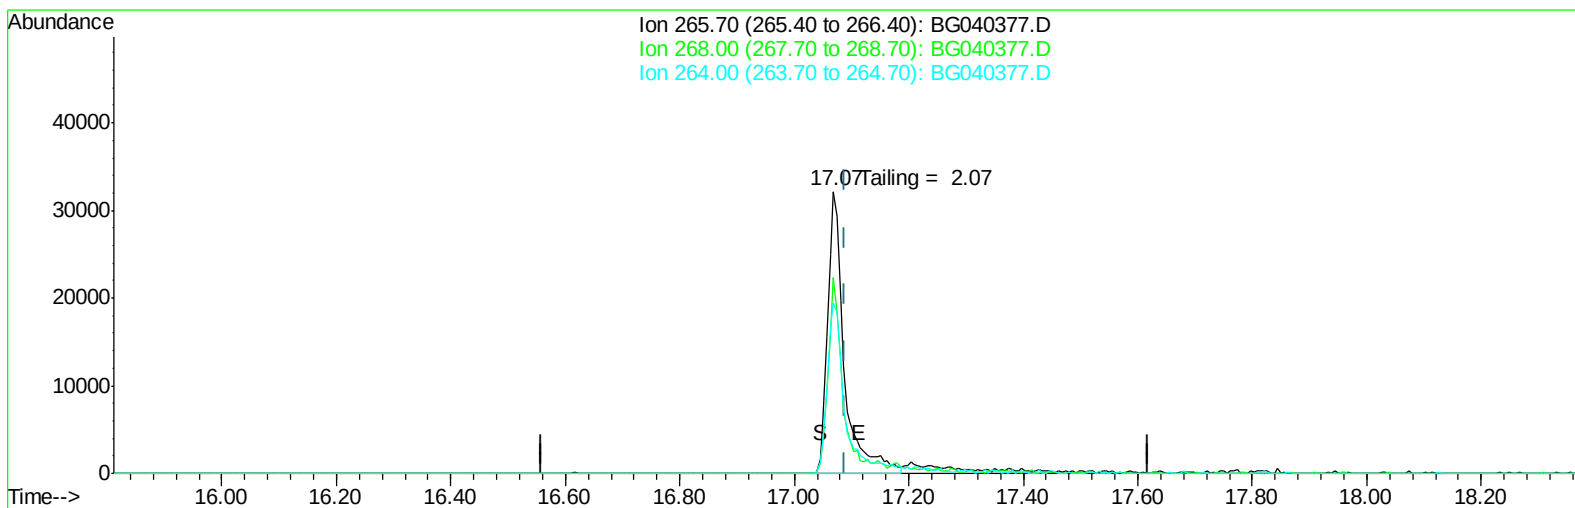

TIC: BG040377.D

(70) Pentachlorophenol (C)




17.069min (-0.020) 22473.70ng

response 65127

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	69.72
264.00	64.80	60.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG040519\
 Data File : BG040377.D
 Acq On : 5 Apr 2019 14:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 04:21:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

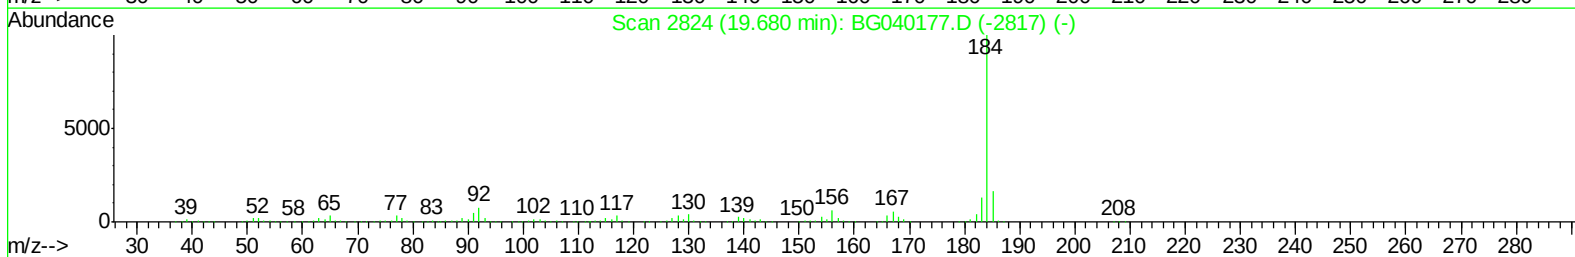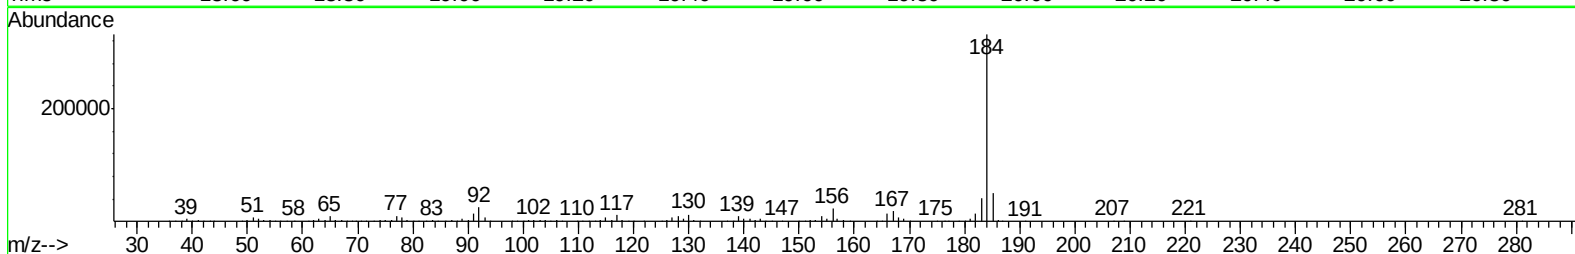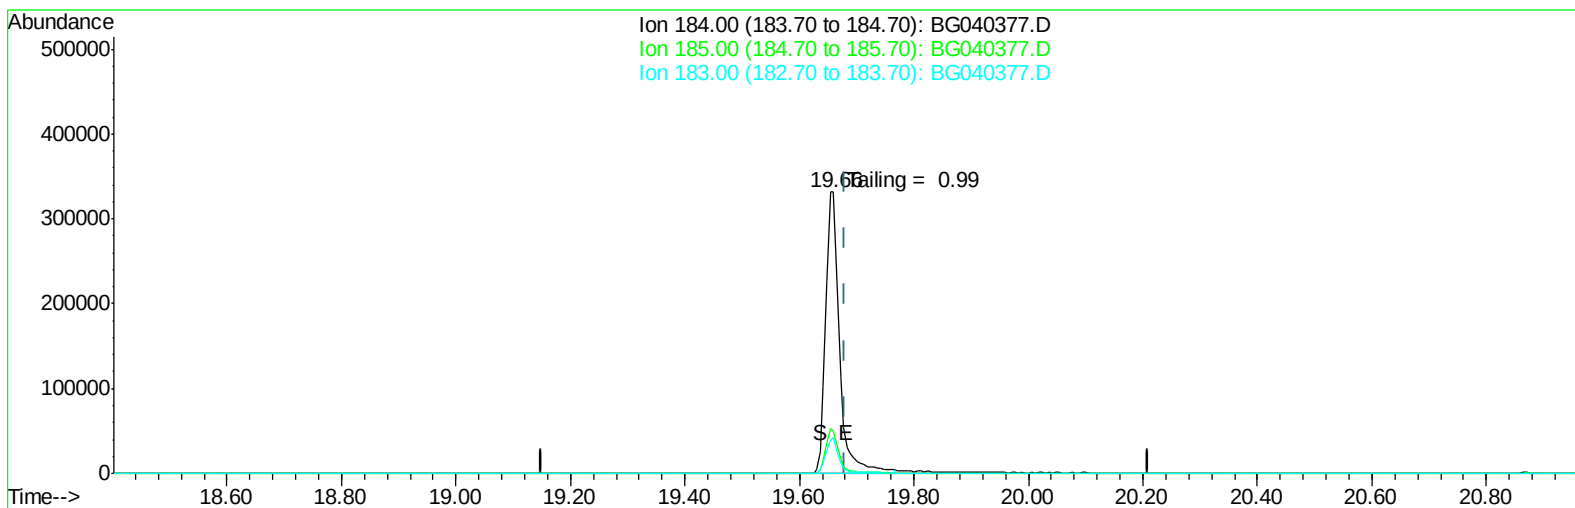

TIC: BG040377.D

(77) Benzidine

19.660min (-0.020) 28179.21ng

response 562723

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.23
183.00	12.90	12.53
0.00	0.00	0.00