

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
 Data File : BG040389.D
 Acq On : 5 Apr 2019 23:05
 Operator : JU/SJ
 Sample : K2242-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TWP-02

Quant Time: Apr 06 00:47:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	75774	20.00	ng	-0.03
21) Naphthalene-d8	10.86	136	294214	20.00	ng	-0.03
39) Acenaphthene-d10	14.68	164	179548	20.00	ng	-0.03
64) Phenanthrene-d10	17.42	188	426085	20.00	ng	-0.03
76) Chrysene-d12	21.69	240	456398	20.00	ng	-0.04
87) Perylene-d12	24.97	264	453161	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	287112	62.99	ng	-0.01
7) Phenol-d6	7.20	99	257349	40.85	ng	-0.03
23) Nitrobenzene-d5	9.22	82	448111	80.96	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	269593	138.93	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	969487	80.01	ng	-0.03
79) Terphenyl-d14	20.02	244	1669357	82.29	ng	-0.03


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
Data File : BG040389.D
Acq On : 5 Apr 2019 23:05
Operator : JU/SJ
Sample : K2242-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TWP-02

Quant Time: Apr 06 00:47:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

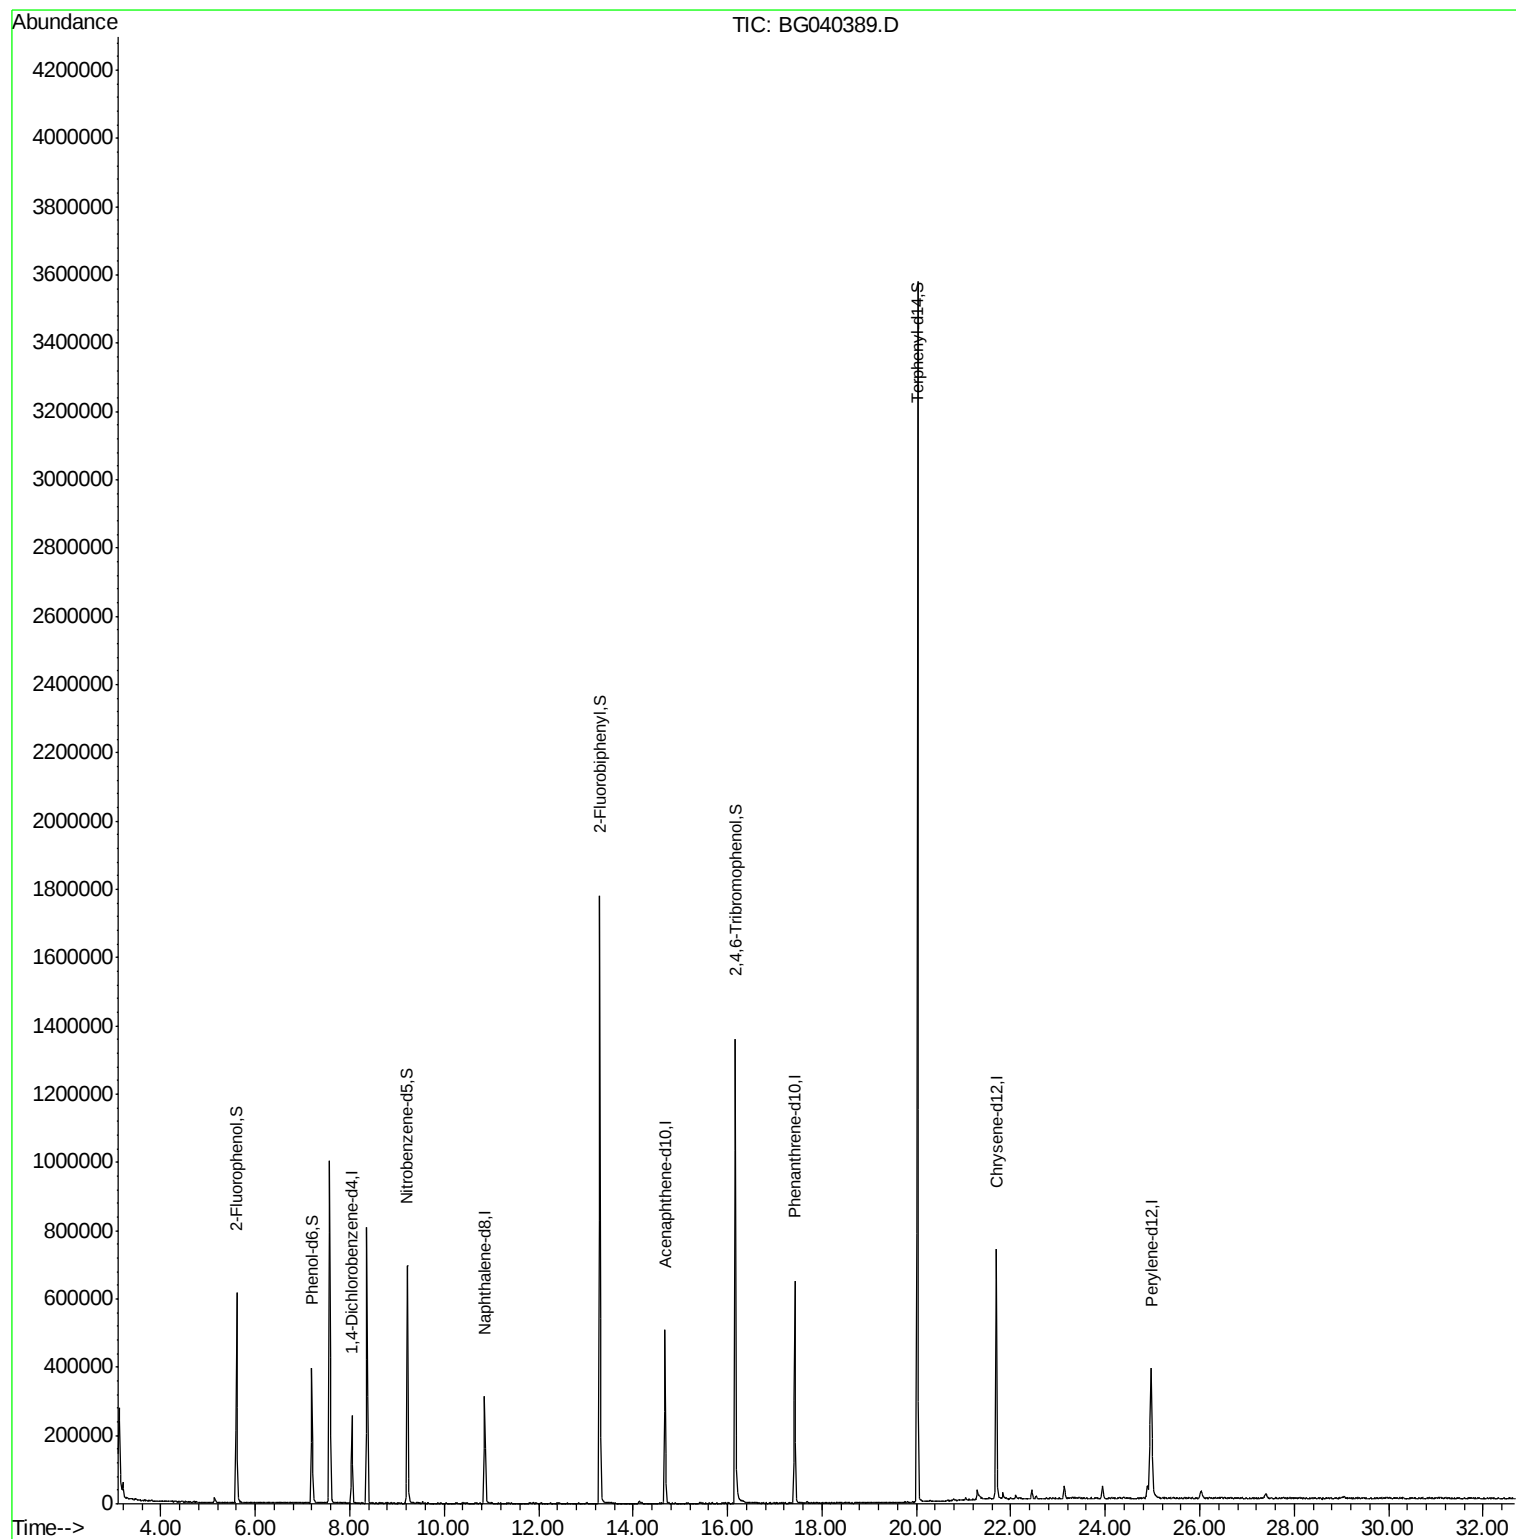




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.03 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Instrument :
BNA_G
ClientSampleId :
TWP-02

Tot Ion:152 Resp: 75774
Ion Ratio Lower Upper
152 100
150 149.2 123.7 185.5
115 56.2 46.9 70.3

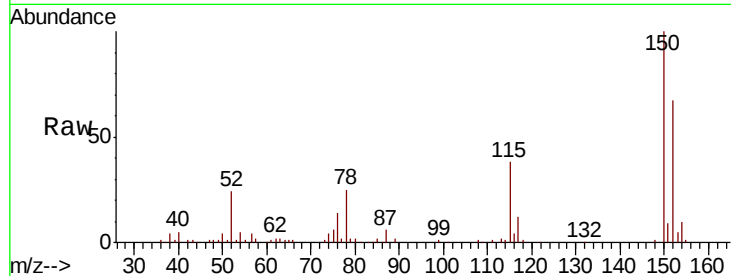


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

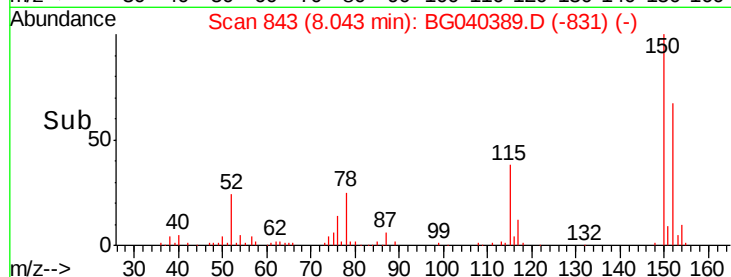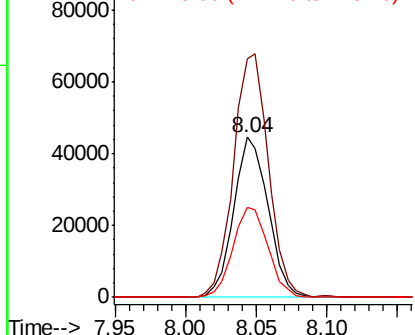



#5


2-Fluorophenol
Concen: 62.990 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.01 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Tgt Ion:112 Resp: 287112
Ion Ratio Lower Upper
112 100
64 67.5 54.2 81.2
63 31.2 26.4 39.6

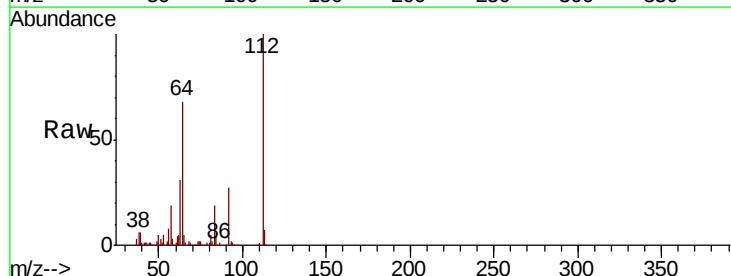

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

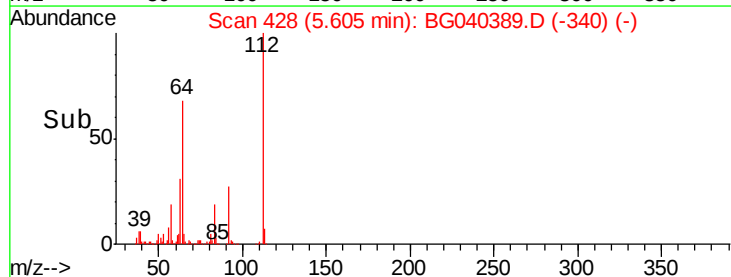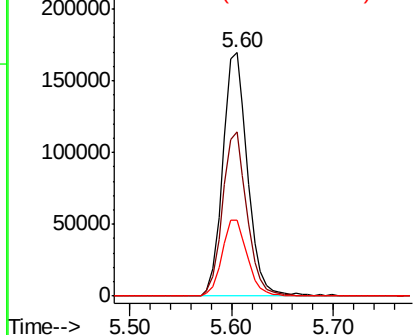

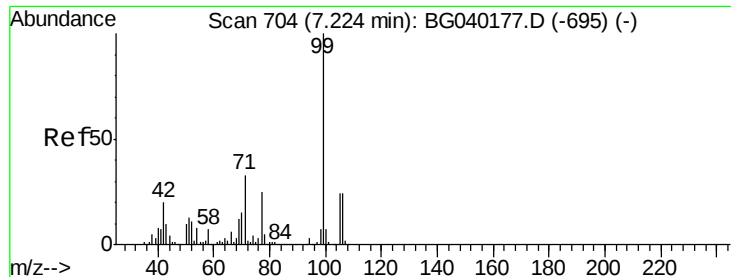

#7

Phenol-d6

Concen: 40.853 ng

RT: 7.20 min Scan# 699

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Instrument :

BNA_G

ClientSampleId :

TWP-02


Tot Ion: 99 Resp: 257349

Ion Ratio Lower Upper




99 100

42 18.5 16.2 24.2

71 30.4 26.8 40.2

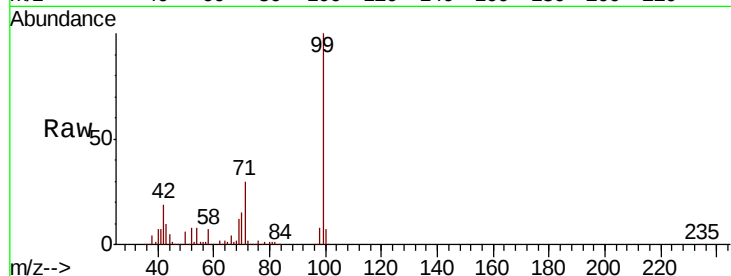

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

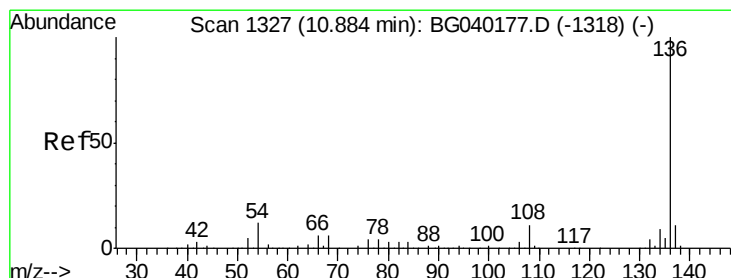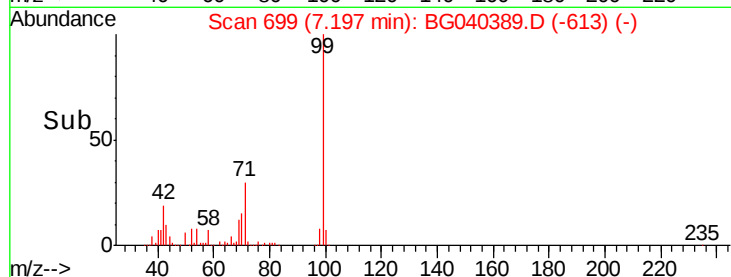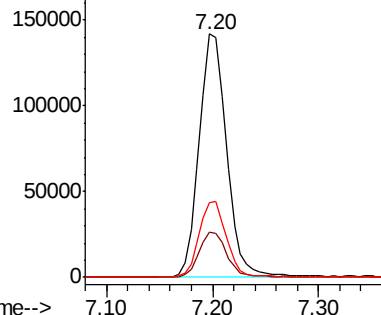

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1322

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Tgt Ion: 136 Resp: 294214


Ion Ratio Lower Upper

136 100



137 11.6 8.9 13.3


54 10.3 9.6 14.4

68 7.1 5.1 7.7

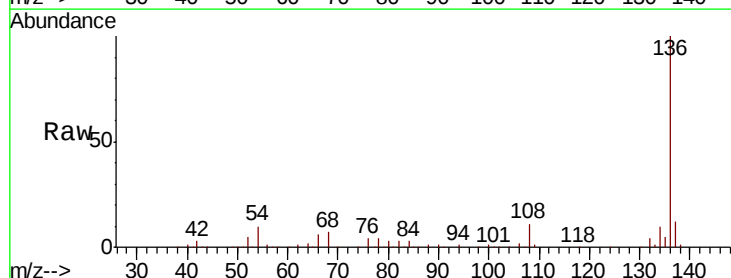

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


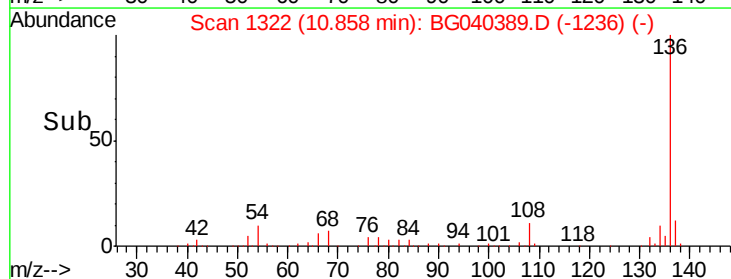
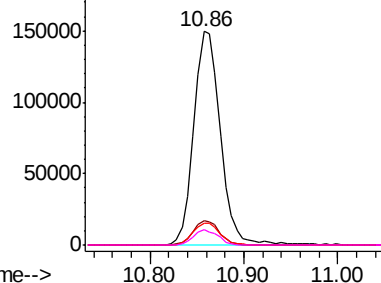


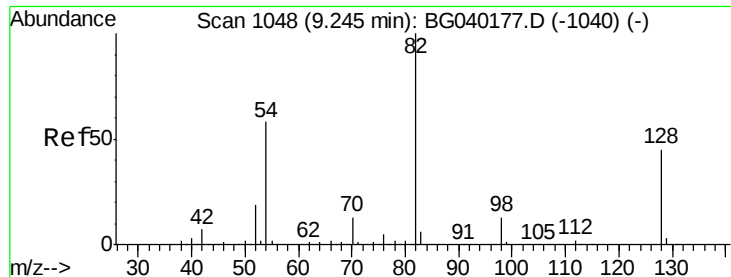

#23
Nitrobenzene-d5
Concen: 80.957 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05




Instrument :
BNA_G
ClientSampleId :
TWP-02

Tot Ion: 82 Resp: 448111
Ion Ratio Lower Upper
82 100
128 44.6 35.8 53.8
54 54.9 46.2 69.2

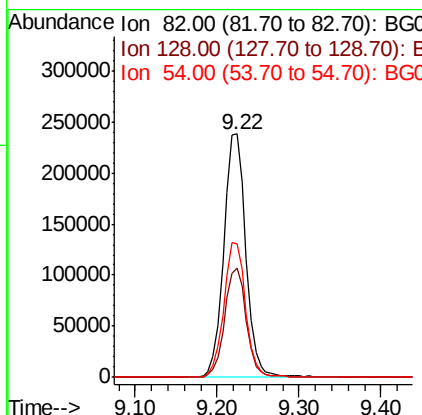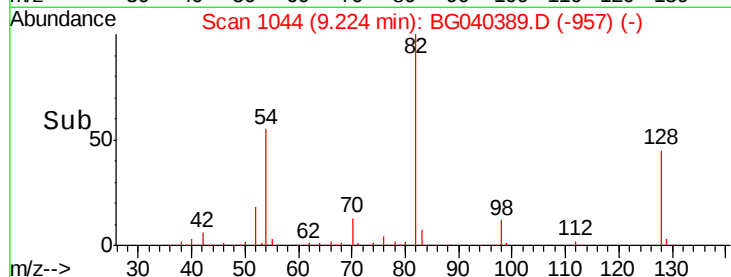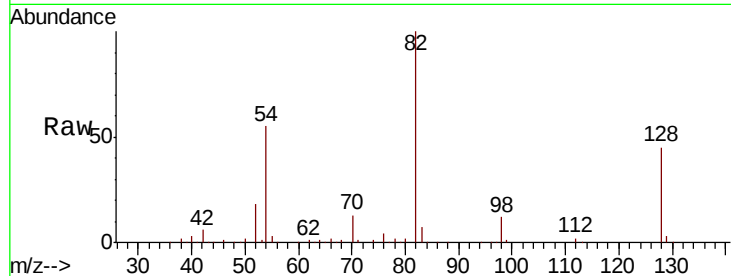

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1972
Delta R.T. -0.03 min
Lab File: BG040389.D
Acq: 5 Apr 2019 23:05

Tgt Ion:164 Resp: 179548
Ion Ratio Lower Upper
164 100
162 100.7 77.4 116.2
160 43.1 35.3 52.9

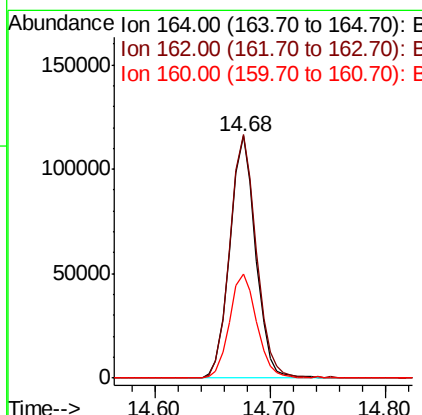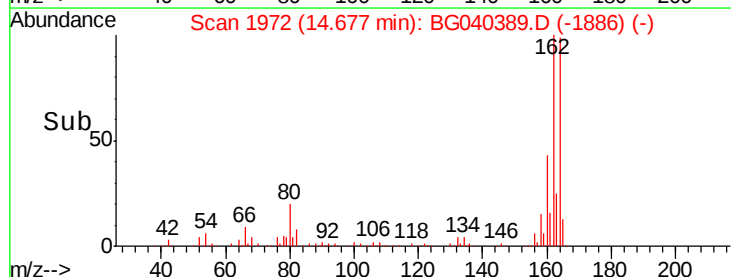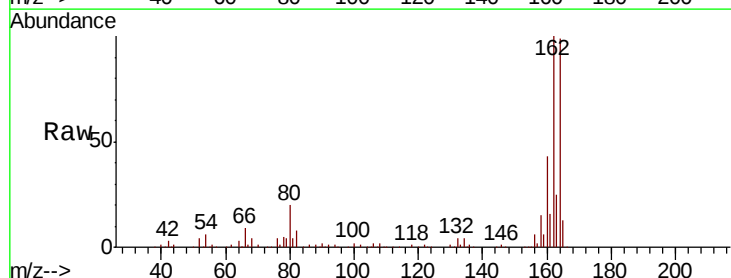




#42
 2,4,6-Tribromophenol
 Concen: 138.934 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. -0.02 min
 Lab File: BG040389.D
 Acq: 5 Apr 2019 23:05

Instrument :
 BNA_G
 ClientSampleId :
 TWP-02

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	76.6	115.0
141	38.0	32.6	48.8


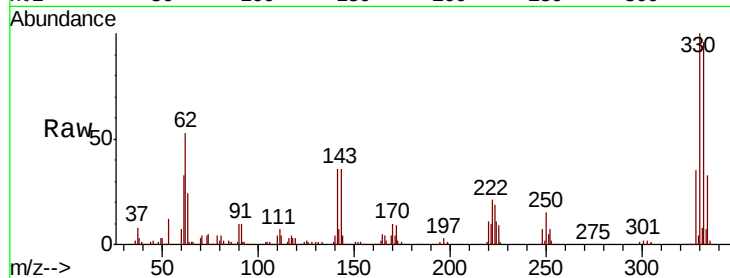


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

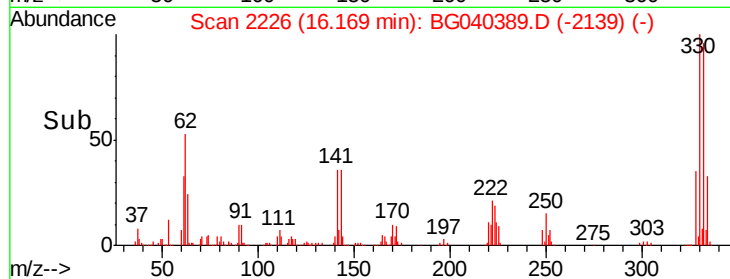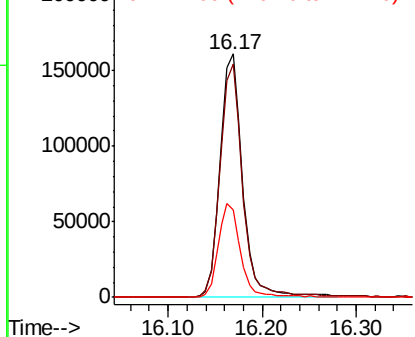

#45
 2-Fluorobiphenyl
 Concen: 80.009 ng
 RT: 13.30 min Scan# 1737
 Delta R.T. -0.03 min
 Lab File: BG040389.D
 Acq: 5 Apr 2019 23:05

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	30.5	45.7
170	25.2	20.1	30.1


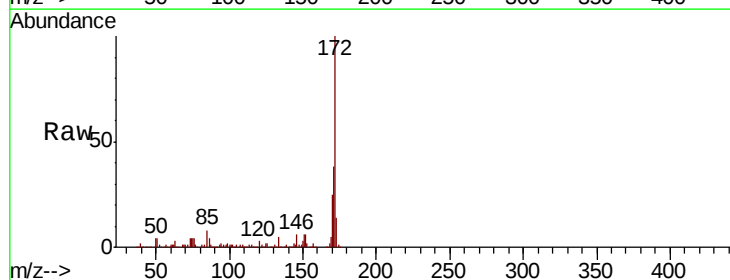



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

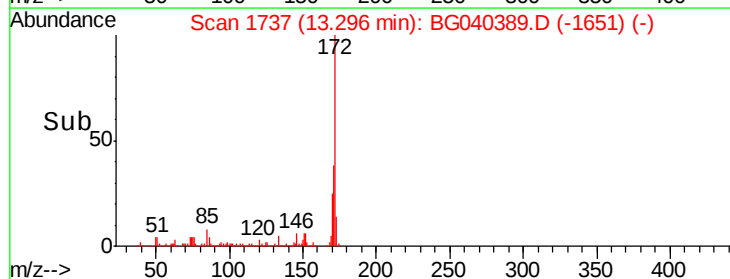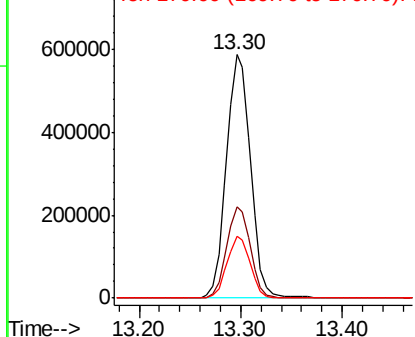

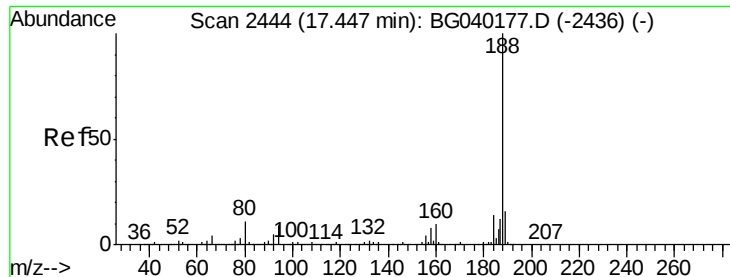

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2439

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Instrument :

BNA_G

ClientSampleId :

TWP-02


Tot Ion:188 Resp: 426085

Ion Ratio Lower Upper

188 100

94 8.6 7.0 10.4




80 10.9 8.6 13.0

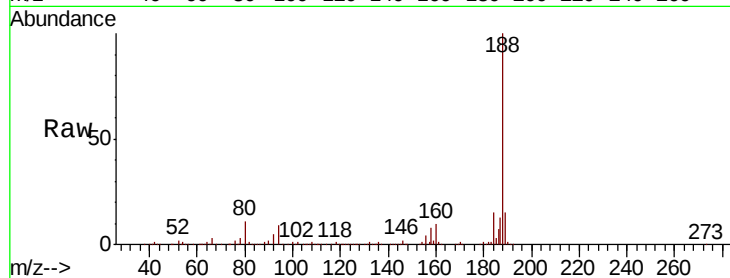

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

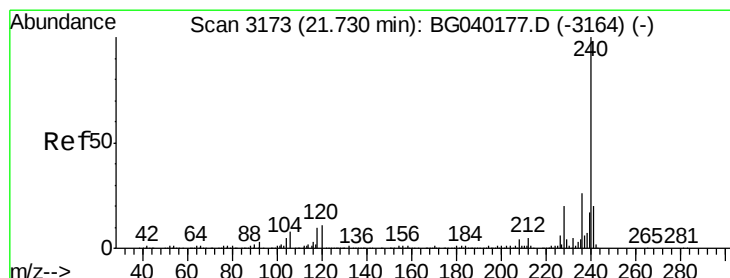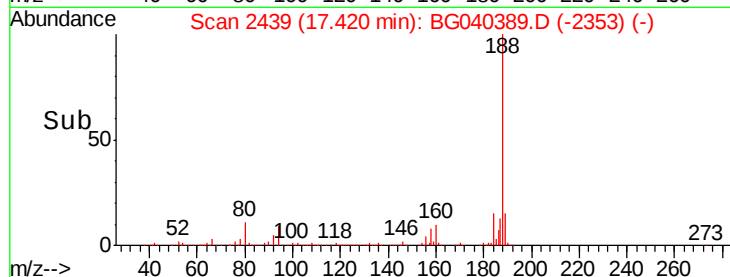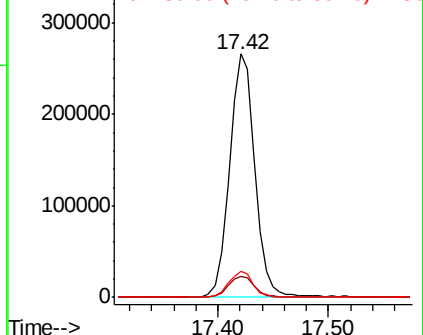

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3166

Delta R.T. -0.04 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05


Tgt Ion:240 Resp: 456398

Ion Ratio Lower Upper

240 100

120 10.6 8.4 12.6



236 25.6 20.8 31.2

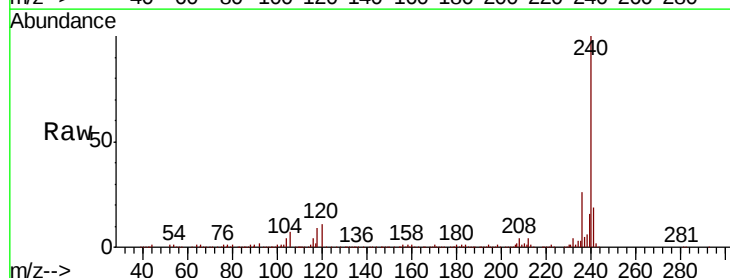

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

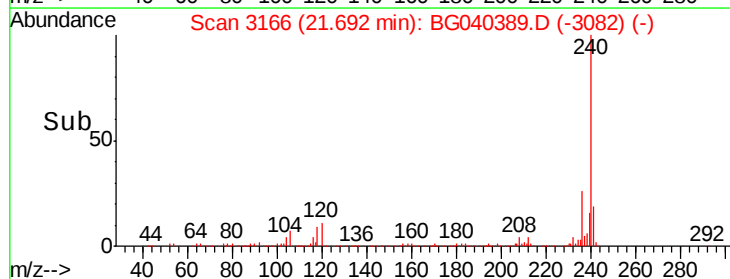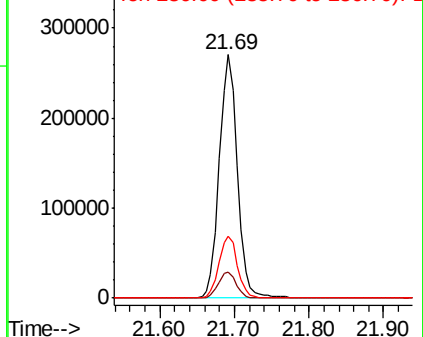



#79

Terphenyl-d14

Concen: 82.285 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.03 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05

Instrument :

BNA_G

ClientSampleId :

TWP-02


Tot Ion:244 Resp: 1669357

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.6




122 11.9 8.5 12.7

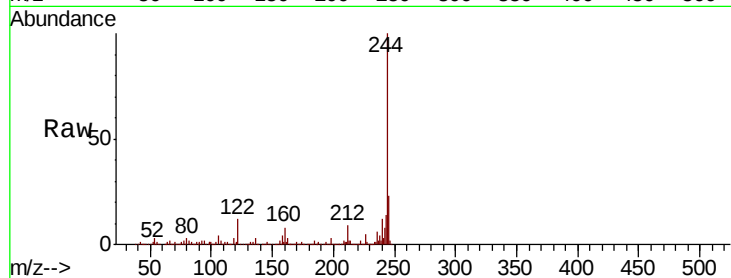

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

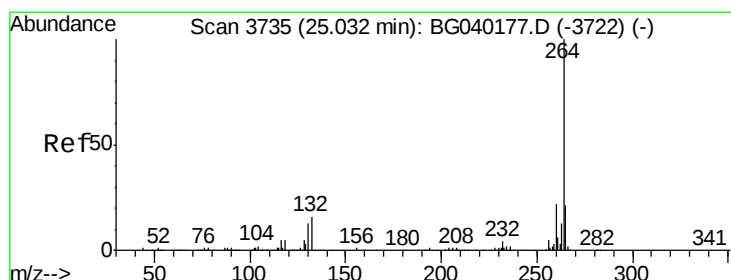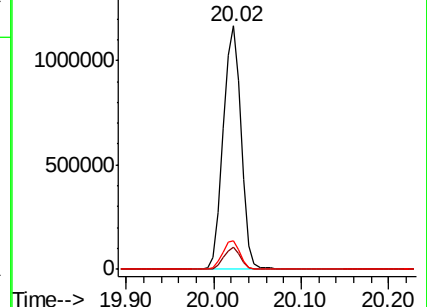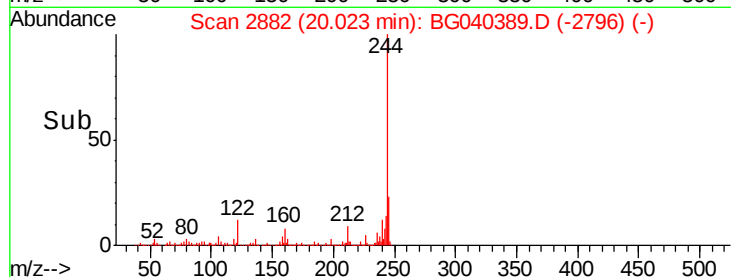

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.97 min Scan# 3724

Delta R.T. -0.06 min

Lab File: BG040389.D

Acq: 5 Apr 2019 23:05


Tgt Ion:264 Resp: 453161

Ion Ratio Lower Upper

264 100

260 23.7 17.9 26.9

265 21.3 16.8 25.2

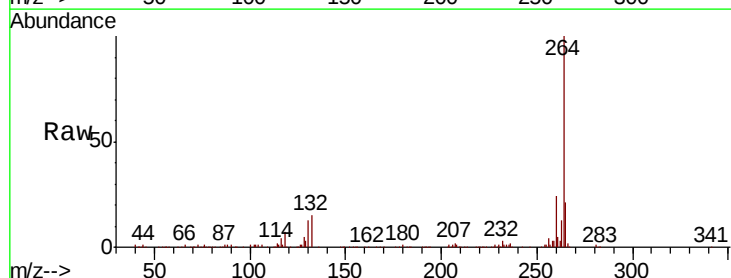

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

