

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
 Data File : BG040385.D
 Acq On : 5 Apr 2019 20:25
 Operator : JU/SJ
 Sample : PB118634BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB118634BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.603	418	428	443	rBV	1036944	1678642	43.14%	8.390%
2	7.201	690	700	714	rBV	1022955	1783412	45.83%	8.914%
3	7.577	756	764	774	rBV	997366	1728012	44.41%	8.637%
4	8.047	835	844	852	rVB	202684	354032	9.10%	1.770%
5	8.364	891	898	912	rBV	731144	1300550	33.42%	6.501%
6	9.222	1036	1044	1057	rBV	581054	1066550	27.41%	5.331%
7	10.861	1314	1323	1336	rBV	245450	474071	12.18%	2.370%
8	13.300	1730	1738	1753	rBV	1494653	2437886	62.65%	12.185%
9	14.675	1966	1972	1982	rBV3	380567	648844	16.67%	3.243%
10	16.161	2219	2225	2247	rBV	936130	1675996	43.07%	8.377%
11	17.418	2433	2439	2450	rBV2	519861	841221	21.62%	4.205%
12	20.021	2876	2882	2895	rBV	2912152	3891231	100.00%	19.450%
13	21.690	3159	3166	3177	rBV	601034	1098231	28.22%	5.489%
14	24.968	3714	3724	3741	rVB2	339089	1028040	26.42%	5.138%


Sum of corrected areas: 20006718

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
Data File : BG040385.D
Acq On : 5 Apr 2019 20:25
Operator : JU/SJ
Sample : PB118634BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

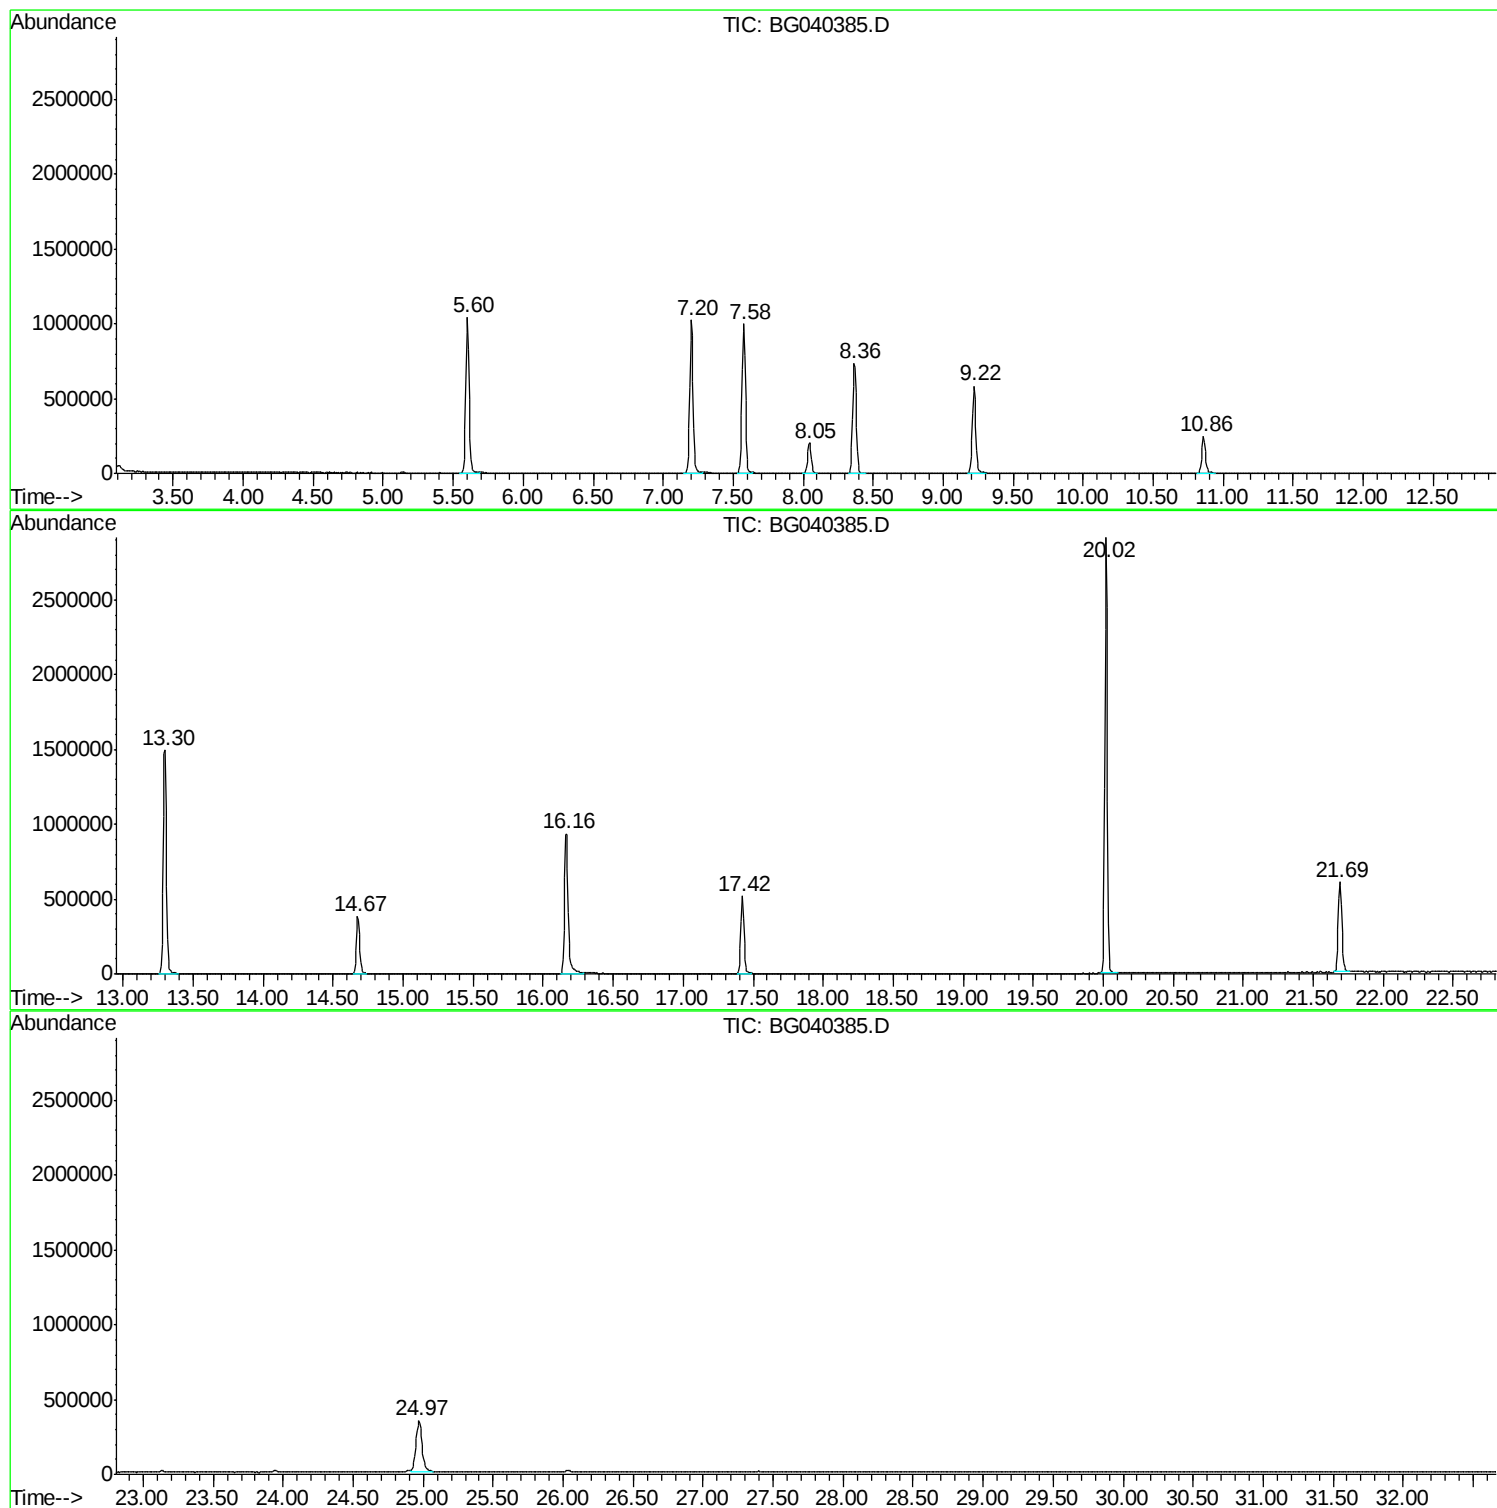

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040519\
Data File : BG040385.D
Acq On : 5 Apr 2019 20:25
Operator : JU/SJ
Sample : PB118634BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118634BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	97.62 ng	1728010	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

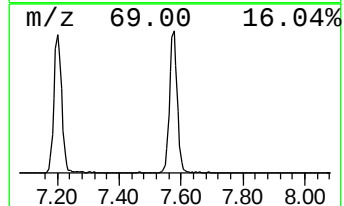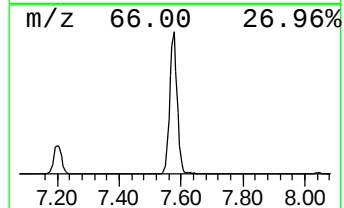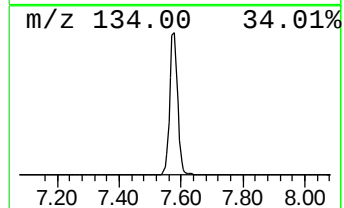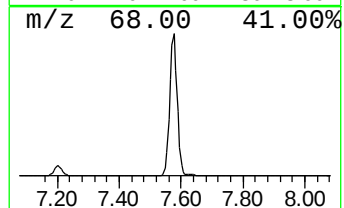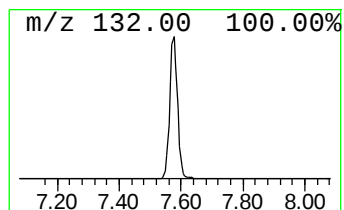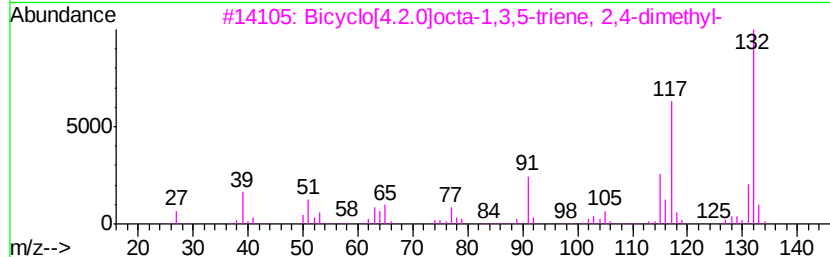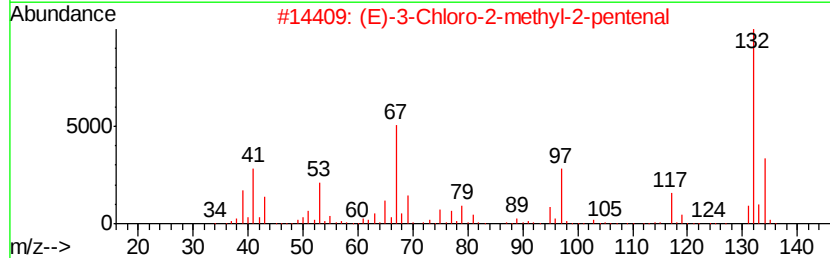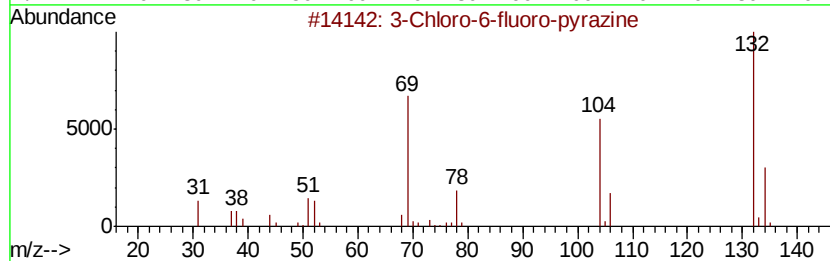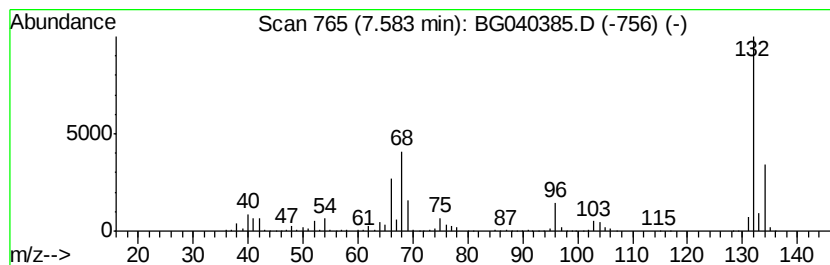

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040519\
Data File : BG040385.D
Acq On : 5 Apr 2019 20:25
Operator : JU/SJ
Sample : PB118634BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	97.6	ng	1728010	1	8.05	354032	20.0