
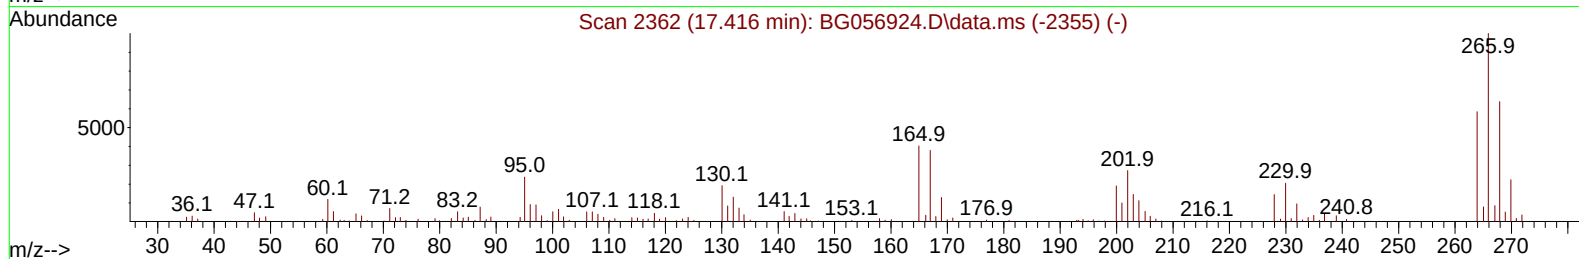
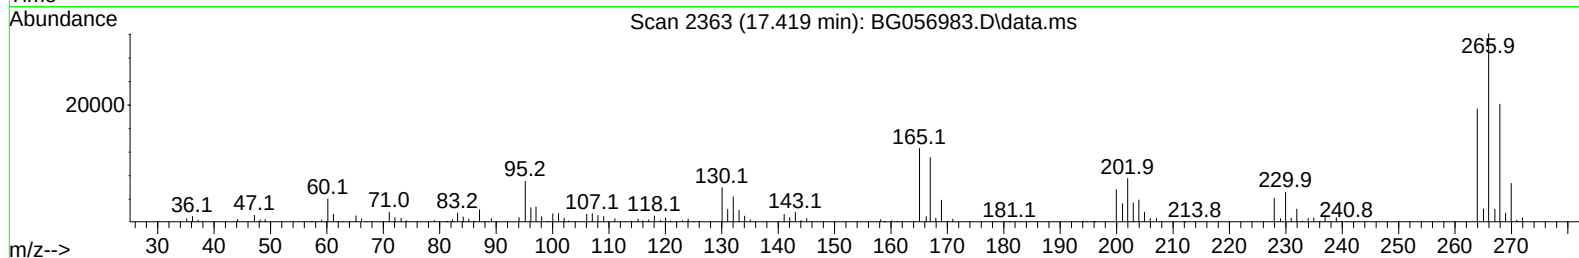


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056983.D
Acq On : 5 Apr 2023 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 01:57:04 2023
Response via : Initial Calibration

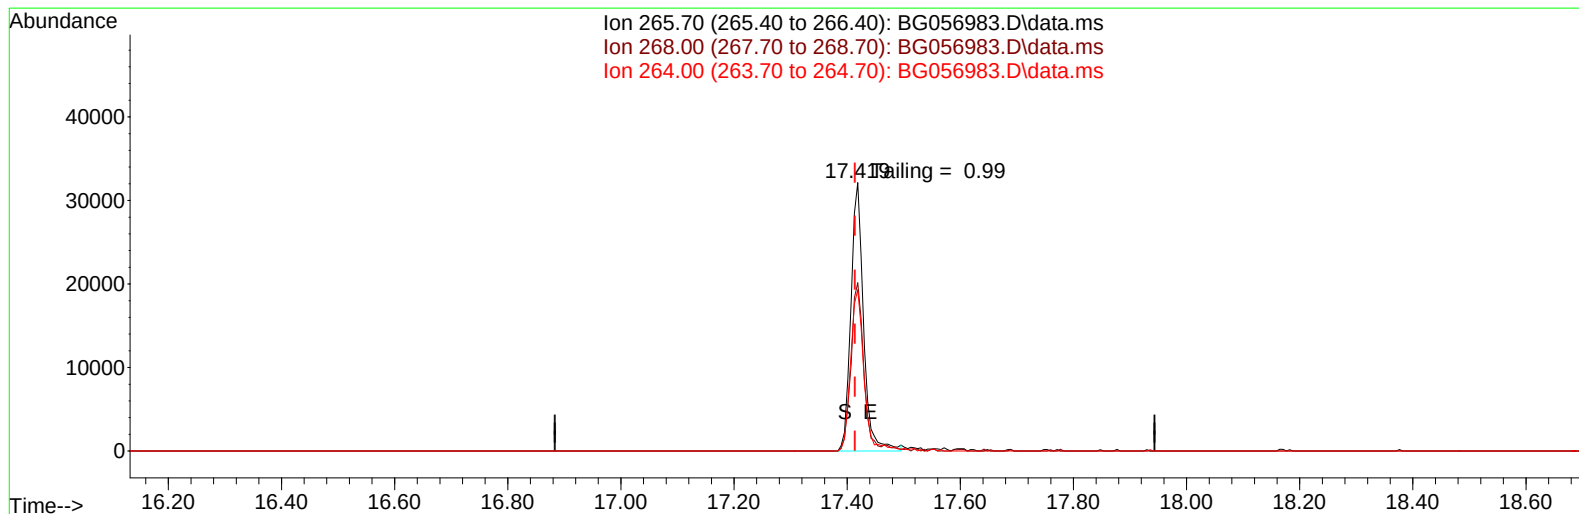

TIC: BG056983.D\data.ms

(70) Pentachlorophenol (C)




17.419min (+ 0.005) 19680.79 ng

response 49743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.71
264.00	58.50	60.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056983.D
Acq On : 5 Apr 2023 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 01:57:04 2023
Response via : Initial Calibration

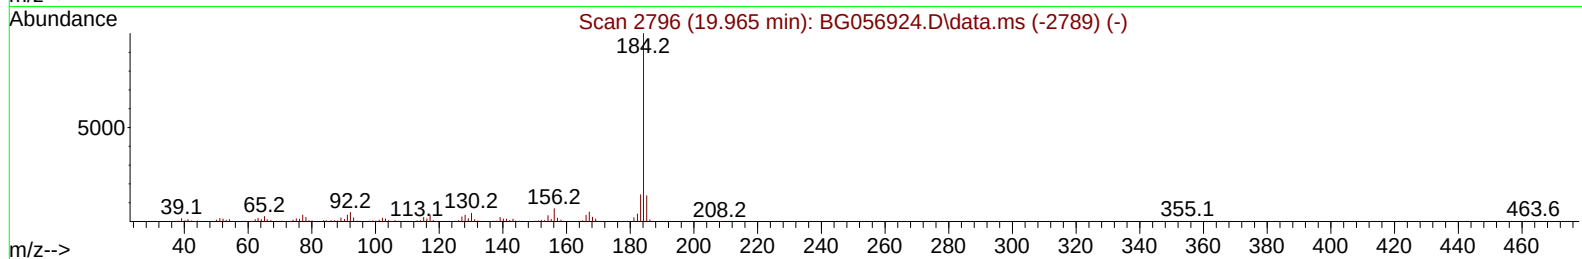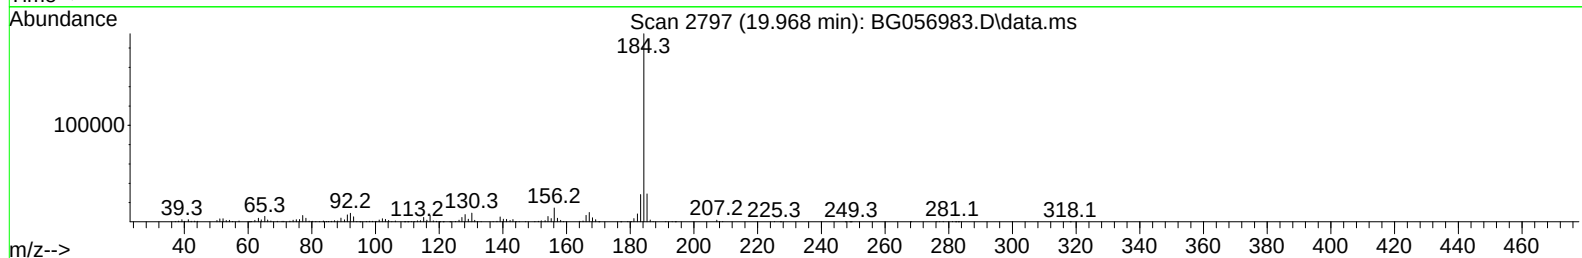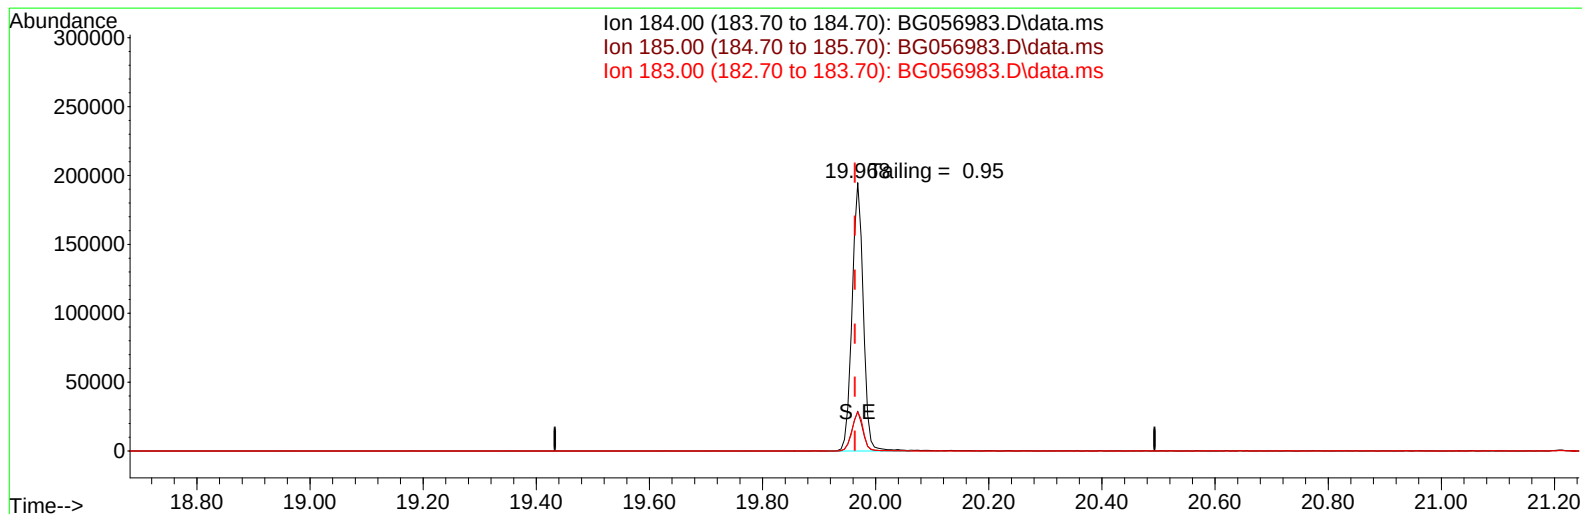

TIC: BG056983.D\data.ms

(77) Benzidine**19.968min (+ 0.005) 150814.84 ng****response 267947**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.87
183.00	14.20	14.53
0.00	0.00	0.00