
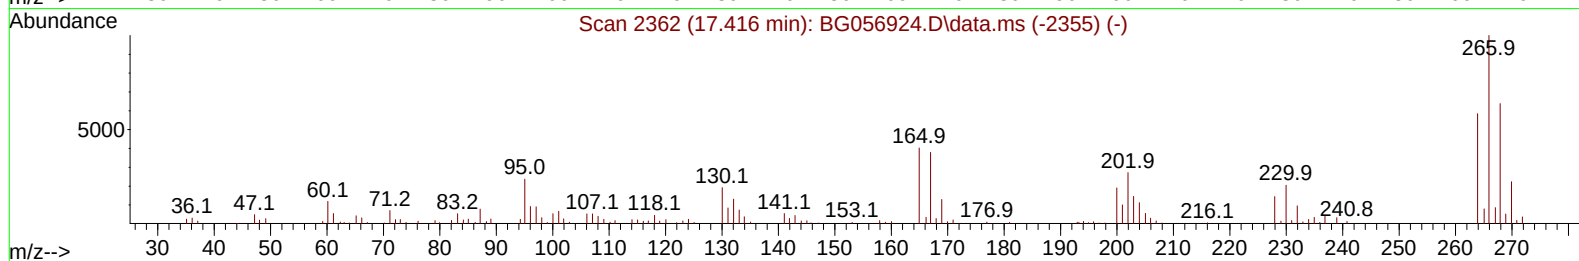
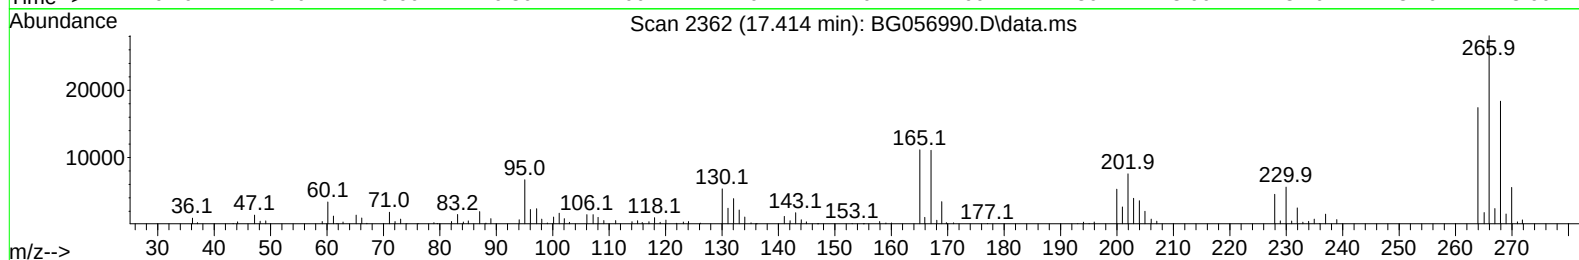


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056990.D
Acq On : 5 Apr 2023 14:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:15:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 01:57:04 2023
Response via : Initial Calibration

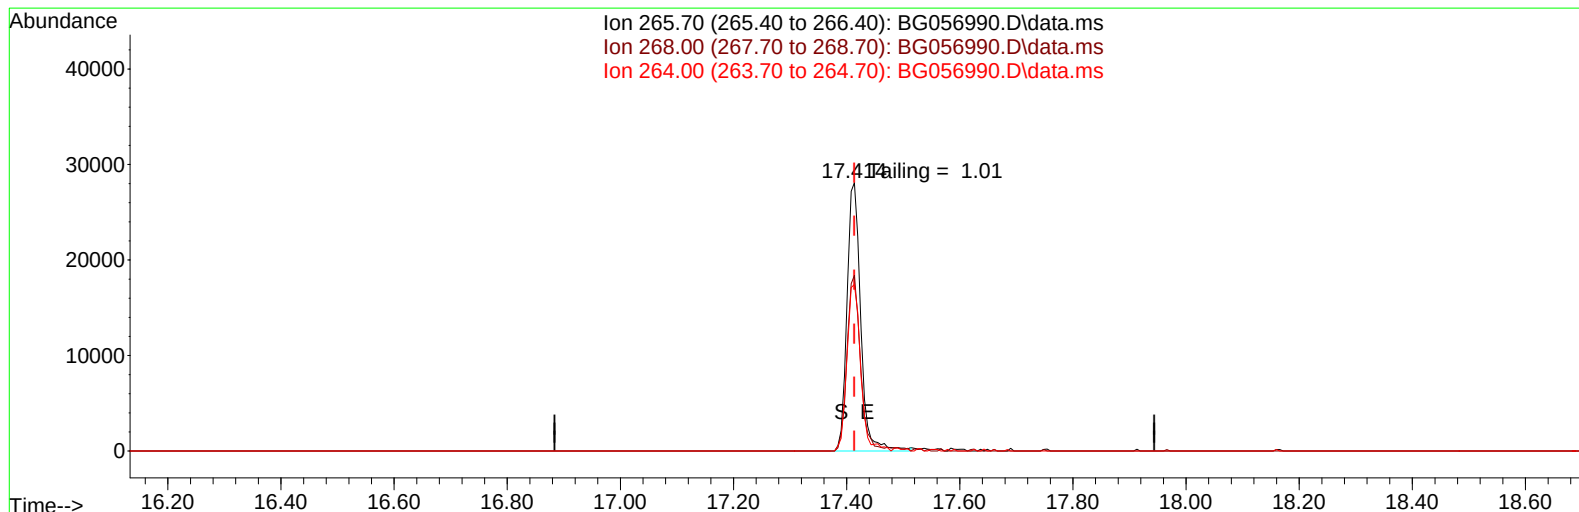

TIC: BG056990.D\data.ms

(70) Pentachlorophenol (C)




17.414min (+ 0.000) 32235.42 ng

response 47244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.41
264.00	58.50	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
 Data File : BG056990.D
 Acq On : 5 Apr 2023 14:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 04:15:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 01:57:04 2023
 Response via : Initial Calibration

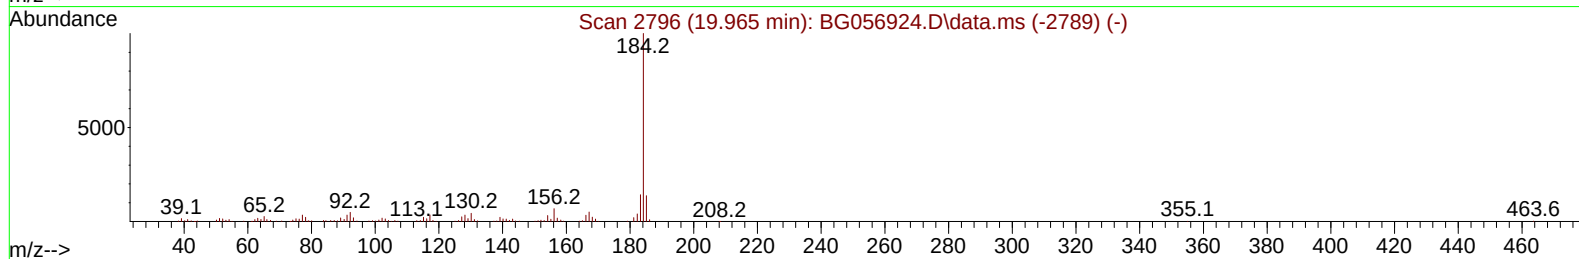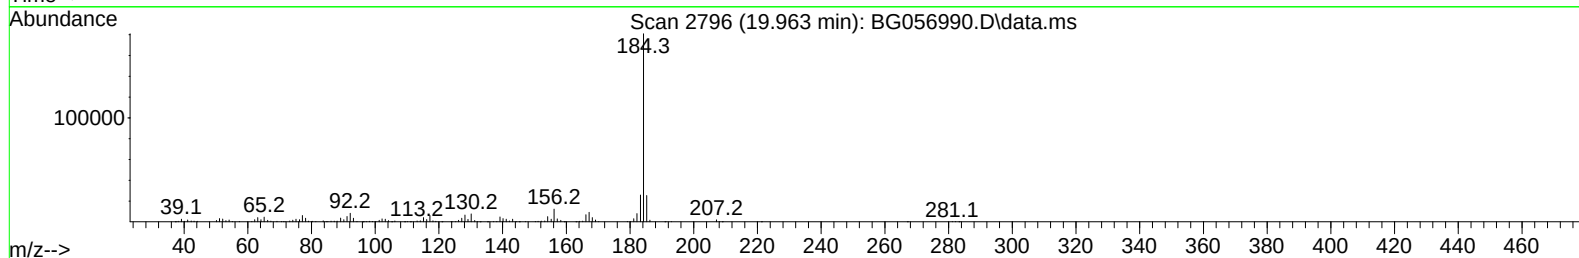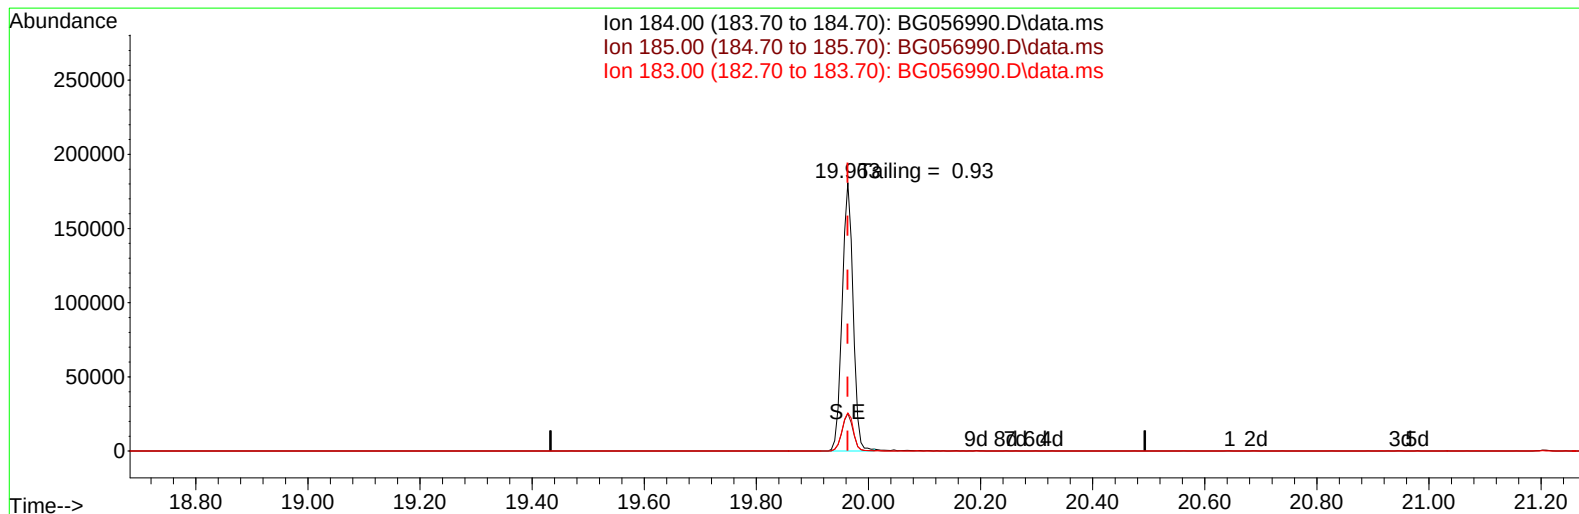

TIC: BG056990.D\data.ms

(77) Benzidine

19.963min (+ 0.000) 159402.21 ng m

response 248348

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.02
183.00	14.20	14.28
0.00	0.00	0.00