


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
 Data File : BG056983.D
 Acq On : 5 Apr 2023 9:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 01:57:04 2023

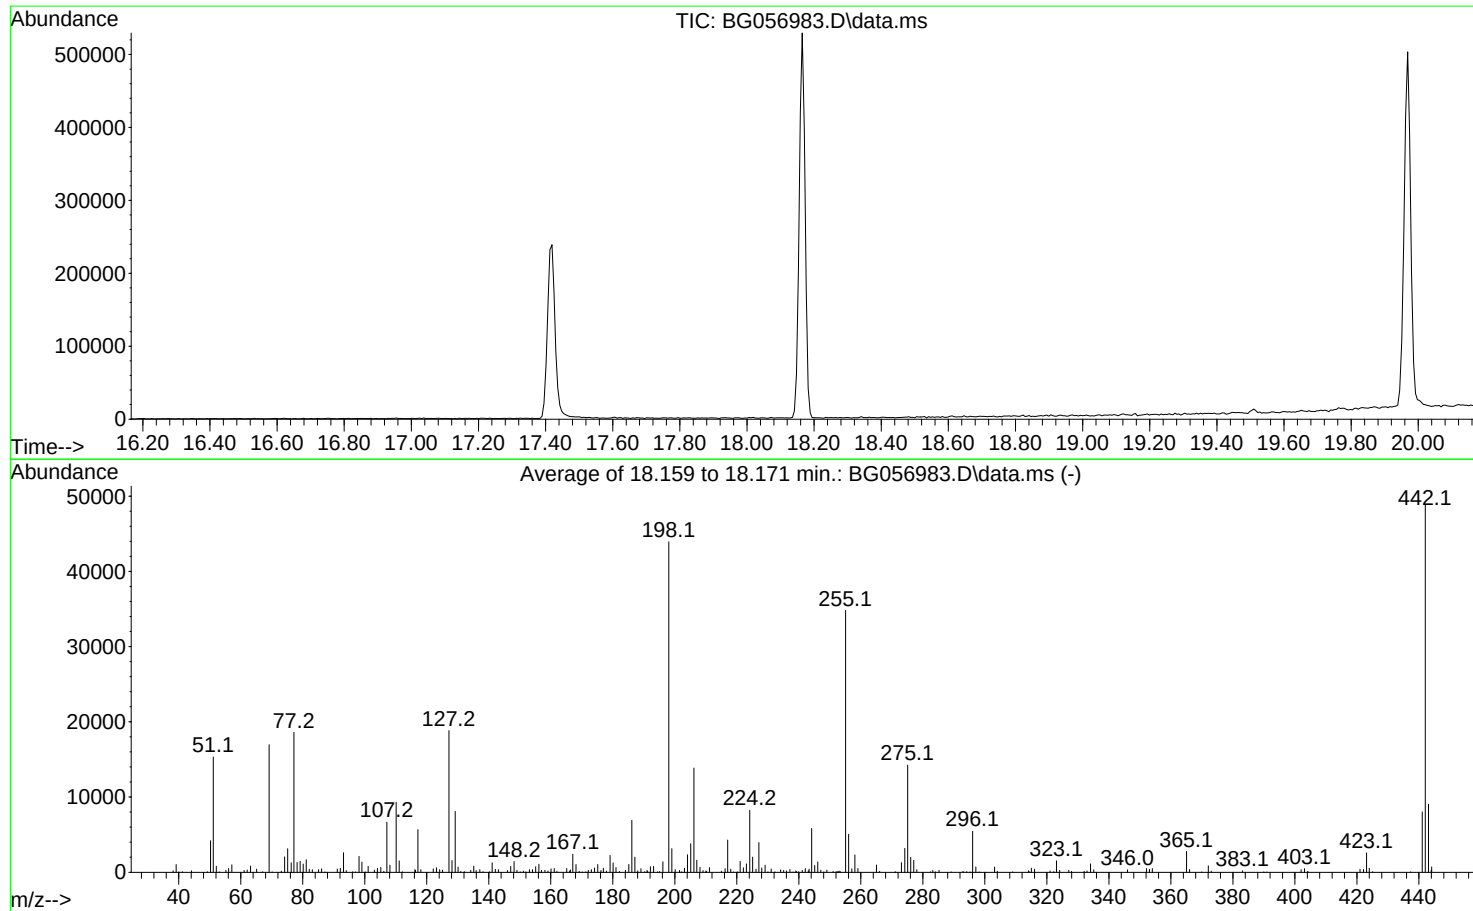




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	15330	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	16962	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	42.9	18836	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43941	PASS
199	198	5	9	7.2	3148	PASS
275	198	10	60	32.4	14234	PASS
365	198	1	100	6.3	2786	PASS
441	198	0.01	100	18.3	8023	PASS
442	442	50	100	100.0	48899	PASS
443	442	15	24	18.5	9050	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056983.D
Acq On : 5 Apr 2023 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 04:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 01:57:04 2023
Response via : Initial Calibration

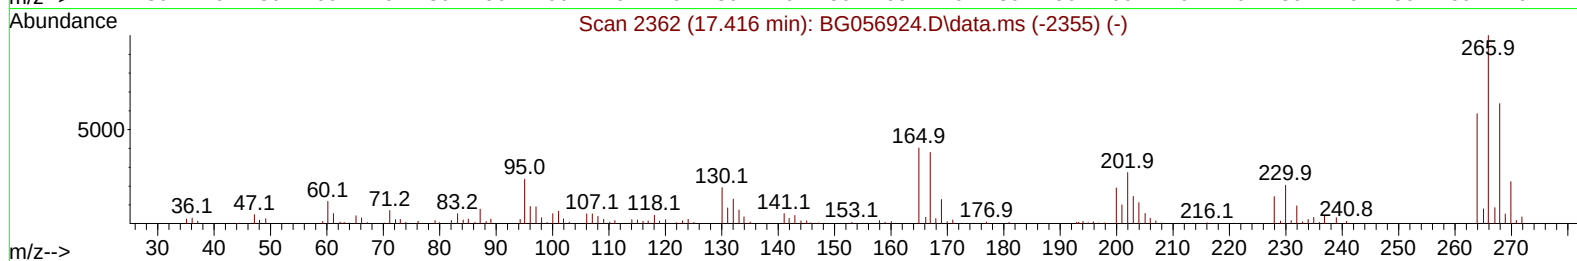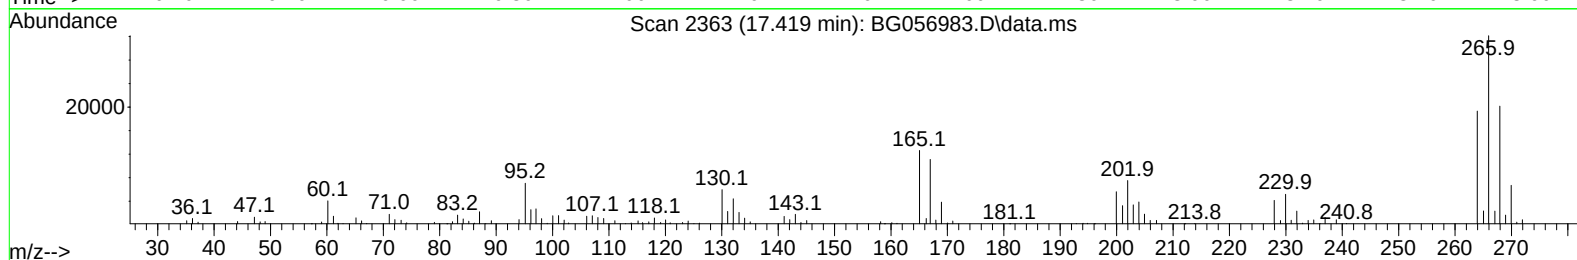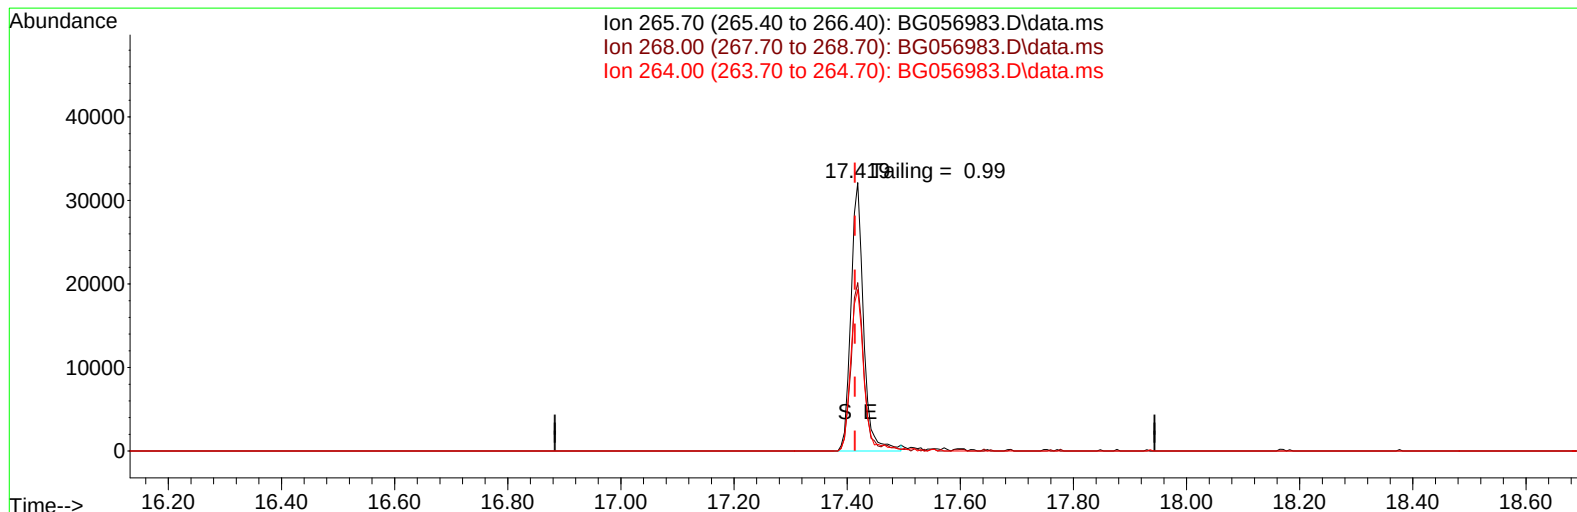

TIC: BG056983.D\data.ms

(70) Pentachlorophenol (C)

17.419min (+ 0.005) 19680.79 ng




response 49743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.71
264.00	58.50	60.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056983.D
Acq On : 5 Apr 2023 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 04:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 01:57:04 2023
Response via : Initial Calibration

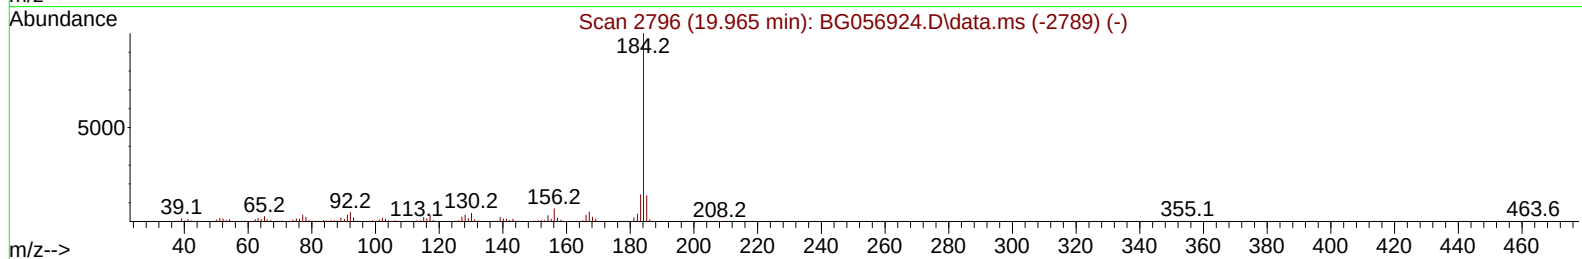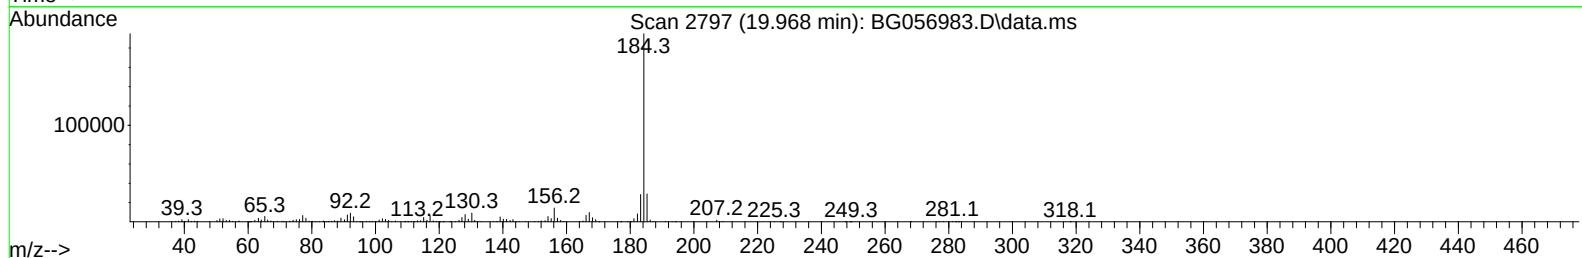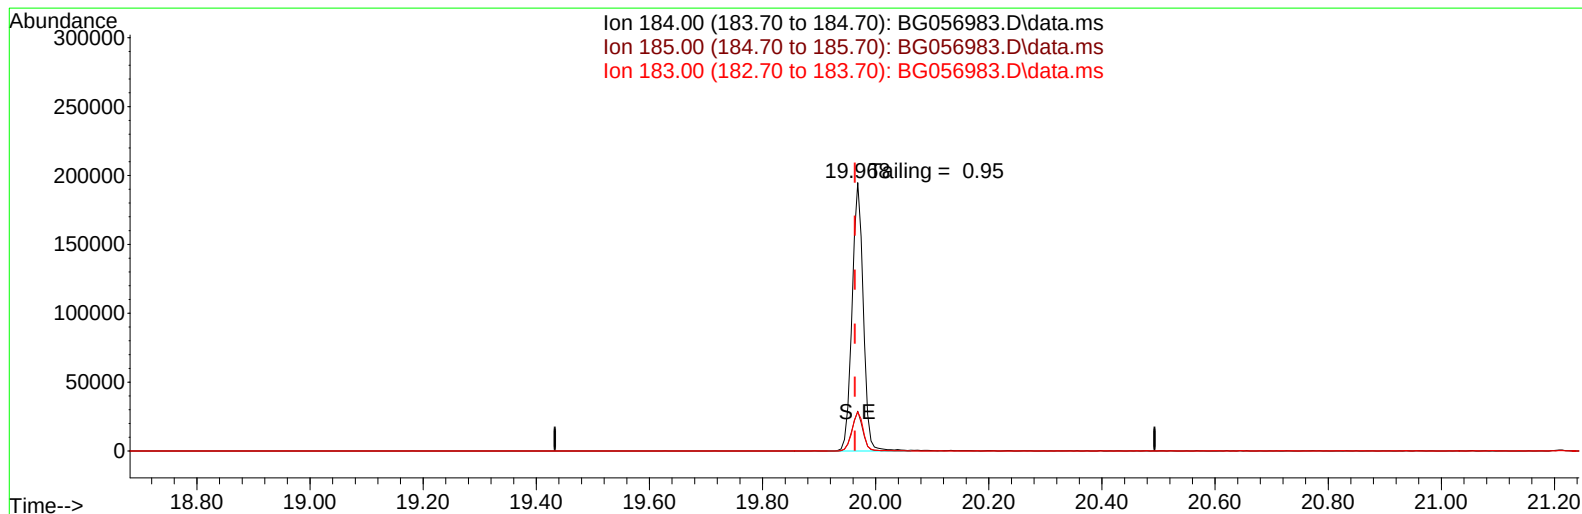

TIC: BG056983.D\data.ms

(77) Benzidine

19.968min (+ 0.005) 150814.84 ng

response 267947

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.87
183.00	14.20	14.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2023	BNA_G	<u>BG056983.D</u>
Compound Name	Response	Retention Time
DDT	120963	21.214
DDD	3662	20.75
DDE	0	20.245
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3662	124625	2.94

Instrument :
BNA_G
ClientSampleId :
DFTPP