


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056990.D
Acq On : 5 Apr 2023 14:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 06 01:57:04 2023

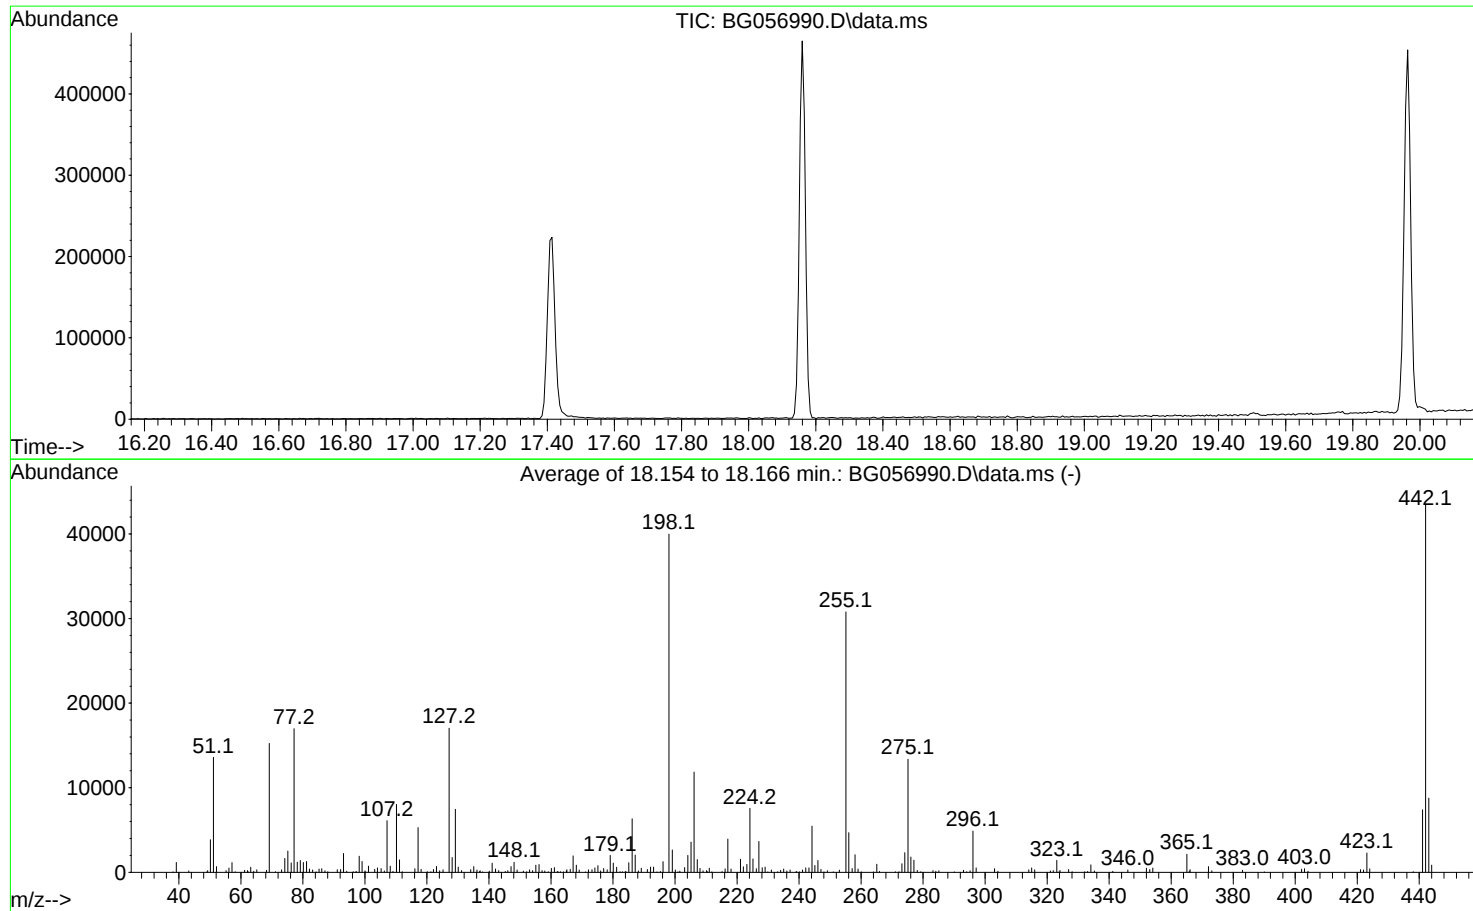




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	13585	PASS
68	69	0.00	2	1.6	247	PASS
69	198	0.00	100	38.1	15249	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	17028	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39989	PASS
199	198	5	9	6.6	2636	PASS
275	198	10	60	33.4	13361	PASS
365	198	1	100	5.3	2121	PASS
441	198	0.01	100	18.5	7395	PASS
442	442	50	100	100.0	43493	PASS
443	442	15	24	20.2	8767	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
Data File : BG056990.D
Acq On : 5 Apr 2023 14:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 06 04:15:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 01:57:04 2023
Response via : Initial Calibration

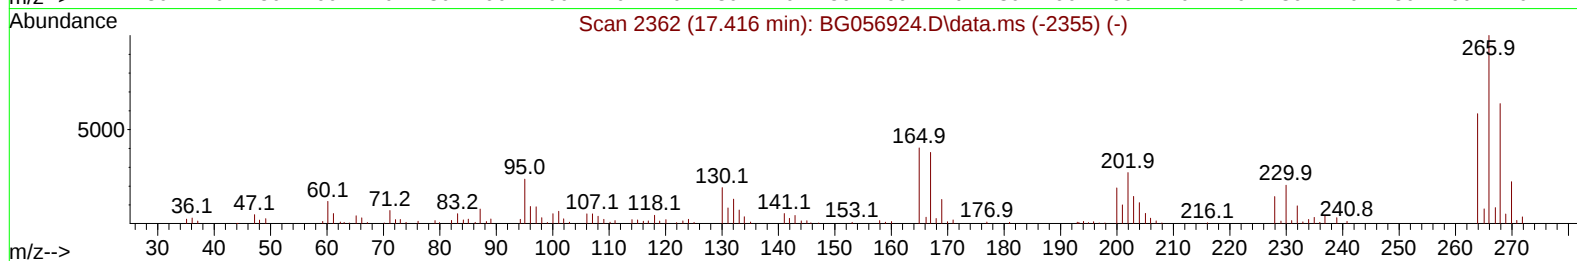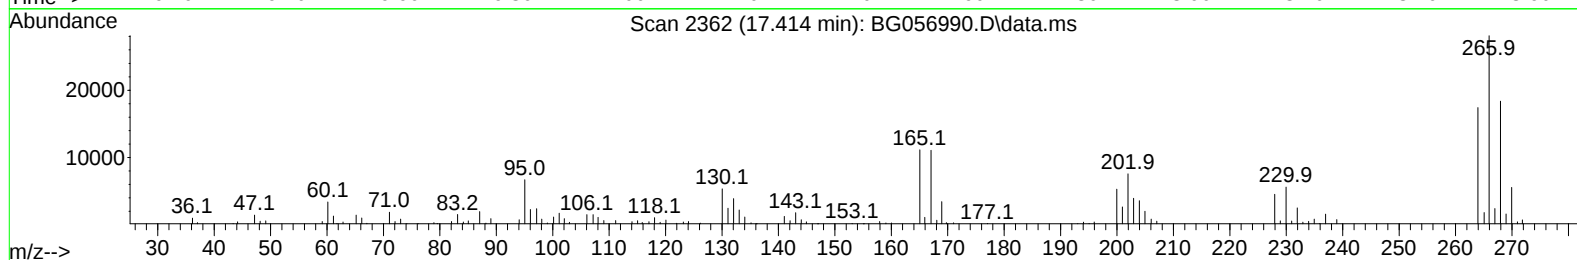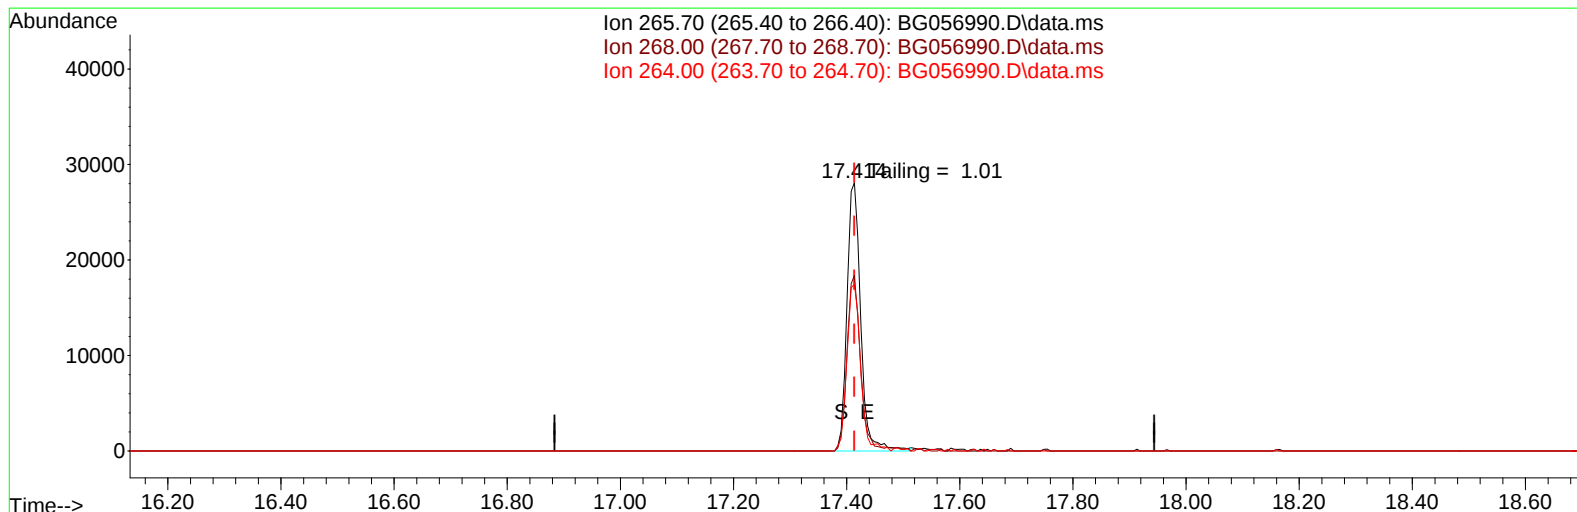

TIC: BG056990.D\data.ms

(70) Pentachlorophenol (C)

17.414min (+ 0.000) 32235.42 ng




response 47244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.41
264.00	58.50	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040523\
 Data File : BG056990.D
 Acq On : 5 Apr 2023 14:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 06 04:15:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 01:57:04 2023
 Response via : Initial Calibration

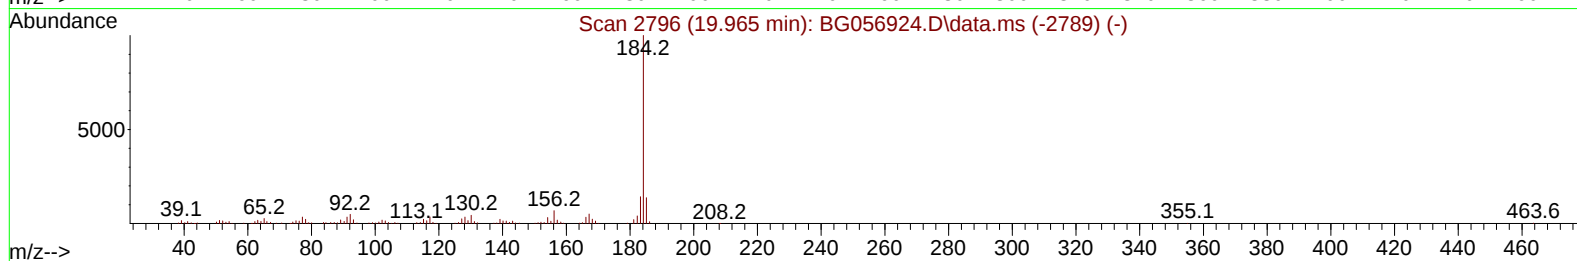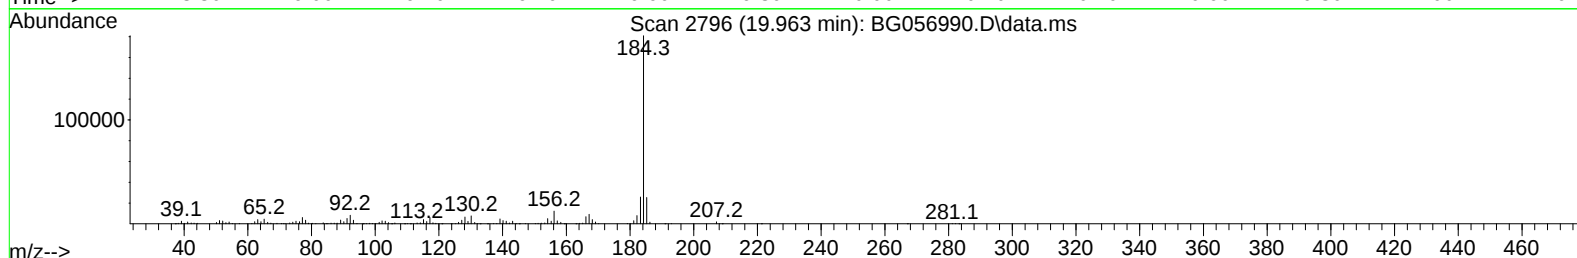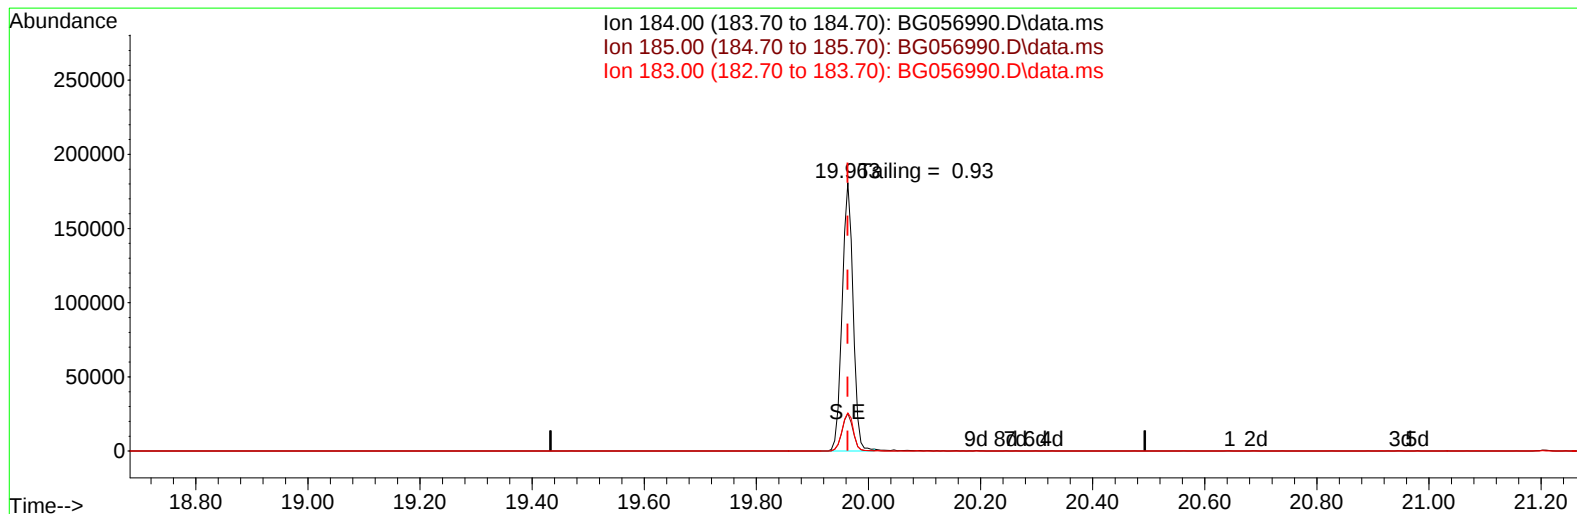

TIC: BG056990.D\data.ms

(77) Benzidine

19.963min (+ 0.000) 159402.21 ng m

response 248348

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.02
183.00	14.20	14.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2023	BNA_G	BG056990.D
Compound Name	Response	Retention Time
DDT	122876	21.209
DDD	3100	20.739
DDE	132	20.245
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3232	126108	2.56

Instrument :
BNA_G
ClientSampleId :
DFTPP