


Data Path : Z:\HPCHEM1\BNA_G\Data\BG040615\
 Data File : BG016223.D
 Acq On : 6 Apr 2015 14:52
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 07 04:17:17 2015

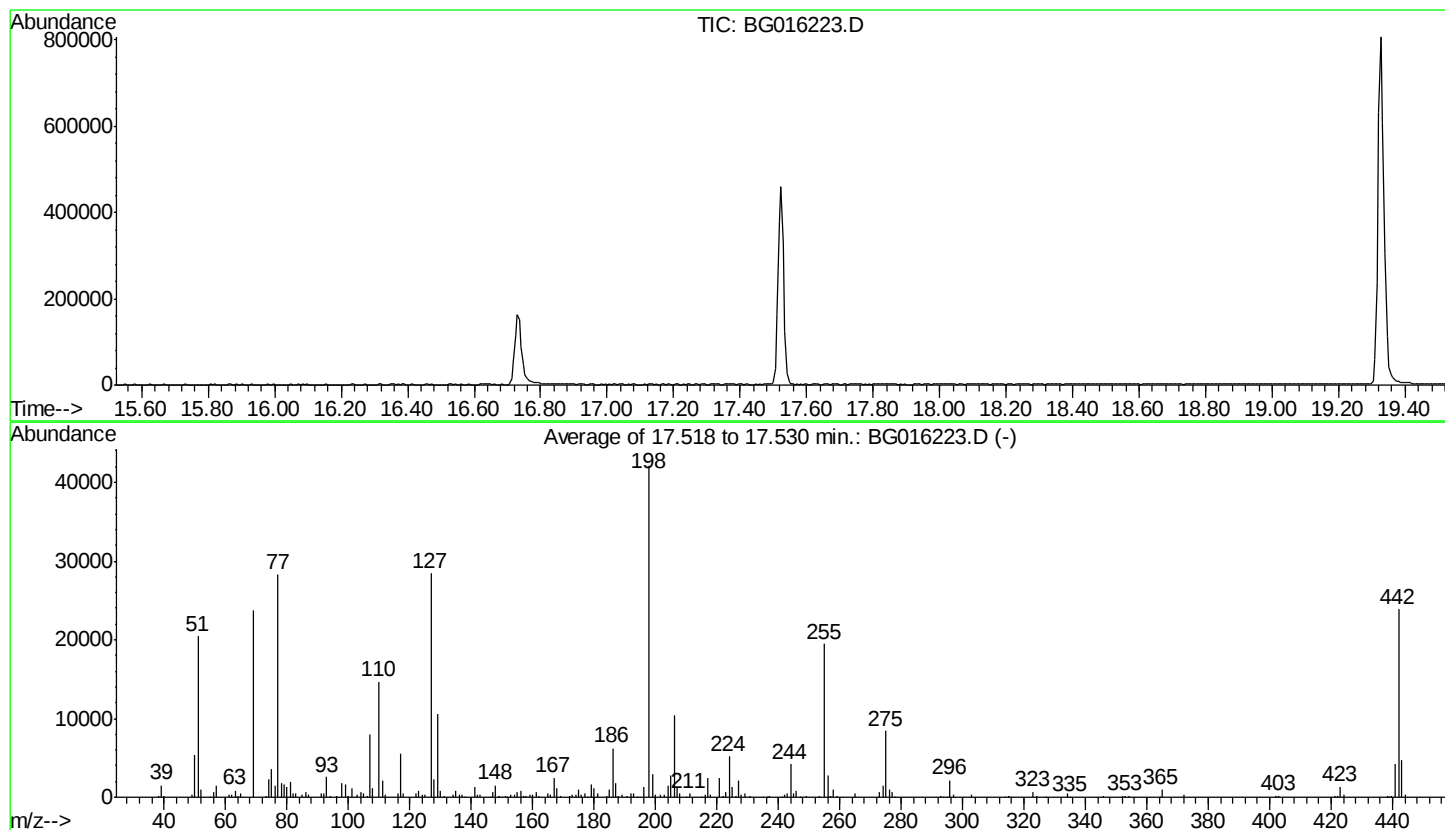

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	20429	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.2	23669	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	67.5	28432	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42128	PASS
199	198	5	9	7.0	2964	PASS
275	198	10	60	20.1	8447	PASS
365	198	1	100	2.2	923	PASS
441	442	0.01	24	18.1	4314	PASS
442	198	50	100	56.7	23888	PASS
443	442	15	24	19.7	4707	PASS