
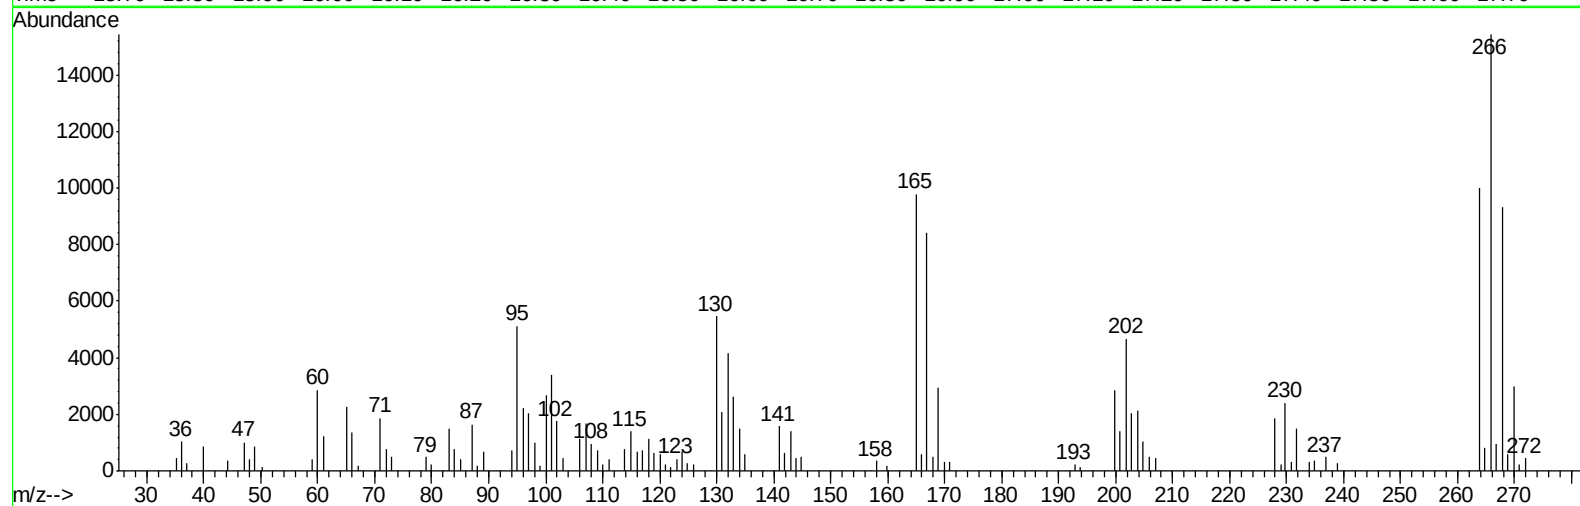


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040615\
Data File : BG016223.D
Acq On : 6 Apr 2015 14:52
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:18:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 07:38:11 2015
Response via : Initial Calibration

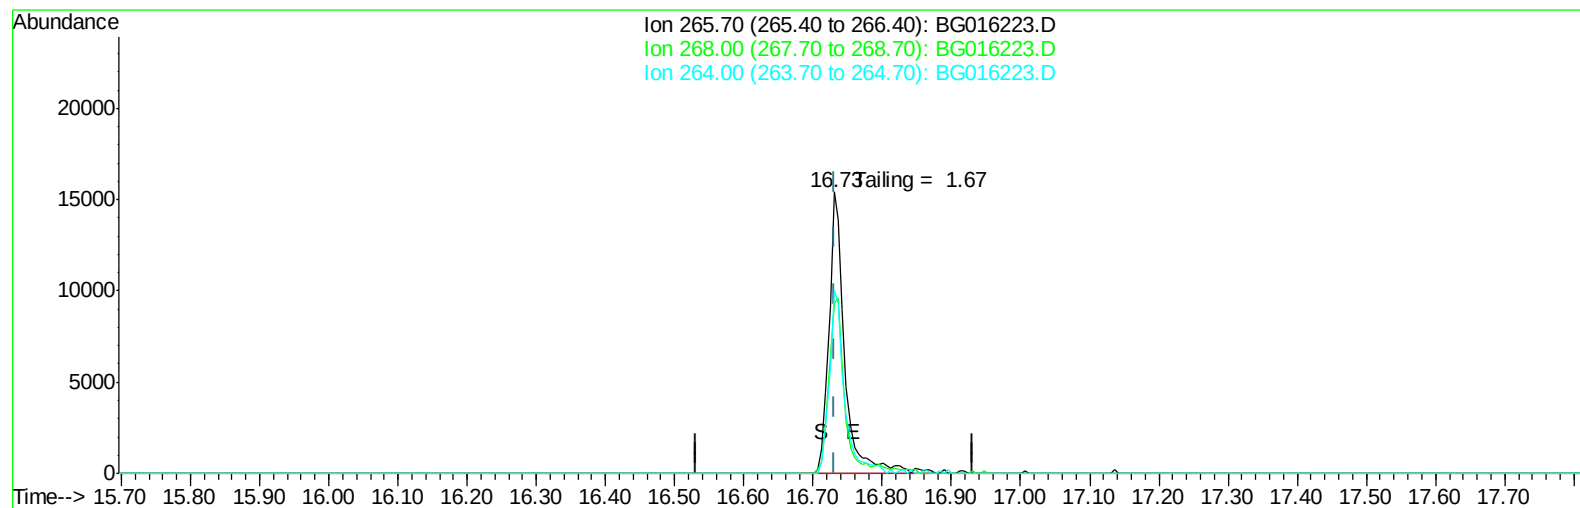

TIC: BG016223.D

(69) Pentachlorophenol (C)



16.730min (-0.001) 0.00ng

response 23939

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	60.52
264.00	66.00	64.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040615\
Data File : BG016223.D
Acq On : 6 Apr 2015 14:52
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:18:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 07:38:11 2015
Response via : Initial Calibration

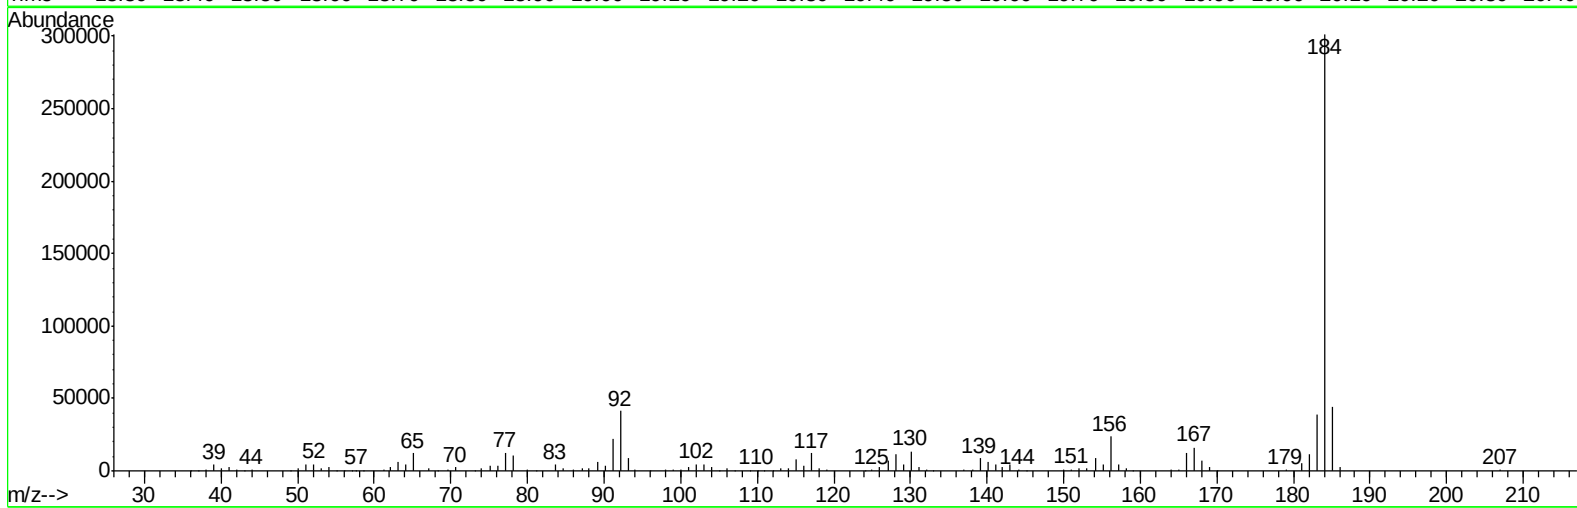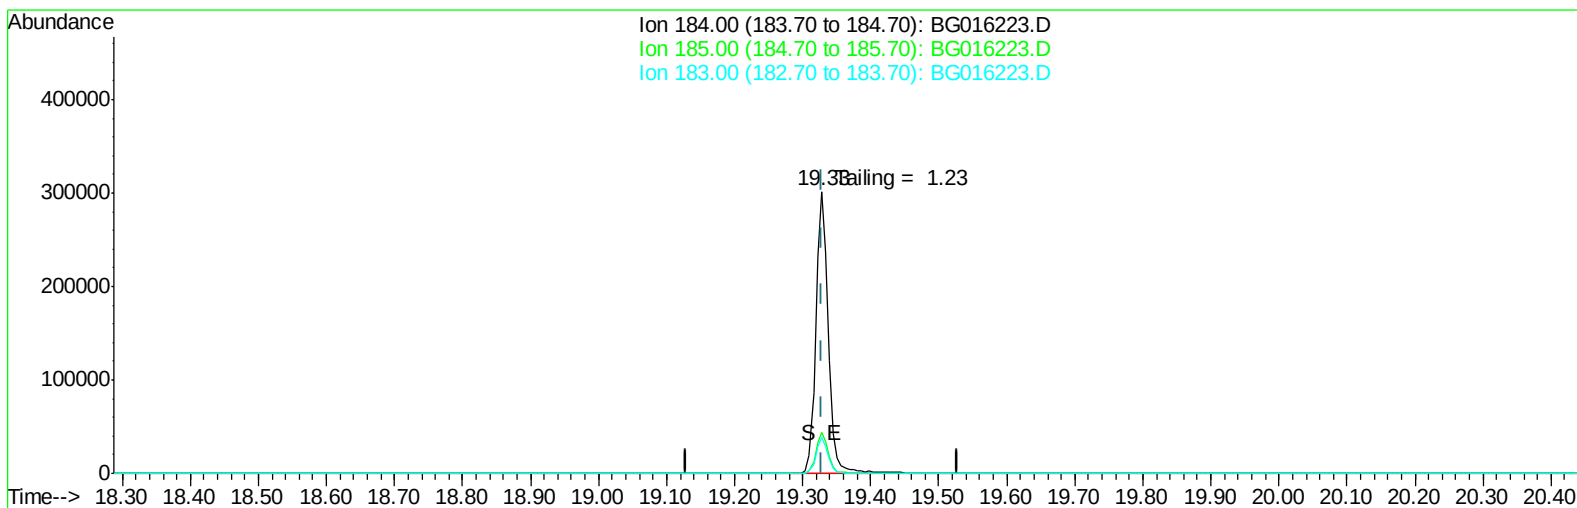

TIC: BG016223.D

(76) Benzidine

19.327min (-0.001) 0.00ng

response 387618

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.64
183.00	13.00	12.81
0.00	0.00	0.00