
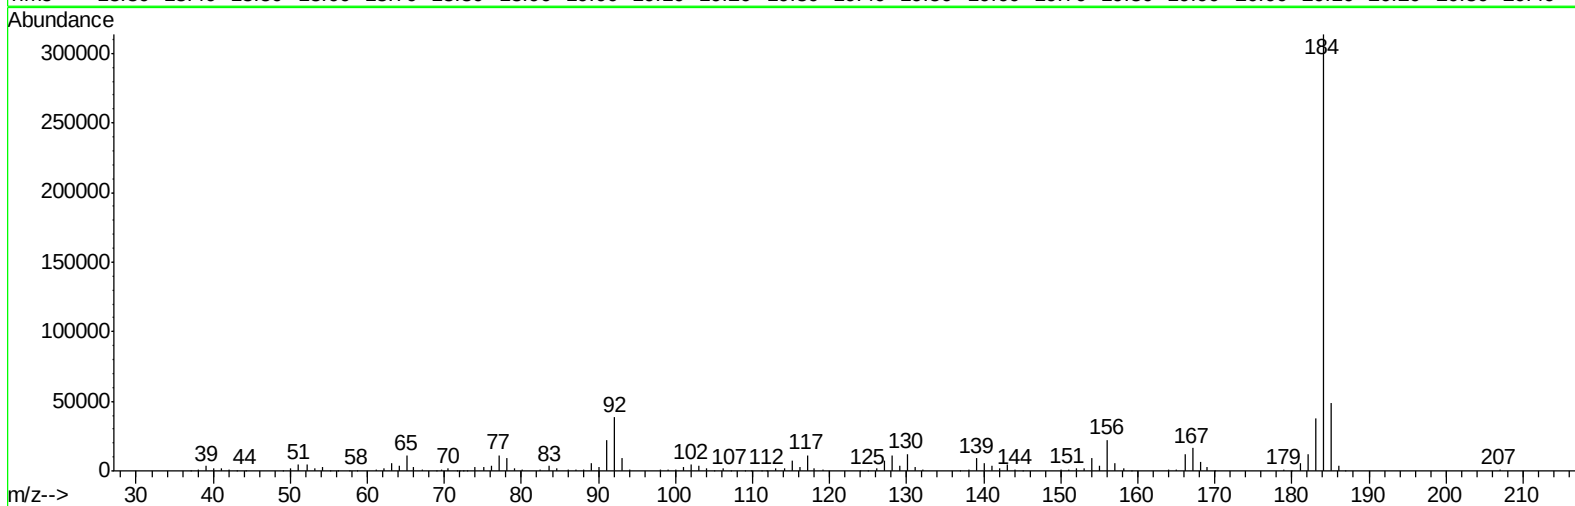


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG040615\
Data File : BG016241.D
Acq On : 7 Apr 2015 2:02
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:18:58 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 07:38:11 2015
Response via : Initial Calibration

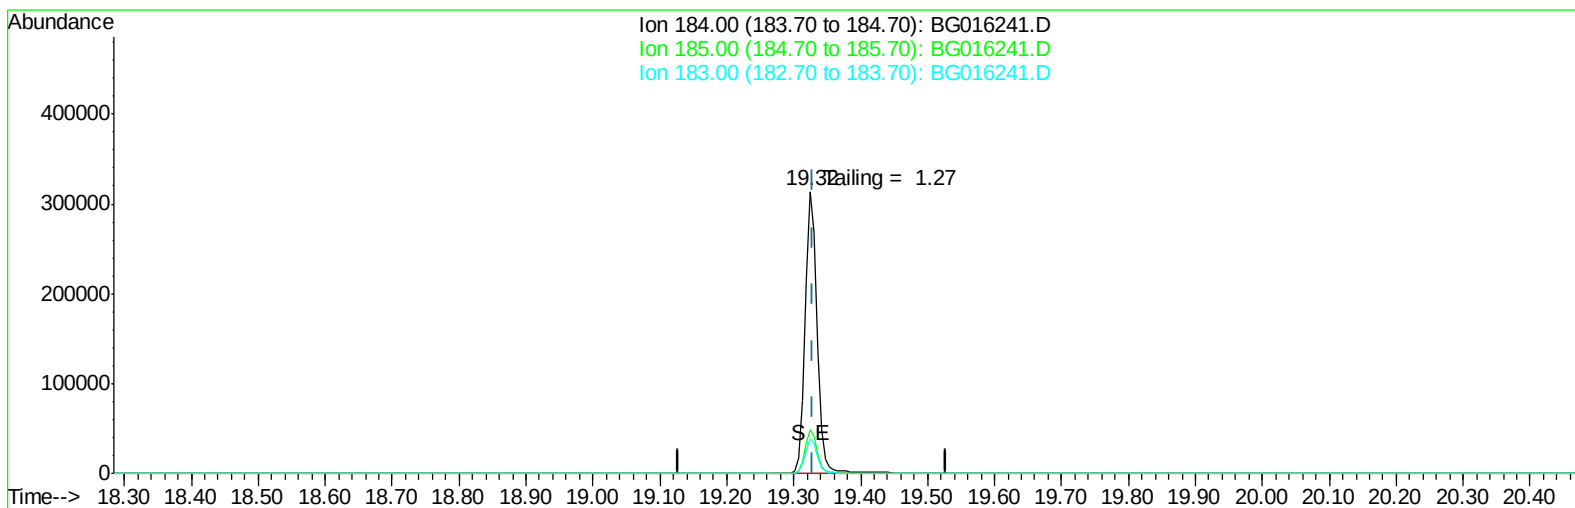

TIC: BG016241.D

(76) Benzidine

19.324min (-0.005) 0.00ng

response 401607

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.55
183.00	13.00	12.17
0.00	0.00	0.00