
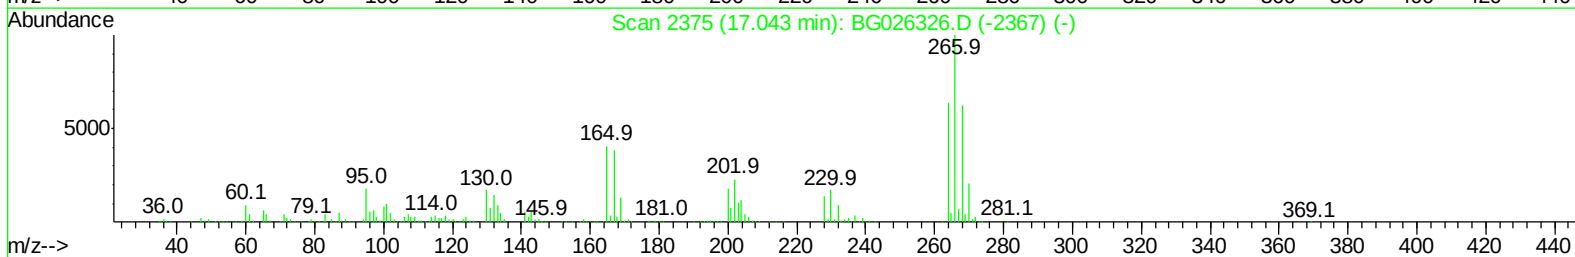
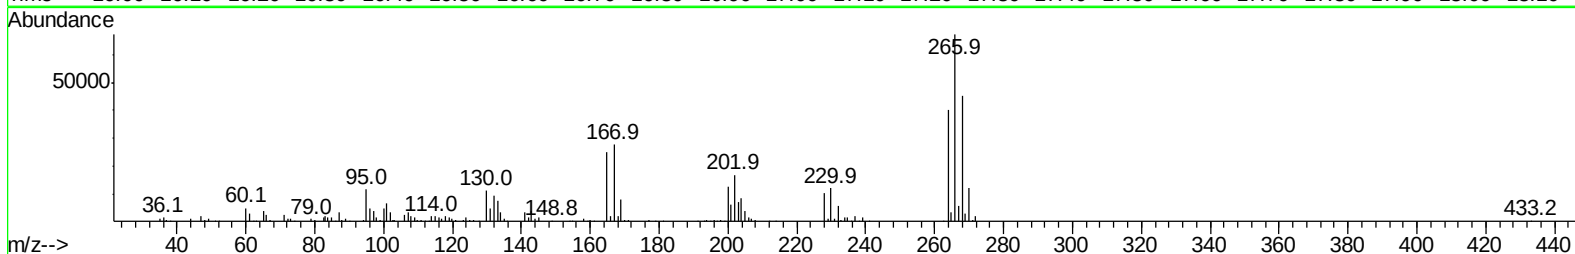


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040617\
Data File : BG026585.D
Acq On : 7 Apr 2017 3:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:32:30 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

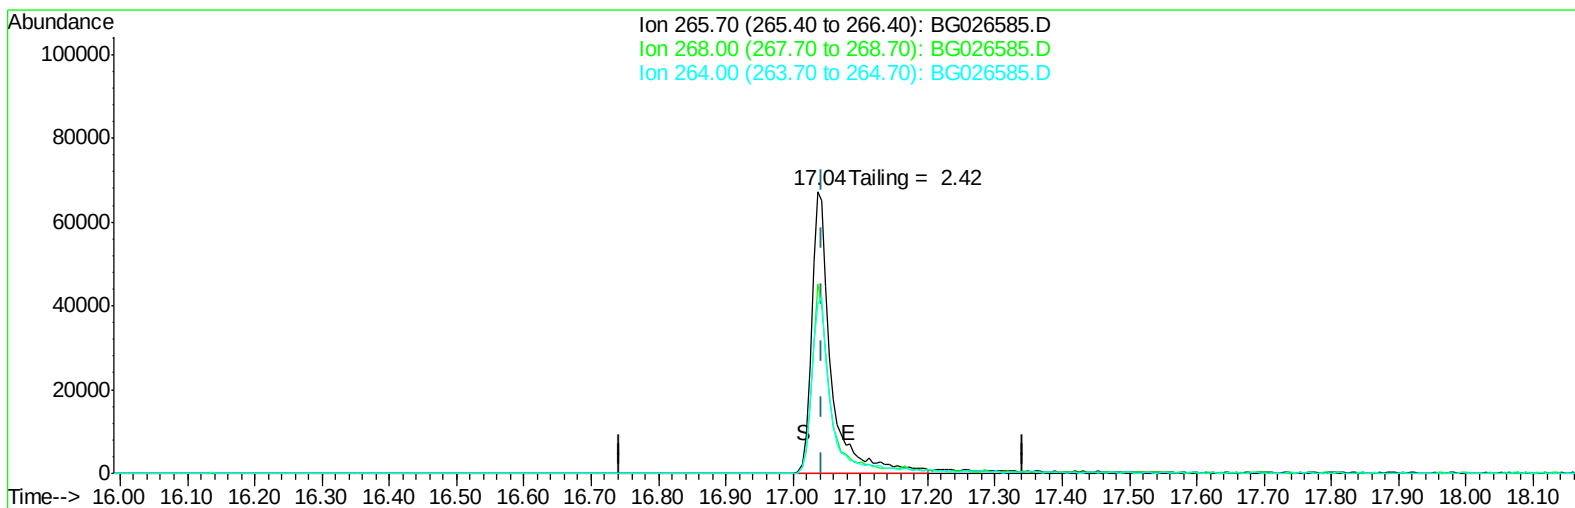

TIC: BG026585.D

(69) Pentachlorophenol (C)




17.036min (-0.006) 0.00ng

response 134363

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	67.42
264.00	62.60	60.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG040617\
Data File : BG026585.D
Acq On : 7 Apr 2017 3:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:32:30 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

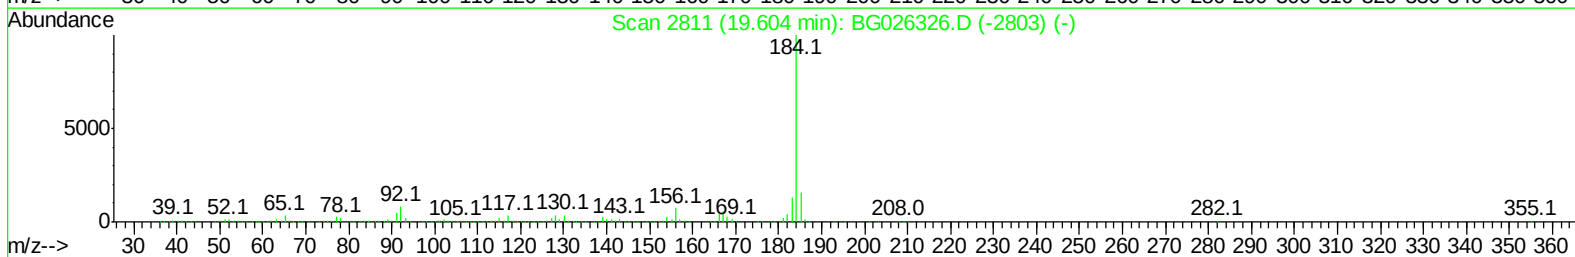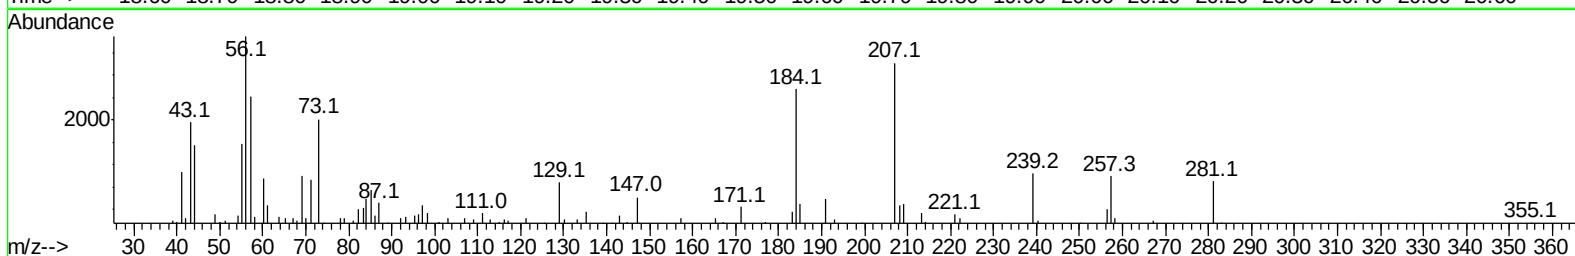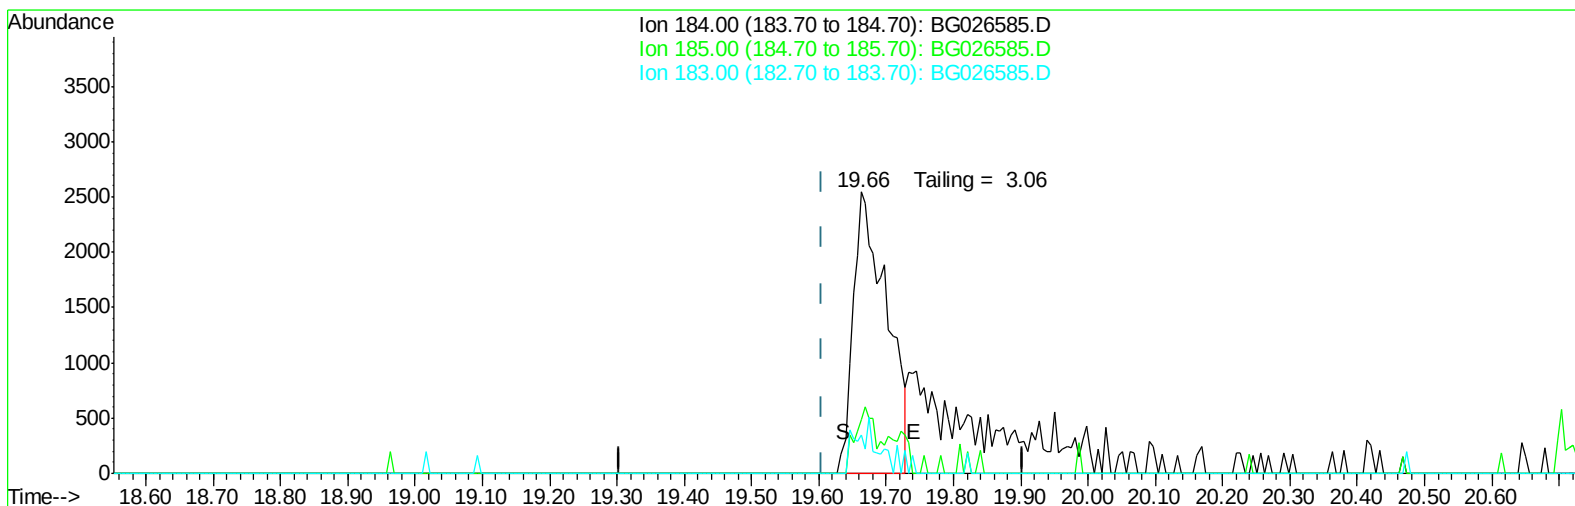

TIC: BG026585.D

(76) Benzidine

19.663min (+0.059) 321.85ng

response 8822

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	19.00
183.00	13.80	13.74
0.00	0.00	0.00