


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040617\
 Data File : BG026568.D
 Acq On : 6 Apr 2017 15:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 20 17:43:27 2017

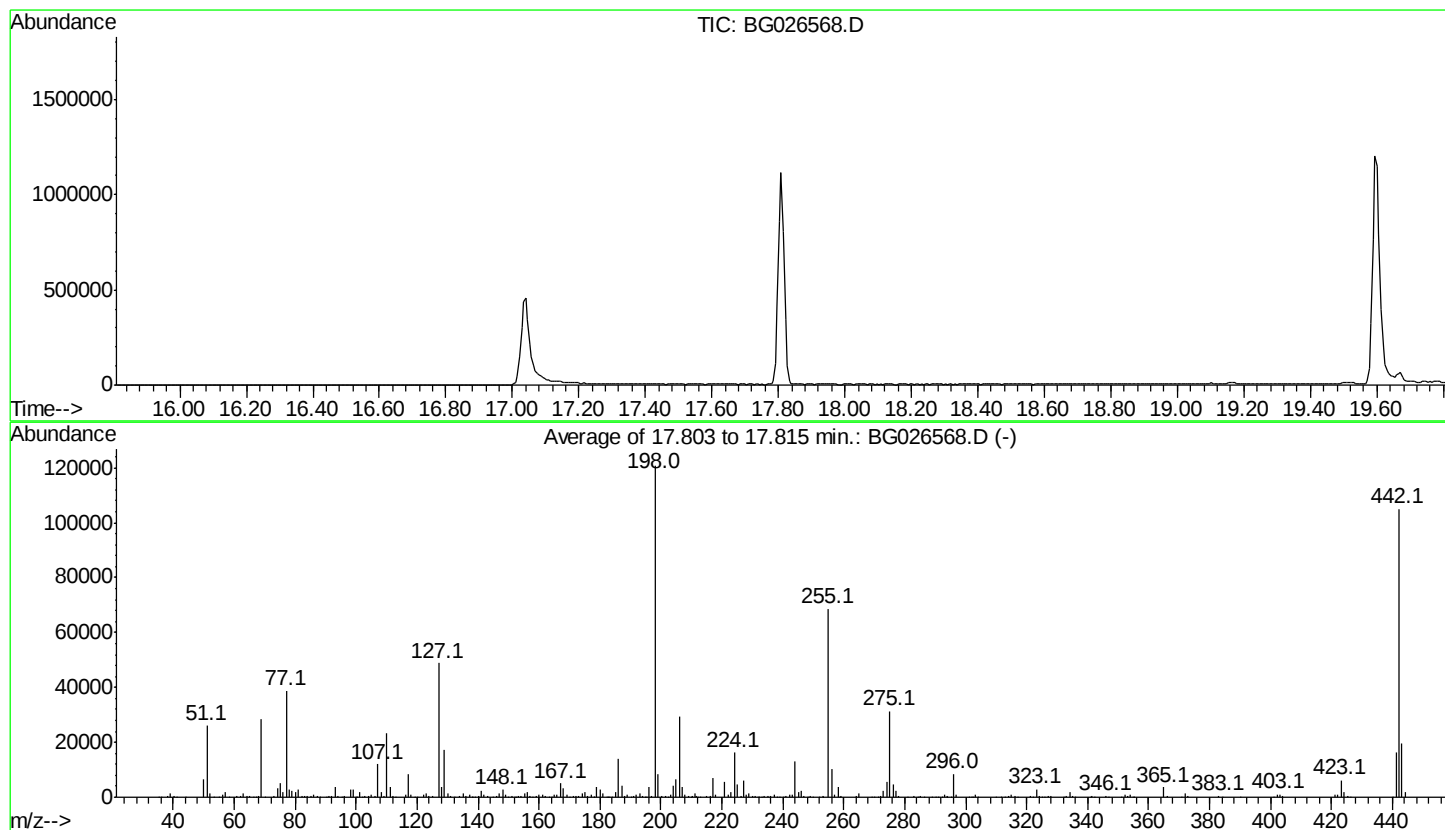

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	25906	PASS
68	69	0.00	2	1.2	338	PASS
69	198	0.00	100	23.7	28658	PASS
70	69	0.00	2	0.5	141	PASS
127	198	10	80	40.4	48864	PASS
197	198	0.00	2	0.3	354	PASS
198	198	100	100	100.0	120802	PASS
199	198	5	9	6.9	8391	PASS
275	198	10	60	25.9	31304	PASS
365	198	1	100	3.0	3573	PASS
441	442	0.01	24	15.5	16268	PASS
442	198	50	100	87.1	105160	PASS
443	442	15	24	18.6	19607	PASS