


Data Path : Z:\HPCHEM1\BNA G\DATA\BG040617\
 Data File : BG026585.D
 Acq On : 7 Apr 2017 3:38
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 20 17:43:27 2017

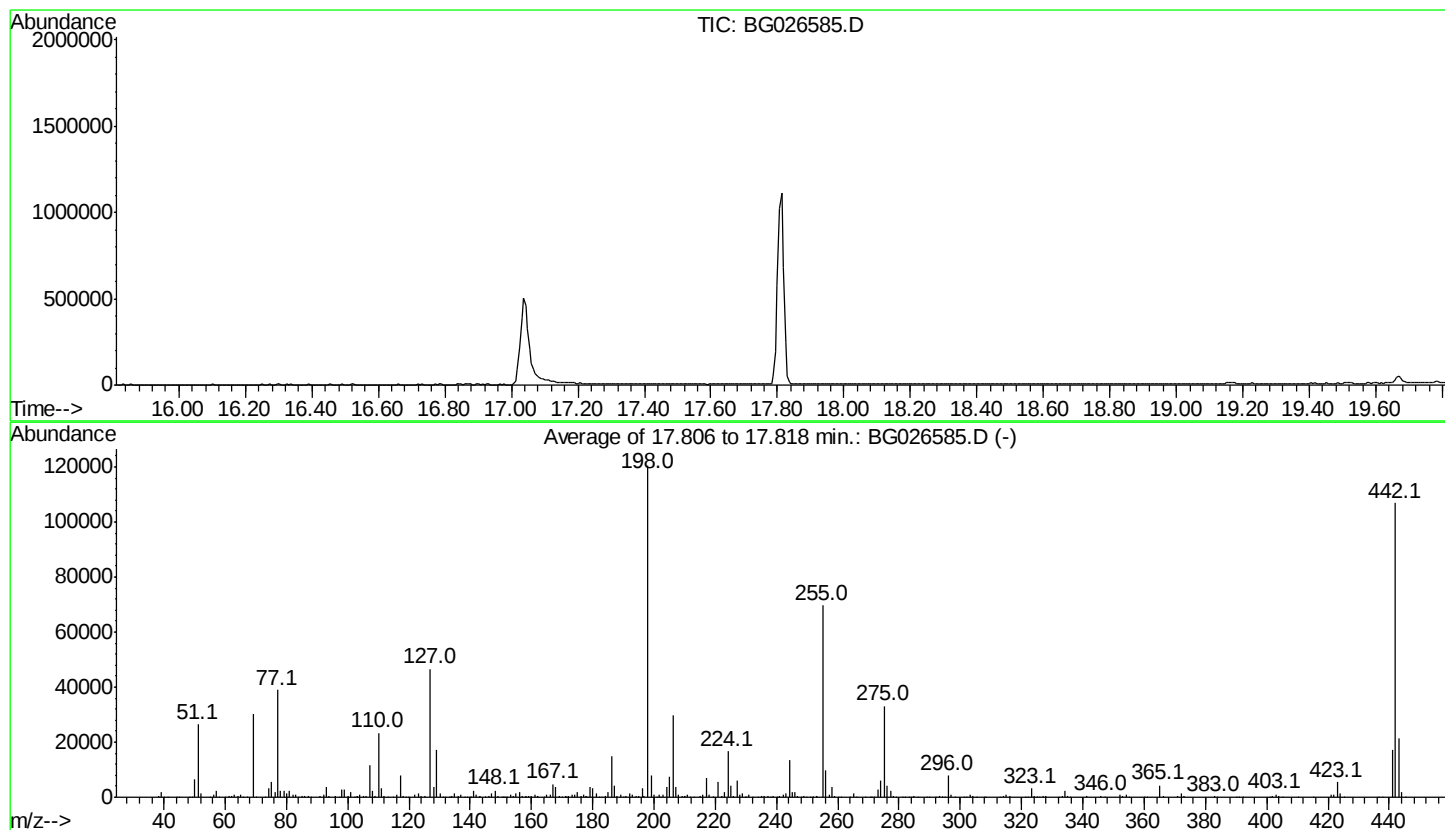

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.0	26502	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.0	30122	PASS
70	69	0.00	2	0.5	163	PASS
127	198	10	80	38.8	46733	PASS
197	198	0.00	2	0.2	280	PASS
198	198	100	100	100.0	120442	PASS
199	198	5	9	6.4	7748	PASS
275	198	10	60	27.4	33042	PASS
365	198	1	100	3.5	4270	PASS
441	442	0.01	24	16.0	17053	PASS
442	198	50	100	88.7	106837	PASS
443	442	15	24	19.9	21216	PASS